

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035328.D
 Acq On : 22 Apr 2024 13:20
 Operator : SY/MD
 Sample : P2182-09 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035328.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	90	rVB	93826	100594	9.51%	1.452%
2	1.532	148	153	171	rVB	121830	147770	13.97%	2.133%
3	2.060	309	317	332	rVB	122907	178350	16.86%	2.574%
4	2.683	507	511	515	rBV3	534	541	0.05%	0.008%
5	2.722	521	523	525	rBV2	402	194	0.02%	0.003%
6	2.754	530	533	536	rVB3	334	234	0.02%	0.003%
7	2.780	536	541	551	rBV3	395	747	0.07%	0.011%
8	2.818	551	553	556	rVB3	228	141	0.01%	0.002%
9	2.841	556	560	563	rBV2	201	194	0.02%	0.003%
10	3.018	612	615	619	rVB3	261	180	0.02%	0.003%
11	3.191	665	669	670	rBV	227	174	0.02%	0.003%
12	3.307	703	705	711	rVB2	386	284	0.03%	0.004%
13	3.333	711	713	716	rVB2	198	129	0.01%	0.002%
14	3.365	720	723	726	rBV3	301	222	0.02%	0.003%
15	3.477	755	758	763	rBV3	260	316	0.03%	0.005%
16	3.580	785	790	793	rBV2	244	228	0.02%	0.003%
17	3.706	826	829	834	rVB2	167	125	0.01%	0.002%
18	3.748	839	842	845	rVB2	496	306	0.03%	0.004%
19	3.815	845	863	884	rBV2	14065	49373	4.67%	0.713%
20	4.175	973	975	979	rBV2	321	180	0.02%	0.003%
21	4.249	983	998	1022	rBV	177523	460013	43.50%	6.640%
22	4.641	1117	1120	1122	rBV2	255	167	0.02%	0.002%
23	4.661	1124	1126	1128	rVV2	305	134	0.01%	0.002%
24	4.751	1151	1154	1157	rBV	295	178	0.02%	0.003%
25	4.828	1175	1178	1180	rVV2	437	257	0.02%	0.004%
26	4.857	1183	1187	1192	rVB2	238	238	0.02%	0.003%
27	4.953	1202	1217	1234	rBV2	372696	1057544	100.00%	15.264%
28	5.439	1365	1368	1371	rBV2	327	229	0.02%	0.003%
29	5.535	1386	1398	1427	rBV	209102	453644	42.90%	6.548%
30	5.834	1481	1491	1509	rBV7	6532	16182	1.53%	0.234%
31	5.989	1526	1539	1580	rBV	254560	547085	51.73%	7.896%
32	6.233	1613	1615	1620	rVB2	637	344	0.03%	0.005%
33	6.272	1625	1627	1631	rBV3	487	388	0.04%	0.006%
34	6.294	1631	1634	1636	rVB	459	262	0.02%	0.004%
35	6.317	1639	1641	1645	rBV3	333	206	0.02%	0.003%
36	6.339	1645	1648	1650	rBV2	337	199	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035328.D
 Acq On : 22 Apr 2024 13:20
 Operator : SY/MD
 Sample : P2182-09 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.413	1667	1671	1672	rBV2	200	157	0.01%	0.002%
38	6.468	1683	1688	1691	rBV2	120	135	0.01%	0.002%
39	6.532	1701	1708	1710	rBV2	329	318	0.03%	0.005%
40	6.587	1721	1725	1728	rBV	183	144	0.01%	0.002%
41	6.609	1728	1732	1733	rBV	200	128	0.01%	0.002%
42	6.712	1761	1764	1766	rVB3	439	246	0.02%	0.004%
43	6.728	1766	1769	1773	rBV2	343	237	0.02%	0.003%
44	6.744	1773	1774	1777	rVB	376	169	0.02%	0.002%
45	6.764	1777	1780	1781	rBV	317	186	0.02%	0.003%
46	6.802	1790	1792	1795	rVB	321	141	0.01%	0.002%
47	6.837	1799	1803	1806	rVB2	258	194	0.02%	0.003%
48	6.915	1817	1827	1852	rBV	88405	180471	17.07%	2.605%
49	7.246	1919	1930	1956	rBV	246713	452546	42.79%	6.532%
50	7.558	2018	2027	2054	rBV	63803	127430	12.05%	1.839%
51	7.744	2082	2085	2091	rBV3	567	718	0.07%	0.010%
52	7.834	2109	2113	2117	rBV3	429	404	0.04%	0.006%
53	7.953	2147	2150	2156	rVB2	522	327	0.03%	0.005%
54	8.030	2166	2174	2213	rBV2	126784	336251	31.80%	4.853%
55	8.452	2303	2305	2311	rVB4	481	431	0.04%	0.006%
56	8.625	2353	2359	2364	rBV4	522	564	0.05%	0.008%
57	8.661	2364	2370	2373	rVB2	645	614	0.06%	0.009%
58	8.693	2373	2380	2383	rBV3	475	570	0.05%	0.008%
59	8.712	2383	2386	2390	rBV2	273	205	0.02%	0.003%
60	8.738	2390	2394	2397	rBV	314	232	0.02%	0.003%
61	8.786	2398	2409	2413	rBV	306122	470102	44.45%	6.785%
62	9.075	2496	2499	2504	rBV3	502	372	0.04%	0.005%
63	9.114	2509	2511	2516	rBV2	367	285	0.03%	0.004%
64	9.194	2532	2536	2539	rBV3	515	409	0.04%	0.006%
65	9.316	2572	2574	2576	rBV3	310	122	0.01%	0.002%
66	9.358	2583	2587	2588	rBV2	236	137	0.01%	0.002%
67	9.371	2588	2591	2592	rVV	302	171	0.02%	0.002%
68	9.381	2592	2594	2597	rVV2	367	165	0.02%	0.002%
69	9.400	2597	2600	2607	rVV3	396	398	0.04%	0.006%
70	9.477	2622	2624	2627	rBV3	460	214	0.02%	0.003%
71	9.558	2645	2649	2654	rVB2	391	335	0.03%	0.005%
72	9.616	2664	2667	2668	rBV	256	135	0.01%	0.002%
73	9.670	2677	2684	2687	rBV2	562	617	0.06%	0.009%
74	9.744	2704	2707	2708	rBV2	293	189	0.02%	0.003%
75	9.792	2721	2722	2727	rVB2	341	189	0.02%	0.003%
76	9.834	2732	2735	2736	rBV2	286	139	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035328.D
 Acq On : 22 Apr 2024 13:20
 Operator : SY/MD
 Sample : P2182-09 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.857	2739	2742	2744	rBV2	225	141	0.01%	0.002%
78	10.149	2822	2833	2863	rVV	475163	751563	71.07%	10.848%
79	10.484	2936	2937	2940	rBV	247	148	0.01%	0.002%
80	10.564	2959	2962	2964	rBV	240	191	0.02%	0.003%
81	10.609	2974	2976	2979	rVB2	419	218	0.02%	0.003%
82	10.657	2987	2991	2995	rBV2	180	181	0.02%	0.003%
83	10.767	3022	3025	3027	rVV2	294	155	0.01%	0.002%
84	10.866	3053	3056	3059	rBV	321	296	0.03%	0.004%
85	10.905	3065	3068	3069	rBV	294	182	0.02%	0.003%
86	10.998	3093	3097	3100	rVB2	254	227	0.02%	0.003%
87	11.017	3100	3103	3106	rBV2	427	289	0.03%	0.004%
88	11.053	3111	3114	3117	rBV2	354	239	0.02%	0.003%
89	11.088	3120	3125	3128	rBV2	443	391	0.04%	0.006%
90	11.127	3128	3137	3145	rBV2	11043	17388	1.64%	0.251%
91	11.185	3145	3155	3188	rVV2	245576	624329	59.04%	9.011%
92	11.561	3260	3272	3297	rBV3	323974	712504	67.37%	10.284%
93	11.956	3392	3395	3397	rBV	346	242	0.02%	0.003%
94	12.136	3448	3451	3454	rBV2	282	223	0.02%	0.003%
95	12.210	3472	3474	3480	rBV2	558	451	0.04%	0.007%
96	12.593	3587	3593	3601	rVB6	1102	1857	0.18%	0.027%
97	13.197	3771	3781	3805	rBV2	100931	164558	15.56%	2.375%
98	13.448	3854	3859	3869	rVB2	4284	6220	0.59%	0.090%
99	13.512	3877	3879	3882	rBV2	474	237	0.02%	0.003%
100	13.680	3922	3931	3949	rBV2	31669	51989	4.92%	0.750%




Sum of corrected areas: 6928368

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035328.D
Acq On : 22 Apr 2024 13:20
Operator : SY/MD
Sample : P2182-09 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

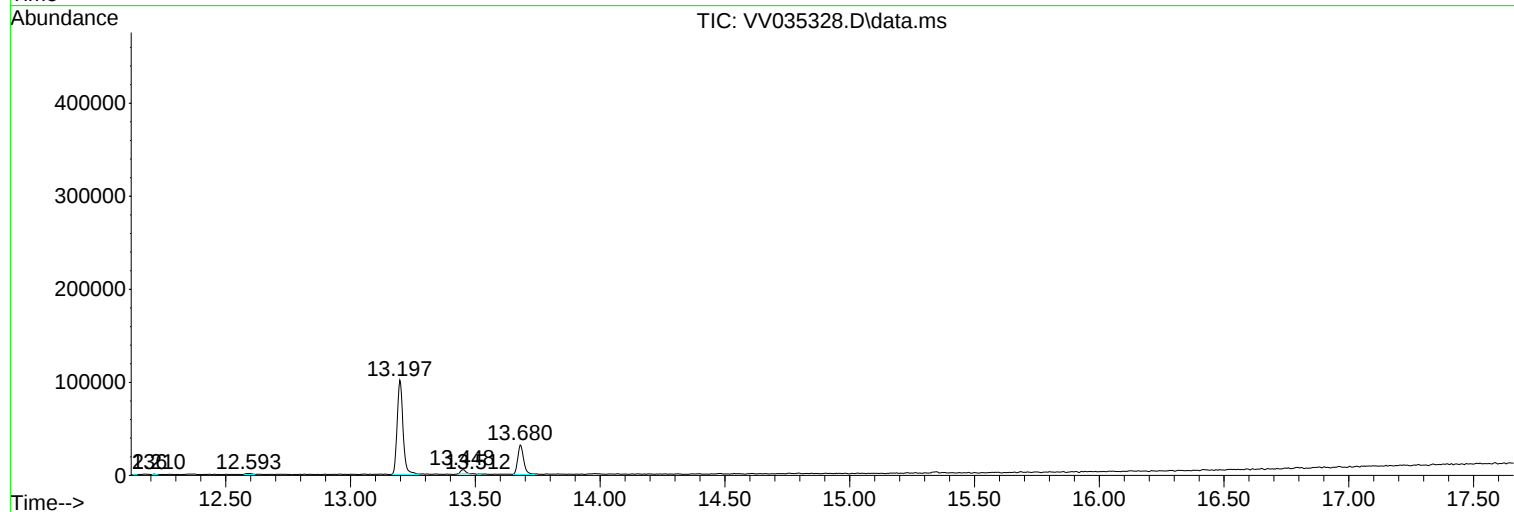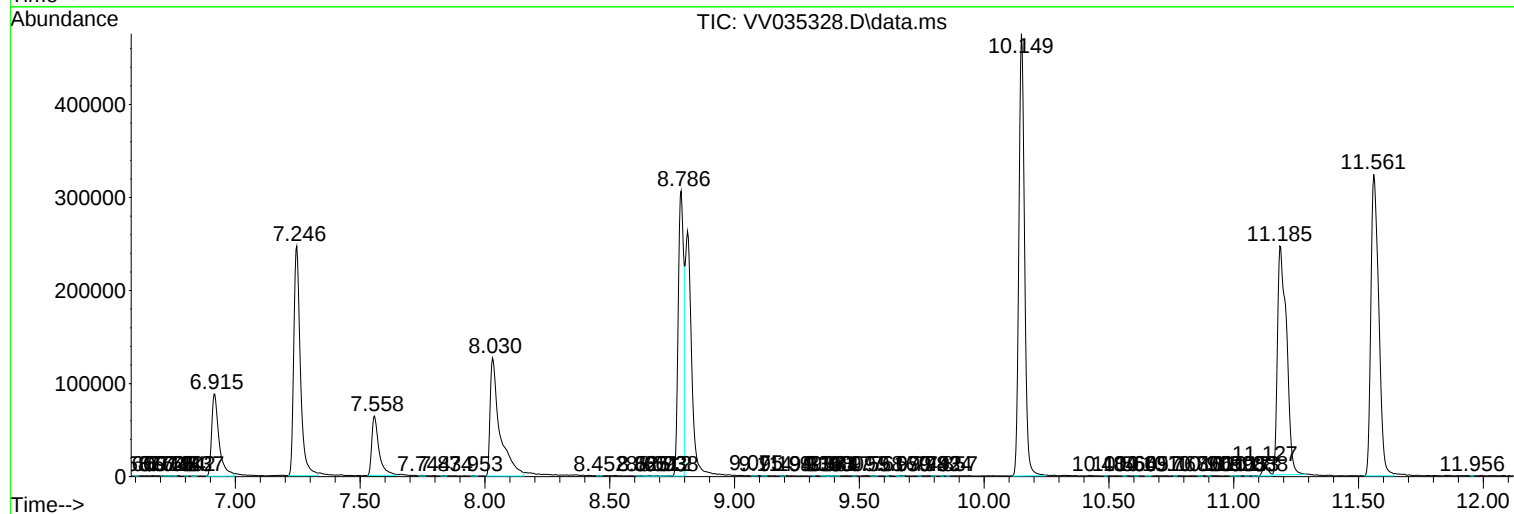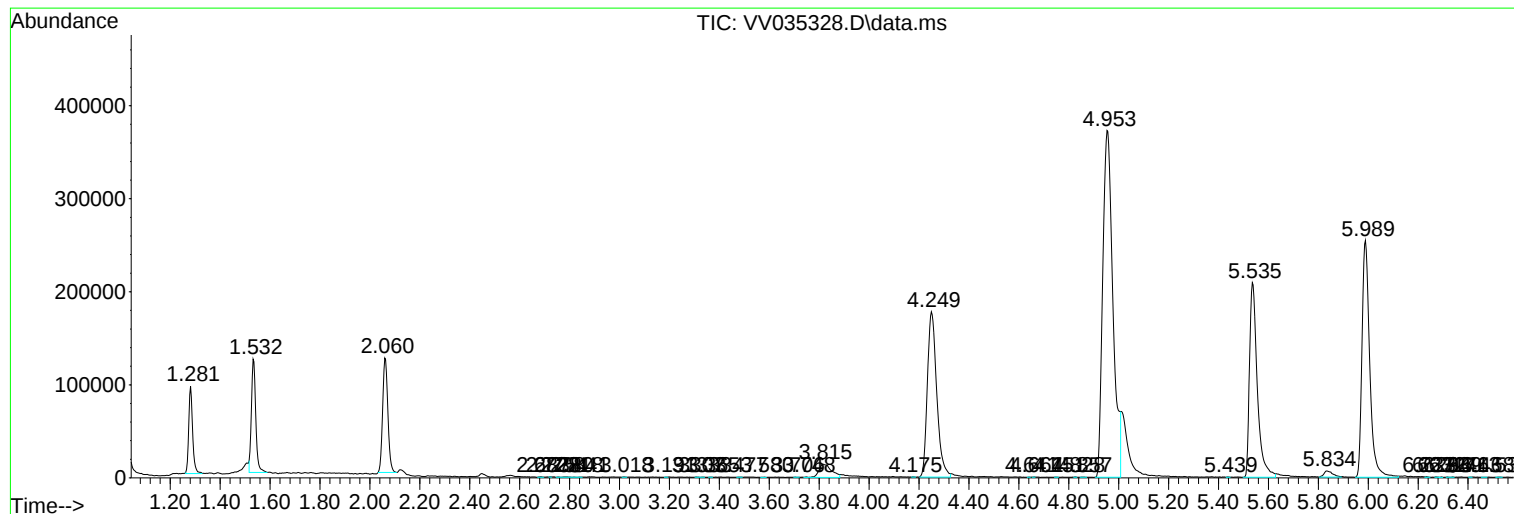

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035328.D
Acq On : 22 Apr 2024 13:20
Operator : SY/MD
Sample : P2182-09 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035328.D
Acq On : 22 Apr 2024 13:20
Operator : SY/MD
Sample : P2182-09 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------