

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035329.D
 Acq On : 22 Apr 2024 13:43
 Operator : SY/MD
 Sample : P2182-08 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035329.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	76407	80725	8.68%	1.466%
2	1.532	147	153	168	rVB	107625	127900	13.75%	2.323%
3	2.060	309	317	329	rBV	101418	145515	15.64%	2.642%
4	2.507	454	456	458	rBV2	405	182	0.02%	0.003%
5	2.642	495	498	500	rBV2	526	245	0.03%	0.004%
6	2.825	553	555	556	rVB	353	105	0.01%	0.002%
7	2.896	572	577	586	rBV3	533	715	0.08%	0.013%
8	2.931	586	588	589	rBV2	169	81	0.01%	0.001%
9	2.963	595	598	599	rBV	152	81	0.01%	0.001%
10	3.015	611	614	617	rBV2	232	168	0.02%	0.003%
11	3.146	654	655	656	rBV2	105	27	0.00%	0.000%
12	3.291	697	700	701	rBV2	228	114	0.01%	0.002%
13	3.333	712	713	717	rVB2	278	135	0.01%	0.002%
14	3.352	717	719	722	rBV	148	85	0.01%	0.002%
15	3.436	743	745	749	rBV3	228	178	0.02%	0.003%
16	3.532	773	775	779	rBV2	246	163	0.02%	0.003%
17	3.587	789	792	794	rVV2	182	83	0.01%	0.002%
18	3.600	794	796	802	rVB	292	204	0.02%	0.004%
19	3.667	813	817	818	rBV	227	162	0.02%	0.003%
20	3.677	818	820	822	rVV	291	123	0.01%	0.002%
21	3.712	830	831	833	rBV	113	43	0.00%	0.001%
22	3.815	849	863	878	rBV2	13454	42443	4.56%	0.771%
23	4.249	982	998	1028	rBV	160413	417438	44.87%	7.580%
24	4.642	1118	1120	1121	rBV	234	75	0.01%	0.001%
25	4.767	1157	1159	1160	rBV	137	64	0.01%	0.001%
26	4.812	1168	1173	1175	rBV2	299	186	0.02%	0.003%
27	4.844	1180	1183	1188	rVV2	305	268	0.03%	0.005%
28	4.953	1201	1217	1253	rBV2	326363	930399	100.00%	16.895%
29	5.275	1315	1317	1319	rBV	260	153	0.02%	0.003%
30	5.384	1349	1351	1353	rBV	257	120	0.01%	0.002%
31	5.433	1363	1366	1367	rBV	190	103	0.01%	0.002%
32	5.535	1388	1398	1424	rBV	172205	369239	39.69%	6.705%
33	5.838	1482	1492	1504	rBV6	6450	14656	1.58%	0.266%
34	5.934	1520	1522	1523	rBV6	250	77	0.01%	0.001%
35	5.989	1527	1539	1571	rVV	231907	490211	52.69%	8.902%
36	6.256	1619	1622	1626	rBV3	549	545	0.06%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035329.D
 Acq On : 22 Apr 2024 13:43
 Operator : SY/MD
 Sample : P2182-08 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.330	1644	1645	1649	rVB	286	129	0.01%	0.002%
38	6.352	1649	1652	1653	rBV	140	83	0.01%	0.002%
39	6.365	1653	1656	1657	rBV	266	150	0.02%	0.003%
40	6.375	1657	1659	1662	rVV2	266	121	0.01%	0.002%
41	6.410	1668	1670	1673	rBV	182	69	0.01%	0.001%
42	6.561	1713	1717	1719	rBV	147	119	0.01%	0.002%
43	6.574	1719	1721	1722	rBV	236	88	0.01%	0.002%
44	6.625	1733	1737	1738	rBV	386	225	0.02%	0.004%
45	6.757	1771	1778	1783	rBV5	636	734	0.08%	0.013%
46	6.793	1786	1789	1792	rBV	229	182	0.02%	0.003%
47	6.844	1802	1805	1809	rVB2	157	102	0.01%	0.002%
48	6.863	1809	1811	1814	rBV	160	115	0.01%	0.002%
49	6.915	1817	1827	1854	rBV	76739	160443	17.24%	2.913%
50	7.149	1897	1900	1902	rBV2	206	144	0.02%	0.003%
51	7.246	1919	1930	1952	rBV	196898	366243	39.36%	6.651%
52	7.558	2018	2027	2050	rBV2	57698	113998	12.25%	2.070%
53	7.850	2116	2118	2120	rBV2	400	199	0.02%	0.004%
54	7.886	2127	2129	2132	rBV	184	89	0.01%	0.002%
55	7.902	2132	2134	2136	rBV	125	64	0.01%	0.001%
56	7.985	2158	2160	2162	rBV2	255	129	0.01%	0.002%
57	8.030	2165	2174	2214	rBV3	131687	349447	37.56%	6.346%
58	8.535	2329	2331	2334	rBV2	351	184	0.02%	0.003%
59	8.584	2343	2346	2349	rBV3	461	344	0.04%	0.006%
60	8.786	2398	2409	2441	rBV	233084	431271	46.35%	7.831%
61	9.088	2502	2503	2504	rBV	430	137	0.01%	0.002%
62	9.137	2515	2518	2523	rBV3	428	280	0.03%	0.005%
63	9.439	2610	2612	2617	rVB	354	207	0.02%	0.004%
64	9.465	2617	2620	2625	rBV2	274	163	0.02%	0.003%
65	9.490	2625	2628	2632	rBV4	263	171	0.02%	0.003%
66	9.516	2633	2636	2640	rBV2	552	349	0.04%	0.006%
67	9.625	2668	2670	2675	rBV2	235	148	0.02%	0.003%
68	9.661	2679	2681	2687	rVB2	236	133	0.01%	0.002%
69	9.850	2736	2740	2743	rBV2	298	281	0.03%	0.005%
70	9.886	2747	2751	2754	rBV2	362	301	0.03%	0.005%
71	9.953	2768	2772	2776	rBV2	418	432	0.05%	0.008%
72	10.149	2821	2833	2860	rBV	445916	709492	76.26%	12.883%
73	10.352	2894	2896	2900	rBV2	354	291	0.03%	0.005%
74	10.423	2915	2918	2920	rBV	324	179	0.02%	0.003%
75	10.606	2973	2975	2976	rBV	211	80	0.01%	0.001%
76	10.866	3054	3056	3058	rBV	306	145	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035329.D
Acq On : 22 Apr 2024 13:43
Operator : SY/MD
Sample : P2182-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

77	11.104	3127	3130	3131	rBV	259	158	0.02%	0.003%
78	11.133	3134	3139	3144	rVV5	1558	1962	0.21%	0.036%
79	11.185	3146	3155	3183	rVV	173357	311967	33.53%	5.665%
80	11.561	3260	3272	3296	rBV	229446	403218	43.34%	7.322%
81	12.596	3591	3594	3602	rVB3	1035	1020	0.11%	0.019%
82	13.204	3773	3783	3798	rBV3	13244	23069	2.48%	0.419%
83	13.323	3818	3820	3825	rBV2	408	358	0.04%	0.007%
84	13.455	3854	3861	3870	rBV4	3223	4768	0.51%	0.087%




Sum of corrected areas: 5506992

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035329.D
Acq On : 22 Apr 2024 13:43
Operator : SY/MD
Sample : P2182-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

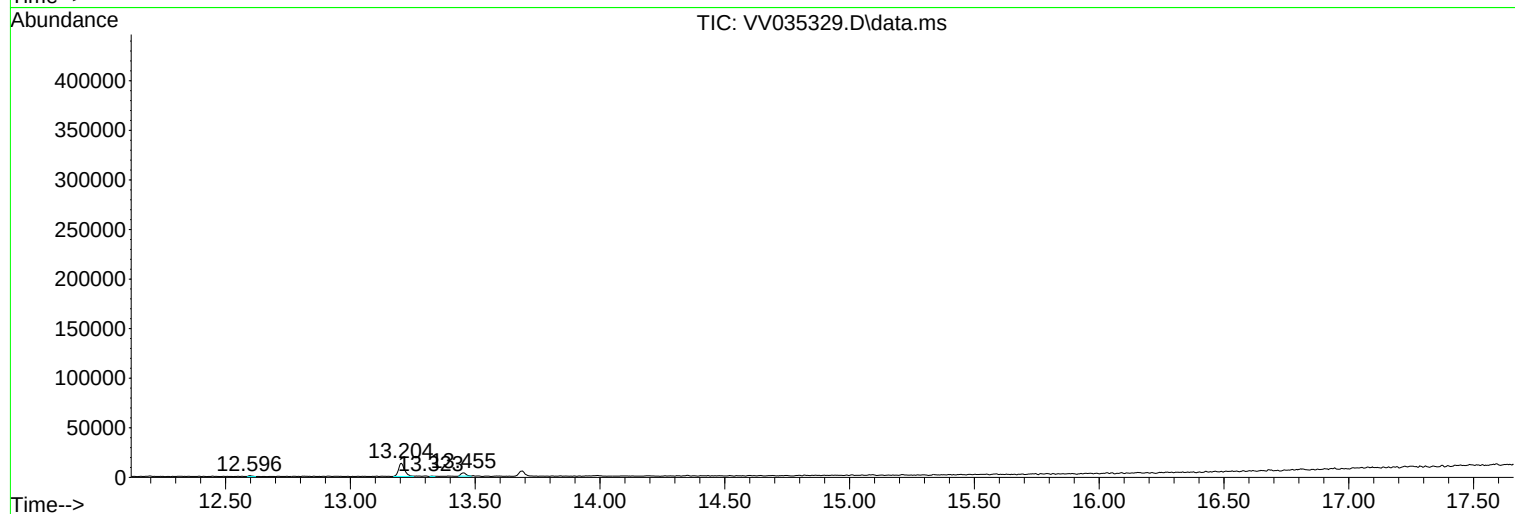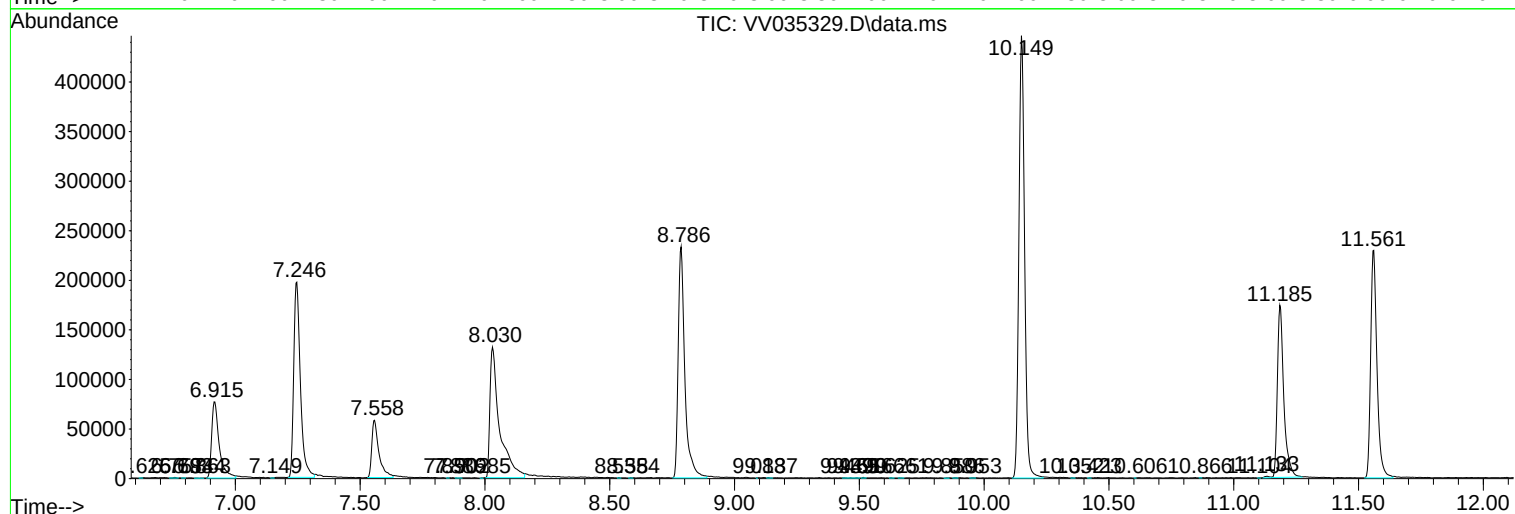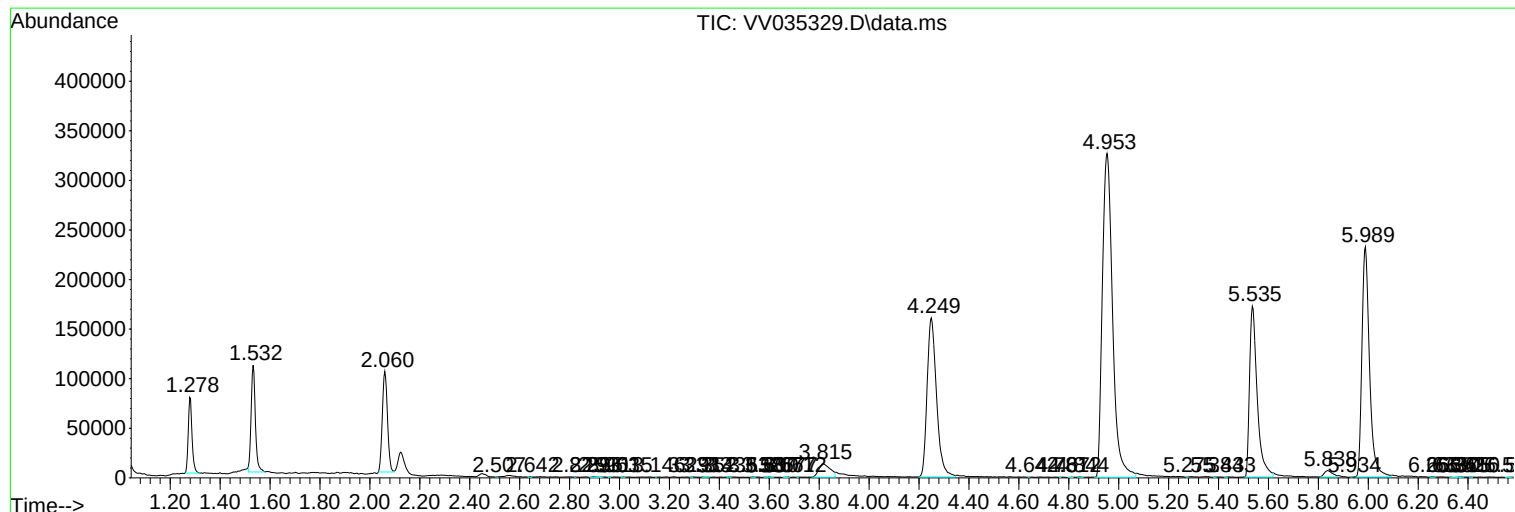

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035329.D
Acq On : 22 Apr 2024 13:43
Operator : SY/MD
Sample : P2182-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035329.D
Acq On : 22 Apr 2024 13:43
Operator : SY/MD
Sample : P2182-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------