

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035330.D
 Acq On : 22 Apr 2024 14:06
 Operator : SY/MD
 Sample : P2182-07 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035330.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rBV	76506	81788	8.89%	1.490%
2	1.532	147	153	168	rVB	108575	127060	13.81%	2.315%
3	2.060	309	317	329	rBV	101951	145209	15.78%	2.646%
4	2.410	422	426	431	rBV2	403	320	0.03%	0.006%
5	2.446	431	437	447	rBV5	3240	5302	0.58%	0.097%
6	2.671	505	507	511	rVB2	376	201	0.02%	0.004%
7	2.706	515	518	519	rBV2	384	190	0.02%	0.003%
8	2.757	531	534	539	rVB	453	246	0.03%	0.004%
9	2.938	587	590	593	rVB2	359	241	0.03%	0.004%
10	2.966	597	599	605	rVB3	317	172	0.02%	0.003%
11	3.002	608	610	611	rBV3	265	97	0.01%	0.002%
12	3.076	631	633	635	rBV3	137	63	0.01%	0.001%
13	3.124	645	648	650	rBV	266	155	0.02%	0.003%
14	3.163	658	660	667	rVB2	408	336	0.04%	0.006%
15	3.204	671	673	677	rVB2	217	86	0.01%	0.002%
16	3.227	677	680	682	rBV2	259	153	0.02%	0.003%
17	3.243	682	685	686	rBV	244	146	0.02%	0.003%
18	3.294	698	701	703	rBV	103	60	0.01%	0.001%
19	3.330	709	712	713	rBV	120	61	0.01%	0.001%
20	3.343	713	716	719	rVB3	286	147	0.02%	0.003%
21	3.378	725	727	729	rBV2	114	65	0.01%	0.001%
22	3.452	748	750	751	rBV2	182	65	0.01%	0.001%
23	3.500	763	765	770	rVB2	338	193	0.02%	0.004%
24	3.526	770	773	778	rVB	280	223	0.02%	0.004%
25	3.548	778	780	783	rVB	130	70	0.01%	0.001%
26	3.571	783	787	791	rBV3	290	215	0.02%	0.004%
27	3.603	795	797	801	rBV2	159	122	0.01%	0.002%
28	3.658	812	814	817	rVB	240	107	0.01%	0.002%
29	3.677	817	820	824	rBV2	267	190	0.02%	0.003%
30	3.722	832	834	836	rBV	114	49	0.01%	0.001%
31	3.815	846	863	890	rBV3	15991	65261	7.09%	1.189%
32	4.249	983	998	1034	rBV	158761	412320	44.81%	7.513%
33	4.494	1072	1074	1076	rBV2	498	250	0.03%	0.005%
34	4.574	1095	1099	1100	rBV	226	167	0.02%	0.003%
35	4.667	1126	1128	1130	rBV2	168	85	0.01%	0.002%
36	4.764	1155	1158	1162	rBV2	189	156	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035330.D
 Acq On : 22 Apr 2024 14:06
 Operator : SY/MD
 Sample : P2182-07 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	4.806	1169	1171	1173	rBV	233	72	0.01%	0.001%
38	4.838	1177	1181	1183	rBV2	252	197	0.02%	0.004%
39	4.902	1198	1201	1202	rBV	204	123	0.01%	0.002%
40	4.954	1202	1217	1256	rBV2	326592	920254	100.00%	16.768%
41	5.436	1365	1367	1371	rBV	395	279	0.03%	0.005%
42	5.535	1386	1398	1428	rBV	171250	371736	40.39%	6.774%
43	5.989	1527	1539	1570	rBV	232436	489321	53.17%	8.916%
44	6.346	1649	1650	1654	rVB	264	102	0.01%	0.002%
45	6.371	1654	1658	1660	rBV2	269	197	0.02%	0.004%
46	6.426	1671	1675	1677	rBV2	214	185	0.02%	0.003%
47	6.462	1685	1686	1688	rVB	280	97	0.01%	0.002%
48	6.474	1688	1690	1693	rBV	148	125	0.01%	0.002%
49	6.497	1695	1697	1700	rBV	139	113	0.01%	0.002%
50	6.606	1729	1731	1734	rBV2	480	297	0.03%	0.005%
51	6.664	1747	1749	1751	rBV	322	144	0.02%	0.003%
52	6.828	1798	1800	1802	rBV	264	142	0.02%	0.003%
53	6.915	1817	1827	1861	rBV	74850	158197	17.19%	2.883%
54	7.101	1883	1885	1889	rVB2	497	278	0.03%	0.005%
55	7.246	1919	1930	1959	rBV	193072	364182	39.57%	6.636%
56	7.516	2012	2014	2017	rBV	375	166	0.02%	0.003%
57	7.558	2017	2027	2055	rBV2	55666	114042	12.39%	2.078%
58	7.838	2113	2114	2120	rVB2	374	287	0.03%	0.005%
59	7.886	2128	2129	2133	rBV2	311	207	0.02%	0.004%
60	7.931	2141	2143	2144	rBV	229	100	0.01%	0.002%
61	7.941	2144	2146	2148	rBV2	290	105	0.01%	0.002%
62	7.976	2152	2157	2159	rBV	299	243	0.03%	0.004%
63	7.992	2160	2162	2165	rBV2	229	142	0.02%	0.003%
64	8.031	2165	2174	2213	rBV2	155070	403587	43.86%	7.354%
65	8.551	2334	2336	2337	rBV2	251	86	0.01%	0.002%
66	8.703	2381	2383	2384	rBV2	143	45	0.00%	0.001%
67	8.786	2395	2409	2442	rBV	230445	420471	45.69%	7.662%
68	9.111	2508	2510	2514	rVB	329	209	0.02%	0.004%
69	9.140	2518	2519	2524	rVB	305	167	0.02%	0.003%
70	9.175	2528	2530	2532	rBV	304	124	0.01%	0.002%
71	9.336	2575	2580	2585	rBV2	281	301	0.03%	0.005%
72	9.432	2607	2610	2614	rBV	307	233	0.03%	0.004%
73	9.497	2629	2630	2635	rBV	267	158	0.02%	0.003%
74	9.526	2637	2639	2641	rVB2	290	106	0.01%	0.002%
75	9.542	2641	2644	2646	rBV	335	163	0.02%	0.003%
76	9.667	2681	2683	2685	rBV2	226	105	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035330.D
 Acq On : 22 Apr 2024 14:06
 Operator : SY/MD
 Sample : P2182-07 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RC9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.699	2690	2693	2697	rBV2	374	288	0.03%	0.005%
78	9.757	2709	2711	2713	rVB	164	66	0.01%	0.001%
79	9.770	2713	2715	2716	rBV	189	84	0.01%	0.002%
80	10.098	2814	2817	2819	rBV	240	152	0.02%	0.003%
81	10.149	2822	2833	2861	rVV	448866	702519	76.34%	12.801%
82	10.593	2968	2971	2973	rBV	240	139	0.02%	0.003%
83	10.735	3013	3015	3016	rBV	210	61	0.01%	0.001%
84	11.133	3133	3139	3145	rBV5	1324	1974	0.21%	0.036%
85	11.185	3145	3155	3185	rVV	171854	299272	32.52%	5.453%
86	11.413	3222	3226	3229	rBV2	359	344	0.04%	0.006%
87	11.558	3260	3271	3296	rBV	219926	380279	41.32%	6.929%
88	11.924	3383	3385	3387	rBV	250	129	0.01%	0.002%
89	12.043	3420	3422	3426	rBV3	362	266	0.03%	0.005%
90	13.140	3759	3763	3764	rBV	612	375	0.04%	0.007%
91	13.207	3776	3784	3796	rBV4	5862	9696	1.05%	0.177%
92	13.455	3854	3861	3869	rBV5	2535	3743	0.41%	0.068%




Sum of corrected areas: 5488046

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035330.D
Acq On : 22 Apr 2024 14:06
Operator : SY/MD
Sample : P2182-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

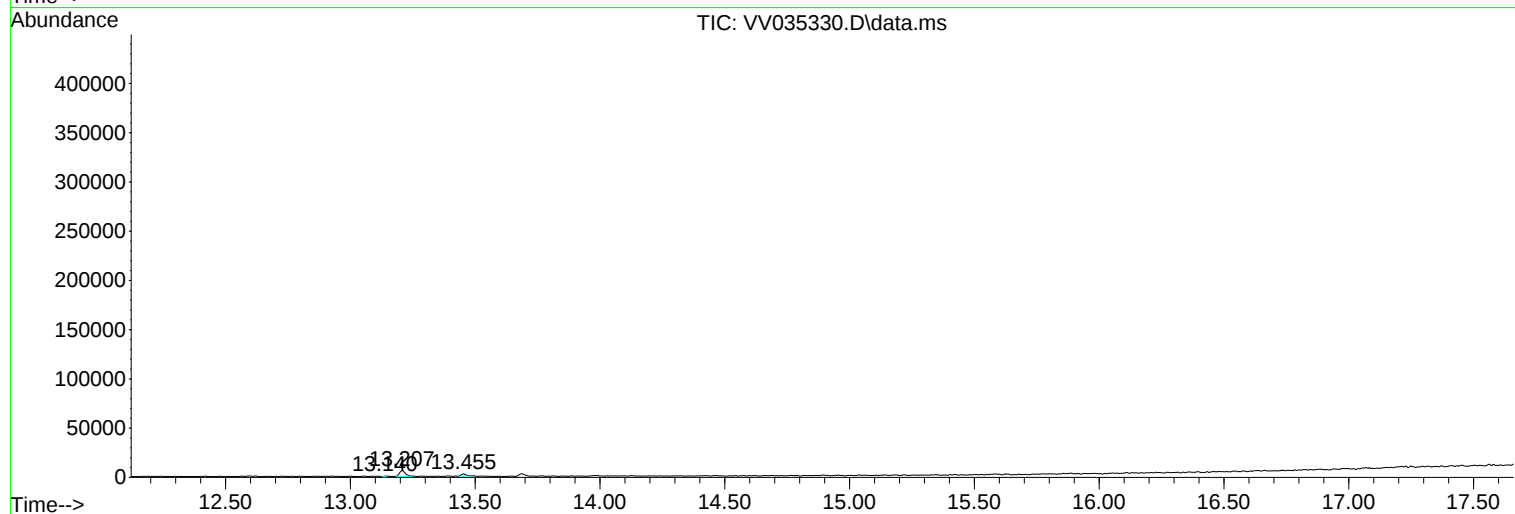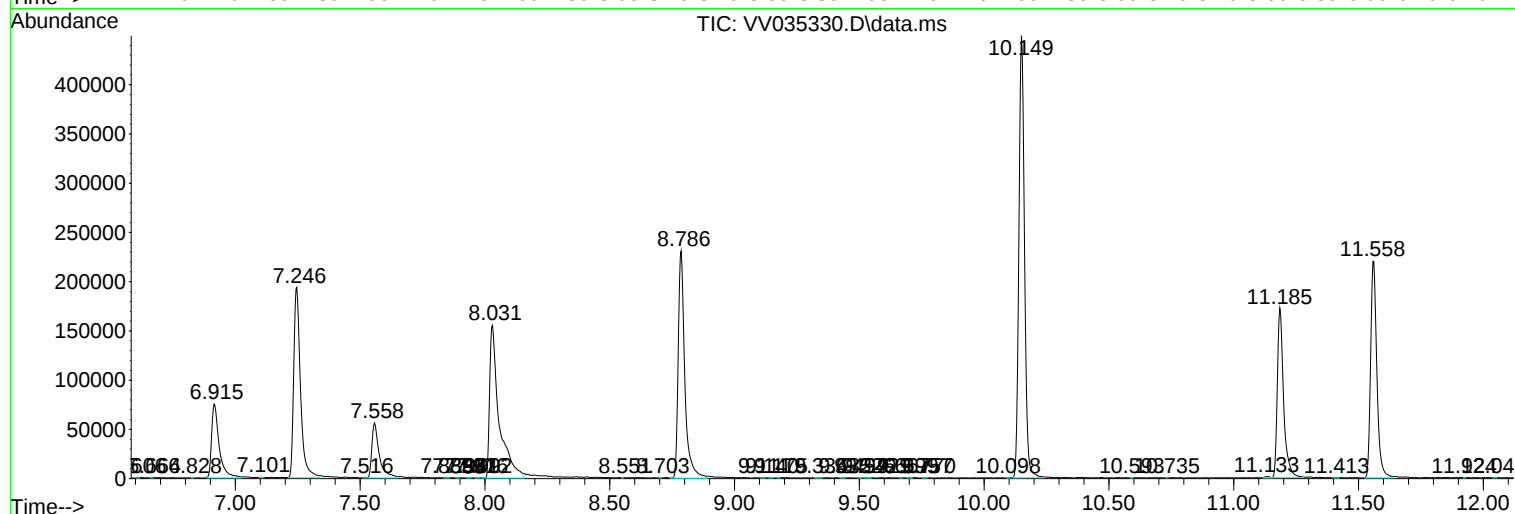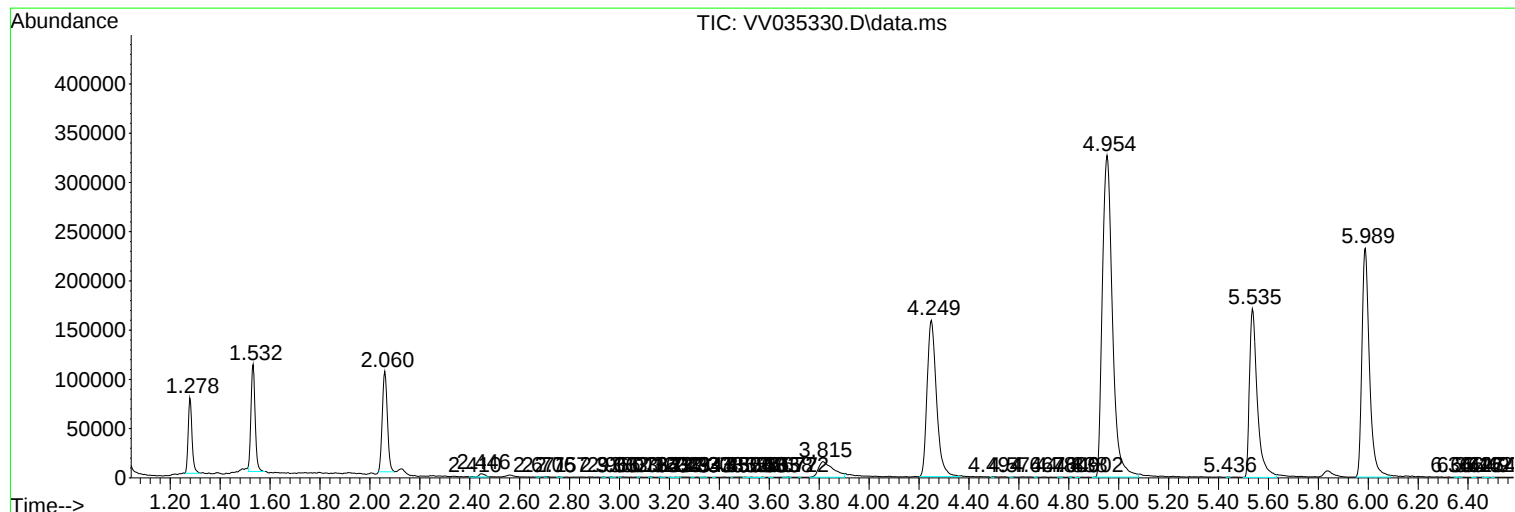

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035330.D
Acq On : 22 Apr 2024 14:06
Operator : SY/MD
Sample : P2182-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035330.D
Acq On : 22 Apr 2024 14:06
Operator : SY/MD
Sample : P2182-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RC9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------