

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035331.D
 Acq On : 22 Apr 2024 14:29
 Operator : SY/MD
 Sample : P2182-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R94

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035331.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	77387	83749	5.69%	1.177%
2	1.532	147	153	165	rVB	107783	125536	8.54%	1.765%
3	2.059	309	317	328	rBV	100969	141031	9.59%	1.983%
4	2.449	431	438	451	rVB5	3974	6554	0.45%	0.092%
5	2.703	515	517	520	rBV	378	216	0.01%	0.003%
6	2.744	527	530	534	rBV2	269	208	0.01%	0.003%
7	2.764	534	536	541	rVB3	292	193	0.01%	0.003%
8	2.793	541	545	550	rBV3	341	361	0.02%	0.005%
9	2.818	550	553	559	rBV3	333	357	0.02%	0.005%
10	2.908	578	581	585	rBV2	233	142	0.01%	0.002%
11	2.973	598	601	602	rBV	318	155	0.01%	0.002%
12	3.005	610	611	615	rBV	181	121	0.01%	0.002%
13	3.149	654	656	659	rVB	249	80	0.01%	0.001%
14	3.207	671	674	676	rBV	354	178	0.01%	0.003%
15	3.223	676	679	682	rVB3	205	141	0.01%	0.002%
16	3.252	684	688	691	rBV2	289	281	0.02%	0.004%
17	3.358	716	721	725	rBV3	283	281	0.02%	0.004%
18	3.481	757	759	760	rVB3	151	46	0.00%	0.001%
19	3.510	765	768	770	rVB	113	62	0.00%	0.001%
20	3.545	775	779	781	rBV	210	127	0.01%	0.002%
21	3.558	781	783	786	rBV	185	134	0.01%	0.002%
22	3.667	810	817	819	rBV2	292	307	0.02%	0.004%
23	3.680	819	821	824	rVB2	383	216	0.01%	0.003%
24	3.703	824	828	830	rBV	290	182	0.01%	0.003%
25	3.731	834	837	841	rVB2	277	193	0.01%	0.003%
26	3.764	841	847	848	rBV	412	269	0.02%	0.004%
27	3.818	848	864	888	rBV2	17786	60651	4.12%	0.853%
28	4.249	982	998	1031	rBV2	152667	403797	27.46%	5.677%
29	4.593	1102	1105	1109	rVB3	452	302	0.02%	0.004%
30	4.612	1109	1111	1112	rBV	144	40	0.00%	0.001%
31	4.651	1121	1123	1126	rVB2	499	259	0.02%	0.004%
32	4.686	1131	1134	1137	rVB2	413	283	0.02%	0.004%
33	4.706	1137	1140	1142	rBV2	317	216	0.01%	0.003%
34	4.760	1152	1157	1160	rBV2	278	186	0.01%	0.003%
35	4.776	1160	1162	1165	rBV	216	115	0.01%	0.002%
36	4.857	1185	1187	1190	rBV2	220	109	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035331.D
 Acq On : 22 Apr 2024 14:29
 Operator : SY/MD
 Sample : P2182-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R94

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	4.883	1190	1195	1202	rBV2	257	389	0.03%	0.005%
38	4.953	1202	1217	1226	rBV2	321072	836285	56.86%	11.757%
39	5.461	1373	1375	1376	rBV	308	116	0.01%	0.002%
40	5.535	1388	1398	1436	rBV	170125	370963	25.22%	5.215%
41	5.796	1477	1479	1483	rVB2	463	224	0.02%	0.003%
42	5.841	1483	1493	1505	rBV6	5236	12694	0.86%	0.178%
43	5.924	1517	1519	1522	rVB2	202	109	0.01%	0.002%
44	5.989	1523	1539	1569	rBV	224261	475759	32.35%	6.688%
45	6.268	1622	1626	1627	rBV2	291	168	0.01%	0.002%
46	6.310	1634	1639	1640	rBV2	186	112	0.01%	0.002%
47	6.368	1654	1657	1658	rBV2	170	87	0.01%	0.001%
48	6.419	1671	1673	1675	rBV	205	76	0.01%	0.001%
49	6.458	1682	1685	1689	rVB2	171	123	0.01%	0.002%
50	6.567	1716	1719	1726	rVB	237	240	0.02%	0.003%
51	6.596	1726	1728	1730	rVB	105	45	0.00%	0.001%
52	6.616	1730	1734	1736	rBV	289	176	0.01%	0.002%
53	6.725	1767	1768	1773	rBV	221	205	0.01%	0.003%
54	6.789	1786	1788	1792	rVB	307	193	0.01%	0.003%
55	6.841	1802	1804	1808	rVB2	307	194	0.01%	0.003%
56	6.870	1808	1813	1818	rBV2	301	269	0.02%	0.004%
57	6.918	1818	1828	1851	rBV	71497	148606	10.10%	2.089%
58	7.162	1900	1904	1908	rBV2	613	568	0.04%	0.008%
59	7.246	1920	1930	1956	rBV	184126	342289	23.27%	4.812%
60	7.558	2018	2027	2053	rBV2	51808	104826	7.13%	1.474%
61	7.808	2102	2105	2107	rBV3	597	357	0.02%	0.005%
62	7.857	2116	2120	2122	rBV	264	217	0.01%	0.003%
63	7.898	2130	2133	2136	rBV2	408	259	0.02%	0.004%
64	7.940	2144	2146	2150	rVB2	253	123	0.01%	0.002%
65	7.966	2151	2154	2157	rVB2	175	86	0.01%	0.001%
66	7.985	2157	2160	2163	rBV2	204	116	0.01%	0.002%
67	8.030	2166	2174	2218	rBV3	108571	286786	19.50%	4.032%
68	8.452	2303	2305	2309	rBV	391	218	0.01%	0.003%
69	8.522	2324	2327	2335	rVB3	600	660	0.04%	0.009%
70	8.561	2335	2339	2341	rBV2	509	402	0.03%	0.006%
71	8.680	2374	2376	2378	rVB	228	97	0.01%	0.001%
72	8.699	2378	2382	2384	rBV3	590	404	0.03%	0.006%
73	8.812	2397	2417	2455	rBV2	639505	1470726	100.00%	20.676%
74	9.053	2490	2492	2495	rBV	431	198	0.01%	0.003%
75	9.136	2513	2518	2519	rBV2	426	325	0.02%	0.005%
76	9.249	2549	2553	2554	rBV2	288	158	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035331.D
 Acq On : 22 Apr 2024 14:29
 Operator : SY/MD
 Sample : P2182-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R94

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.297	2566	2568	2570	rBV	250	151	0.01%	0.002%
78	9.339	2578	2581	2583	rVB2	293	135	0.01%	0.002%
79	9.484	2624	2626	2628	rVB	170	69	0.00%	0.001%
80	9.583	2654	2657	2662	rVB2	359	211	0.01%	0.003%
81	9.709	2694	2696	2697	rBV	186	53	0.00%	0.001%
82	9.805	2724	2726	2728	rVB	189	70	0.00%	0.001%
83	9.853	2739	2741	2744	rBV	359	259	0.02%	0.004%
84	10.104	2817	2819	2822	rBV2	277	146	0.01%	0.002%
85	10.149	2822	2833	2860	rBV	428882	684451	46.54%	9.622%
86	10.445	2923	2925	2928	rBV	139	96	0.01%	0.001%
87	10.464	2928	2931	2933	rBV2	381	234	0.02%	0.003%
88	10.763	3022	3024	3027	rVB	295	148	0.01%	0.002%
89	10.847	3047	3050	3052	rBV	367	256	0.02%	0.004%
90	10.882	3058	3061	3064	rVB2	416	265	0.02%	0.004%
91	11.127	3127	3137	3145	rBV2	15073	25403	1.73%	0.357%
92	11.207	3146	3162	3184	rVV2	262807	682570	46.41%	9.596%
93	11.570	3260	3275	3301	rBV2	325619	782909	53.23%	11.006%
94	11.930	3384	3387	3390	rBV3	415	299	0.02%	0.004%
95	12.149	3454	3455	3456	rBV3	194	69	0.00%	0.001%
96	12.561	3578	3583	3585	rBV	536	429	0.03%	0.006%
97	12.596	3589	3594	3596	rBV4	1325	1217	0.08%	0.017%
98	13.201	3774	3782	3795	rBV2	26599	43273	2.94%	0.608%
99	13.339	3823	3825	3830	rBV2	514	373	0.03%	0.005%
100	13.686	3926	3933	3940	rBV3	5259	7332	0.50%	0.103%

Sum of corrected areas: 7113344




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035331.D
Acq On : 22 Apr 2024 14:29
Operator : SY/MD
Sample : P2182-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

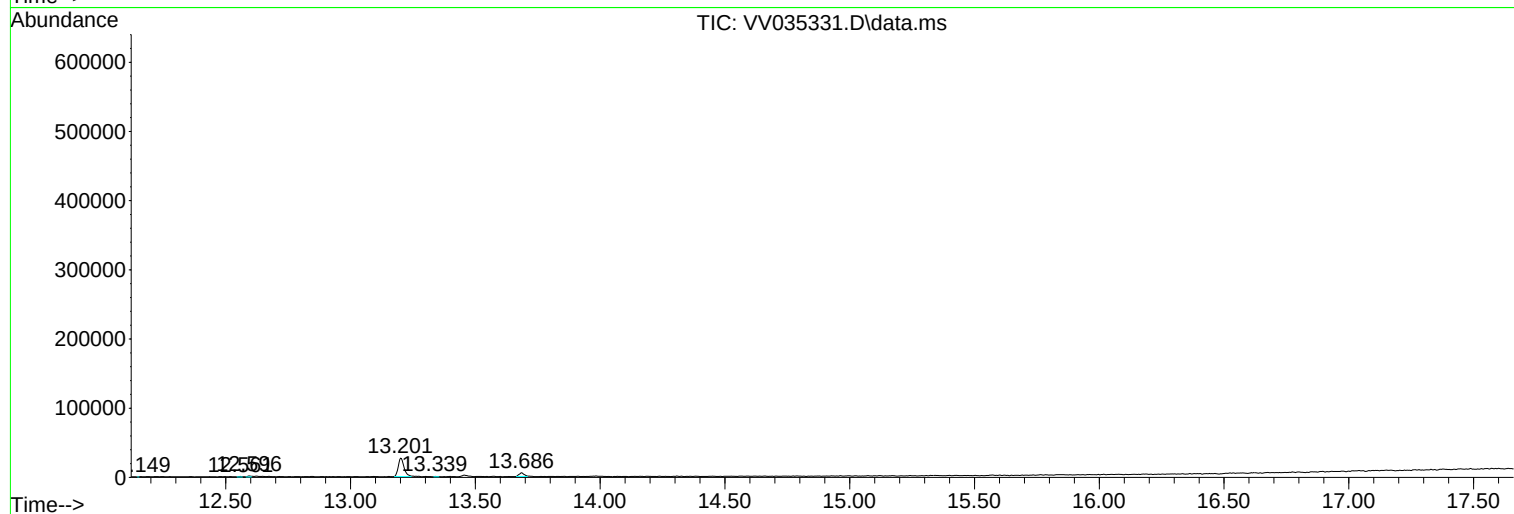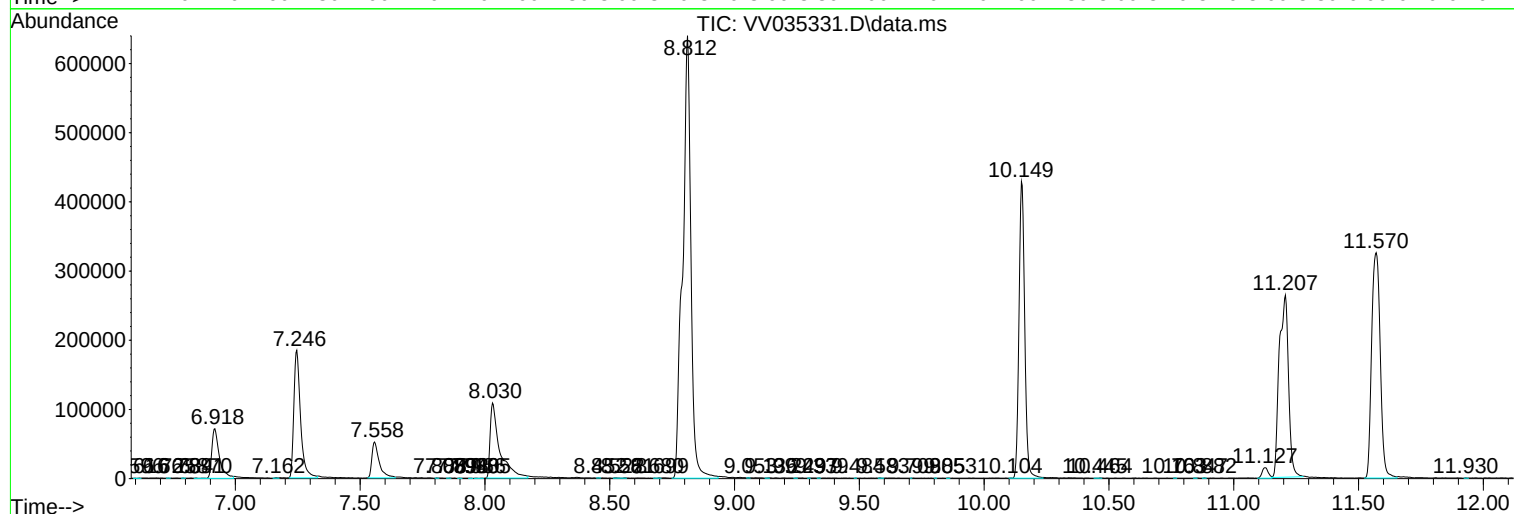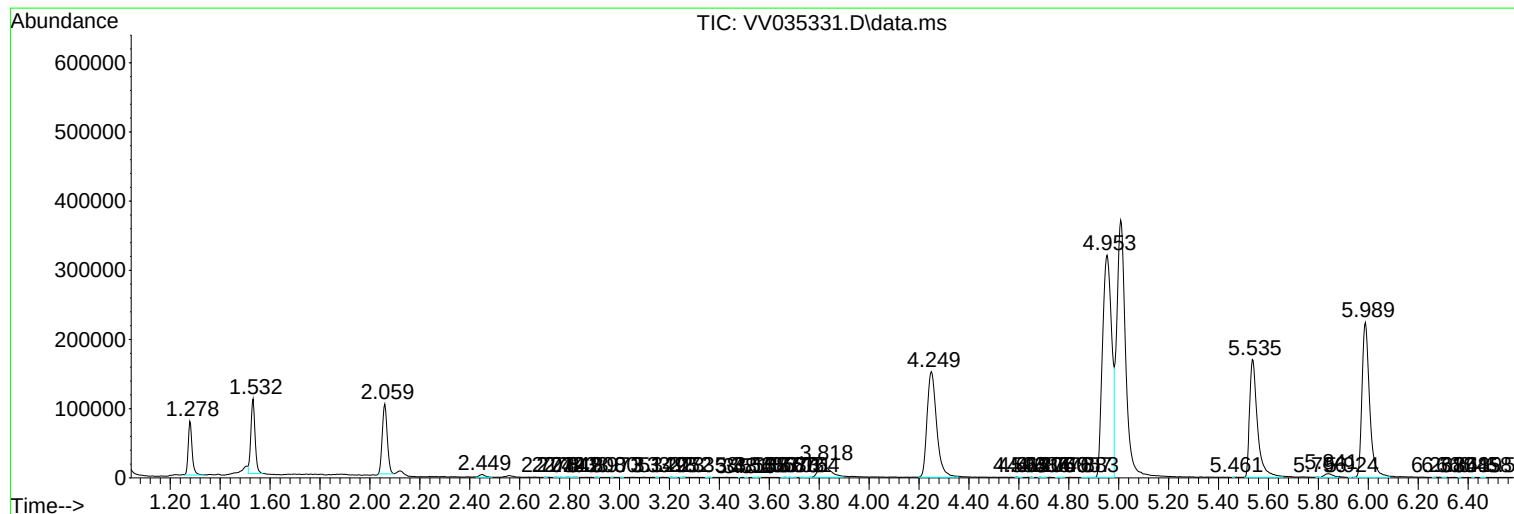

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035331.D
Acq On : 22 Apr 2024 14:29
Operator : SY/MD
Sample : P2182-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035331.D
Acq On : 22 Apr 2024 14:29
Operator : SY/MD
Sample : P2182-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------