

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035333.D
 Acq On : 22 Apr 2024 15:16
 Operator : SY/MD
 Sample : P2182-02 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035333.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	76563	81332	0.75%	0.302%
2	1.532	146	153	169	rVB	107960	130166	1.20%	0.483%
3	2.060	308	317	329	rBV	99507	143225	1.32%	0.532%
4	2.388	416	419	420	rBV2	648	326	0.00%	0.001%
5	2.449	431	438	451	rVB	8480	13567	0.13%	0.050%
6	2.561	464	473	475	rBV4	1661	2359	0.02%	0.009%
7	2.642	495	498	503	rVB2	600	391	0.00%	0.001%
8	2.690	510	513	517	rVB2	440	272	0.00%	0.001%
9	2.716	517	521	524	rBV3	424	416	0.00%	0.002%
10	2.732	524	526	531	rVV3	416	363	0.00%	0.001%
11	2.761	531	535	539	rVB3	386	352	0.00%	0.001%
12	2.876	566	571	575	rBV4	389	382	0.00%	0.001%
13	2.909	578	581	586	rVB	430	408	0.00%	0.002%
14	2.947	586	593	597	rBV3	506	460	0.00%	0.002%
15	3.478	756	758	768	rVB2	255	284	0.00%	0.001%
16	3.812	849	862	886	rBV2	16289	60361	0.56%	0.224%
17	4.182	972	977	979	rBV3	422	309	0.00%	0.001%
18	4.249	981	998	1030	rBV	164238	438859	4.05%	1.629%
19	4.548	1086	1091	1093	rVB2	327	278	0.00%	0.001%
20	4.561	1093	1095	1098	rBV	527	375	0.00%	0.001%
21	4.828	1172	1178	1180	rBV2	473	359	0.00%	0.001%
22	4.953	1202	1217	1222	rBV3	344647	772603	7.13%	2.868%
23	5.005	1224	1233	1278	rVB	2378805	5247798	48.43%	19.477%
24	5.535	1388	1398	1430	rBV	165804	360880	3.33%	1.339%
25	5.841	1482	1493	1507	rBV5	5375	12428	0.11%	0.046%
26	5.928	1516	1520	1523	rBV3	495	348	0.00%	0.001%
27	5.989	1525	1539	1569	rBV	233750	490696	4.53%	1.821%
28	6.153	1588	1590	1594	rVB3	540	360	0.00%	0.001%
29	6.320	1639	1642	1645	rVB	437	214	0.00%	0.001%
30	6.378	1658	1660	1665	rVV3	396	337	0.00%	0.001%
31	6.426	1672	1675	1677	rVV2	342	241	0.00%	0.001%
32	6.436	1677	1678	1681	rVV2	442	217	0.00%	0.001%
33	6.458	1683	1685	1688	rVV	422	289	0.00%	0.001%
34	6.487	1690	1694	1700	rVV2	385	553	0.01%	0.002%
35	6.535	1704	1709	1713	rVV2	474	475	0.00%	0.002%
36	6.555	1713	1715	1719	rVV3	332	267	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035333.D
 Acq On : 22 Apr 2024 15:16
 Operator : SY/MD
 Sample : P2182-02 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.638	1738	1741	1742	rVB2	501	236	0.00%	0.001%
38	6.735	1768	1771	1775	rVB2	389	230	0.00%	0.001%
39	6.857	1808	1809	1814	rVB	415	221	0.00%	0.001%
40	6.918	1818	1828	1859	rBV	74366	154023	1.42%	0.572%
41	7.066	1872	1874	1879	rVB3	493	352	0.00%	0.001%
42	7.162	1901	1904	1908	rBV4	450	415	0.00%	0.002%
43	7.246	1920	1930	1958	rBV	182778	339294	3.13%	1.259%
44	7.558	2018	2027	2052	rBV	53995	111602	1.03%	0.414%
45	7.693	2067	2069	2071	rBV2	391	227	0.00%	0.001%
46	7.908	2134	2136	2141	rBV3	396	336	0.00%	0.001%
47	7.963	2149	2153	2156	rBV3	309	287	0.00%	0.001%
48	8.027	2164	2173	2215	rBV2	159163	381230	3.52%	1.415%
49	8.355	2272	2275	2277	rBV3	567	349	0.00%	0.001%
50	8.368	2277	2279	2287	rVB5	950	916	0.01%	0.003%
51	8.448	2301	2304	2309	rBV2	436	385	0.00%	0.001%
52	8.542	2330	2333	2336	rVB	460	272	0.00%	0.001%
53	8.574	2339	2343	2346	rVB3	468	344	0.00%	0.001%
54	8.616	2352	2356	2358	rBV	383	250	0.00%	0.001%
55	8.725	2388	2390	2395	rVB2	455	248	0.00%	0.001%
56	8.809	2398	2416	2469	rBV	6690151	10834880	100.00%	40.214%
57	9.551	2644	2647	2649	rBV	354	279	0.00%	0.001%
58	9.731	2700	2703	2706	rBV2	543	390	0.00%	0.001%
59	9.838	2733	2736	2738	rBV2	363	223	0.00%	0.001%
60	9.937	2763	2767	2771	rVV2	443	322	0.00%	0.001%
61	10.001	2783	2787	2792	rBV2	278	230	0.00%	0.001%
62	10.149	2820	2833	2858	rBV	452839	725148	6.69%	2.691%
63	10.371	2900	2902	2904	rBV	537	359	0.00%	0.001%
64	10.410	2912	2914	2920	rVV3	355	290	0.00%	0.001%
65	10.458	2926	2929	2933	rBV3	314	300	0.00%	0.001%
66	10.751	3016	3020	3028	rVV4	556	669	0.01%	0.002%
67	10.866	3053	3056	3059	rVV3	467	314	0.00%	0.001%
68	10.940	3077	3079	3084	rVB	373	226	0.00%	0.001%
69	10.995	3091	3096	3101	rBV2	225	258	0.00%	0.001%
70	11.120	3125	3135	3146	rBV2	65701	104799	0.97%	0.389%
71	11.207	3146	3162	3188	rVV	1681524	2818000	26.01%	10.459%
72	11.397	3219	3221	3223	rVB2	966	398	0.00%	0.001%
73	11.481	3244	3247	3249	rBV	483	292	0.00%	0.001%
74	11.497	3249	3252	3254	rBV2	312	219	0.00%	0.001%
75	11.574	3260	3276	3313	rBV2	2085205	3555049	32.81%	13.195%
76	11.915	3380	3382	3387	rVB3	513	375	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035333.D
 Acq On : 22 Apr 2024 15:16
 Operator : SY/MD
 Sample : P2182-02 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	12.075	3430	3432	3436	rBV3	317	226	0.00%	0.001%
78	12.120	3444	3446	3449	rBV	395	234	0.00%	0.001%
79	12.178	3460	3464	3468	rBV3	482	390	0.00%	0.001%
80	12.194	3468	3469	3475	rVB3	361	272	0.00%	0.001%
81	12.342	3511	3515	3523	rVB5	340	378	0.00%	0.001%
82	12.374	3523	3525	3529	rBV2	254	236	0.00%	0.001%
83	12.513	3565	3568	3570	rVB2	466	277	0.00%	0.001%
84	12.593	3589	3593	3597	rBV3	669	704	0.01%	0.003%
85	12.680	3617	3620	3621	rBV2	424	231	0.00%	0.001%
86	12.821	3661	3664	3666	rBV3	490	285	0.00%	0.001%
87	12.860	3673	3676	3679	rBV2	433	334	0.00%	0.001%
88	12.937	3695	3700	3702	rBV2	311	325	0.00%	0.001%
89	12.976	3707	3712	3717	rBV	16404	12443	0.11%	0.046%
90	13.201	3771	3782	3805	rBV2	59811	99940	0.92%	0.371%
91	13.458	3856	3862	3870	rVV3	1654	2297	0.02%	0.009%
92	13.554	3889	3892	3898	rVV3	446	348	0.00%	0.001%
93	13.683	3923	3932	3943	rBV2	14921	24160	0.22%	0.090%
94	13.963	4016	4019	4022	rBV3	461	402	0.00%	0.001%
95	14.027	4037	4039	4045	rBV3	625	575	0.01%	0.002%
96	14.387	4147	4151	4152	rBV2	561	329	0.00%	0.001%
97	14.779	4270	4273	4277	rBV2	779	480	0.00%	0.002%
98	14.886	4304	4306	4308	rBV	599	285	0.00%	0.001%
99	15.017	4345	4347	4354	rBV4	566	525	0.00%	0.002%
100	15.242	4414	4417	4420	rBV4	911	804	0.01%	0.003%




Sum of corrected areas: 26943267

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035333.D
Acq On : 22 Apr 2024 15:16
Operator : SY/MD
Sample : P2182-02 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

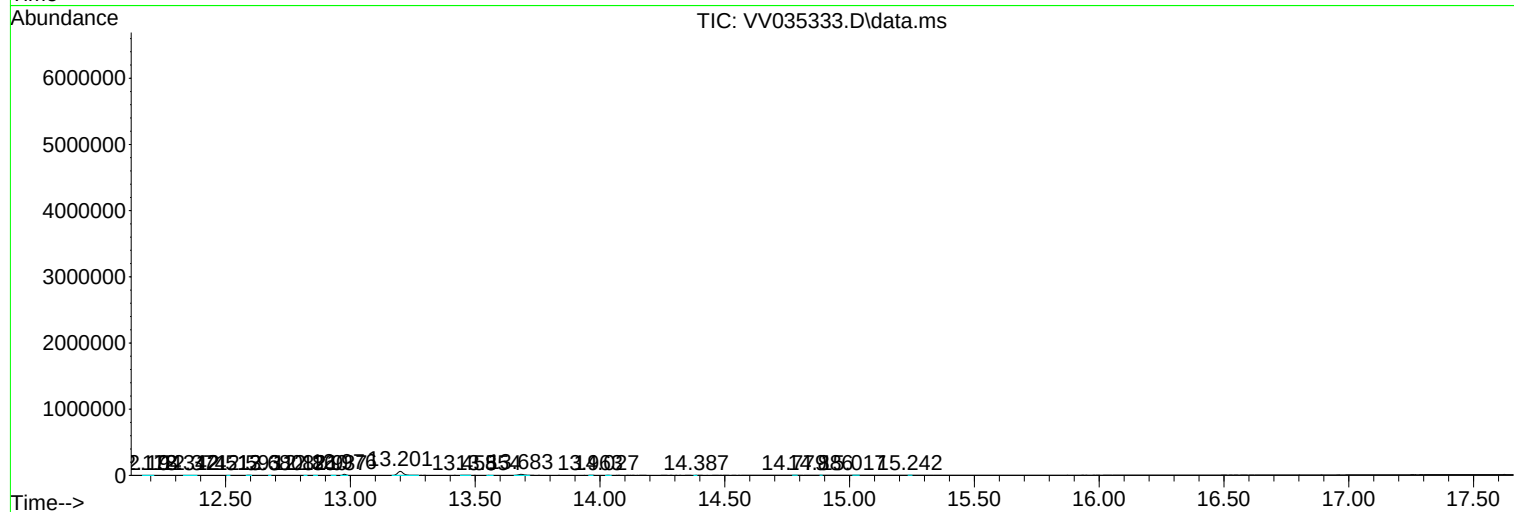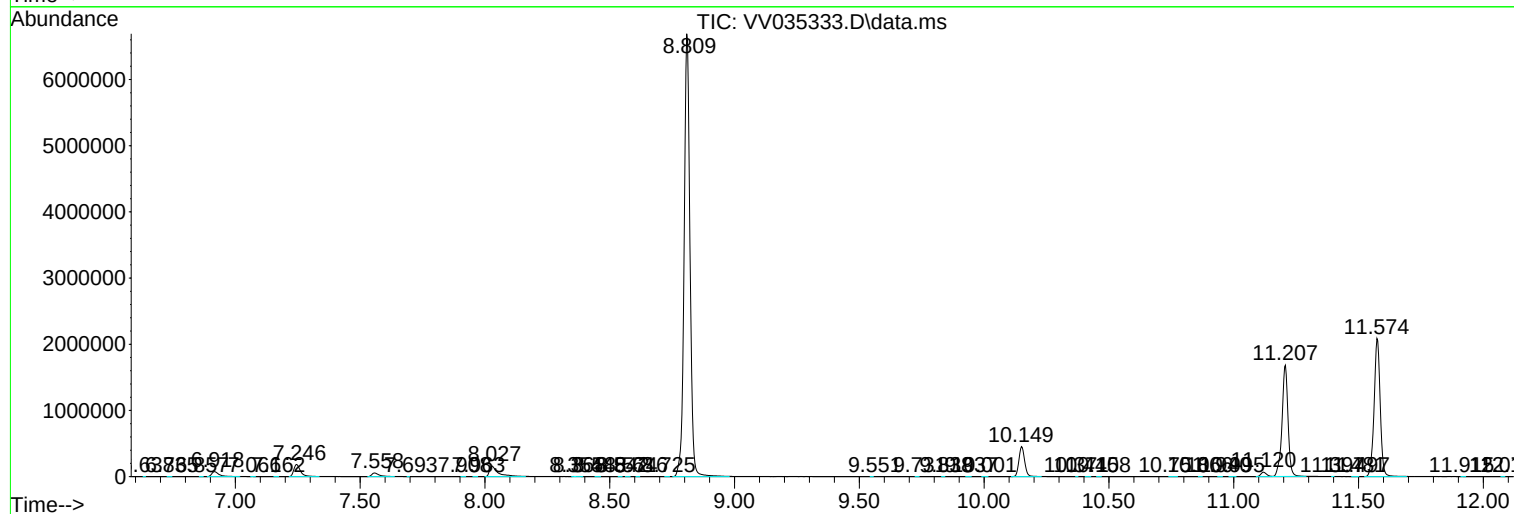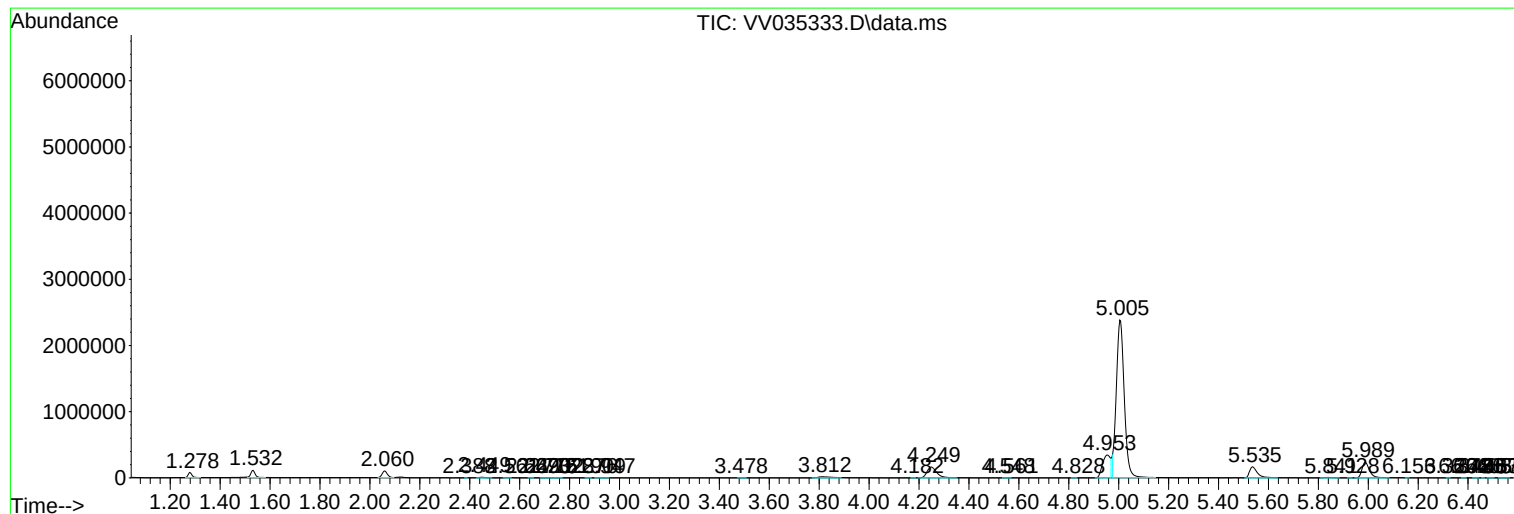

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035333.D
Acq On : 22 Apr 2024 15:16
Operator : SY/MD
Sample : P2182-02 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035333.D
Acq On : 22 Apr 2024 15:16
Operator : SY/MD
Sample : P2182-02 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc