

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035334.D
 Acq On : 22 Apr 2024 15:39
 Operator : SY/MD
 Sample : P2158-04DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035334.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rBV	84713	86870	3.96%	1.082%
2	1.532	147	153	175	rVB	110970	134072	6.11%	1.671%
3	2.060	309	317	329	rVB	107103	152368	6.95%	1.899%
4	2.404	422	424	426	rBV2	340	142	0.01%	0.002%
5	2.452	431	439	448	rVB4	2676	5036	0.23%	0.063%
6	2.622	489	492	493	rBV4	216	107	0.00%	0.001%
7	2.680	508	510	513	rVB2	327	127	0.01%	0.002%
8	2.780	539	541	545	rBV3	188	122	0.01%	0.002%
9	2.870	566	569	572	rBV2	383	260	0.01%	0.003%
10	2.889	572	575	581	rVB2	507	373	0.02%	0.005%
11	2.969	595	600	603	rBV3	350	349	0.02%	0.004%
12	3.021	612	616	618	rBV2	437	315	0.01%	0.004%
13	3.047	621	624	625	rBV	183	90	0.00%	0.001%
14	3.059	625	628	630	rBV	230	145	0.01%	0.002%
15	3.117	643	646	651	rVB3	375	266	0.01%	0.003%
16	3.195	667	670	672	rBV2	340	162	0.01%	0.002%
17	3.249	682	687	688	rBV	301	207	0.01%	0.003%
18	3.281	692	697	700	rBV2	362	292	0.01%	0.004%
19	3.301	700	703	707	rBV2	265	207	0.01%	0.003%
20	3.336	712	714	717	rBV2	296	172	0.01%	0.002%
21	3.371	723	725	729	rVB	257	114	0.01%	0.001%
22	3.394	729	732	736	rVV	318	204	0.01%	0.003%
23	3.416	736	739	742	rVB2	171	115	0.01%	0.001%
24	3.500	762	765	770	rVB	326	259	0.01%	0.003%
25	3.555	778	782	786	rBV2	211	230	0.01%	0.003%
26	3.609	796	799	801	rBV	186	114	0.01%	0.001%
27	3.661	812	815	818	rBV2	186	159	0.01%	0.002%
28	3.693	823	825	829	rBV	152	90	0.00%	0.001%
29	3.725	829	835	838	rBV2	299	233	0.01%	0.003%
30	3.754	843	844	847	rVB2	89	41	0.00%	0.001%
31	3.818	848	864	893	rBV2	14855	56745	2.59%	0.707%
32	4.175	973	975	976	rBV2	205	87	0.00%	0.001%
33	4.249	982	998	1033	rBV	164064	435803	19.87%	5.430%
34	4.513	1078	1080	1083	rBV	247	163	0.01%	0.002%
35	4.619	1111	1113	1119	rVB4	507	405	0.02%	0.005%
36	4.645	1119	1121	1123	rBV	234	158	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035334.D
 Acq On : 22 Apr 2024 15:39
 Operator : SY/MD
 Sample : P2158-04DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	4.683	1131	1133	1138	rVB	296	164	0.01%	0.002%
38	4.712	1138	1142	1143	rBV	304	214	0.01%	0.003%
39	4.722	1143	1145	1148	rBV2	308	209	0.01%	0.003%
40	4.786	1163	1165	1167	rBV2	182	89	0.00%	0.001%
41	4.844	1180	1183	1187	rBV3	324	262	0.01%	0.003%
42	4.953	1202	1217	1224	rBV2	346776	842729	38.43%	10.501%
43	5.455	1372	1373	1377	rVB3	630	346	0.02%	0.004%
44	5.535	1388	1398	1428	rBV	182635	394796	18.00%	4.919%
45	5.838	1482	1492	1499	rBV6	6634	12580	0.57%	0.157%
46	5.918	1515	1517	1519	rBV6	349	207	0.01%	0.003%
47	5.989	1527	1539	1568	rBV	234127	494868	22.57%	6.166%
48	6.249	1618	1620	1621	rBV2	300	138	0.01%	0.002%
49	6.304	1635	1637	1644	rVB2	428	315	0.01%	0.004%
50	6.329	1644	1645	1647	rBV2	311	128	0.01%	0.002%
51	6.397	1663	1666	1670	rVB3	574	338	0.02%	0.004%
52	6.419	1670	1673	1674	rBV2	202	106	0.00%	0.001%
53	6.426	1674	1675	1678	rVV	292	88	0.00%	0.001%
54	6.448	1680	1682	1690	rVB2	398	263	0.01%	0.003%
55	6.493	1695	1696	1697	rBV	166	47	0.00%	0.001%
56	6.503	1697	1699	1701	rBV2	211	102	0.00%	0.001%
57	6.628	1736	1738	1740	rBV	380	199	0.01%	0.002%
58	6.722	1765	1767	1772	rBV2	358	361	0.02%	0.004%
59	6.767	1778	1781	1784	rBV	231	120	0.01%	0.001%
60	6.789	1784	1788	1790	rBV2	387	286	0.01%	0.004%
61	6.870	1810	1813	1814	rBV	125	78	0.00%	0.001%
62	6.918	1818	1828	1858	rBV	75319	159104	7.26%	1.983%
63	7.246	1920	1930	1958	rBV	200009	367816	16.77%	4.583%
64	7.558	2018	2027	2053	rBV	55878	112142	5.11%	1.397%
65	7.773	2091	2094	2100	rVB3	345	294	0.01%	0.004%
66	7.821	2104	2109	2112	rBV2	570	476	0.02%	0.006%
67	7.902	2132	2134	2135	rBV2	204	51	0.00%	0.001%
68	7.972	2152	2156	2157	rBV2	277	176	0.01%	0.002%
69	8.030	2165	2174	2212	rBV2	109479	288486	13.16%	3.595%
70	8.355	2273	2275	2277	rBV2	685	416	0.02%	0.005%
71	8.458	2305	2307	2310	rVB2	705	243	0.01%	0.003%
72	8.632	2359	2361	2362	rBV	157	55	0.00%	0.001%
73	8.702	2379	2383	2385	rBV	216	161	0.01%	0.002%
74	8.722	2385	2389	2391	rBV	278	186	0.01%	0.002%
75	8.812	2399	2417	2451	rBV2	1083244	2192844	100.00%	27.324%
76	9.320	2573	2575	2577	rBV2	272	165	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035334.D
 Acq On : 22 Apr 2024 15:39
 Operator : SY/MD
 Sample : P2158-04DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.509	2631	2634	2637	rBV	462	335	0.02%	0.004%
78	9.593	2656	2660	2663	rBV2	320	258	0.01%	0.003%
79	9.622	2666	2669	2671	rBV	253	150	0.01%	0.002%
80	9.677	2682	2686	2687	rBV	247	160	0.01%	0.002%
81	9.722	2696	2700	2708	rVB4	435	608	0.03%	0.008%
82	9.763	2708	2713	2714	rBV	294	243	0.01%	0.003%
83	9.828	2730	2733	2734	rBV	240	145	0.01%	0.002%
84	9.969	2774	2777	2779	rBV2	285	139	0.01%	0.002%
85	10.011	2787	2790	2793	rBV	274	226	0.01%	0.003%
86	10.149	2821	2833	2866	rBV	454501	715457	32.63%	8.915%
87	10.574	2963	2965	2971	rBV	257	239	0.01%	0.003%
88	10.889	3060	3063	3066	rBV	276	148	0.01%	0.002%
89	11.037	3106	3109	3111	rVB	227	111	0.01%	0.001%
90	11.050	3111	3113	3117	rBV	275	212	0.01%	0.003%
91	11.069	3117	3119	3124	rVB2	341	156	0.01%	0.002%
92	11.127	3127	3137	3145	rBV3	9752	15542	0.71%	0.194%
93	11.207	3146	3162	3186	rVB2	271123	703001	32.06%	8.760%
94	11.451	3234	3238	3239	rBV2	366	241	0.01%	0.003%
95	11.570	3260	3275	3303	rBV2	331152	798014	36.39%	9.944%
96	11.750	3328	3331	3334	rBV2	540	383	0.02%	0.005%
97	12.435	3539	3544	3545	rBV	374	314	0.01%	0.004%
98	13.204	3774	3783	3795	rBV2	20930	35116	1.60%	0.438%
99	13.352	3826	3829	3831	rVB3	402	203	0.01%	0.003%
100	13.686	3929	3933	3947	rVB4	4048	5668	0.26%	0.071%




Sum of corrected areas: 8025319

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035334.D
Acq On : 22 Apr 2024 15:39
Operator : SY/MD
Sample : P2158-04DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

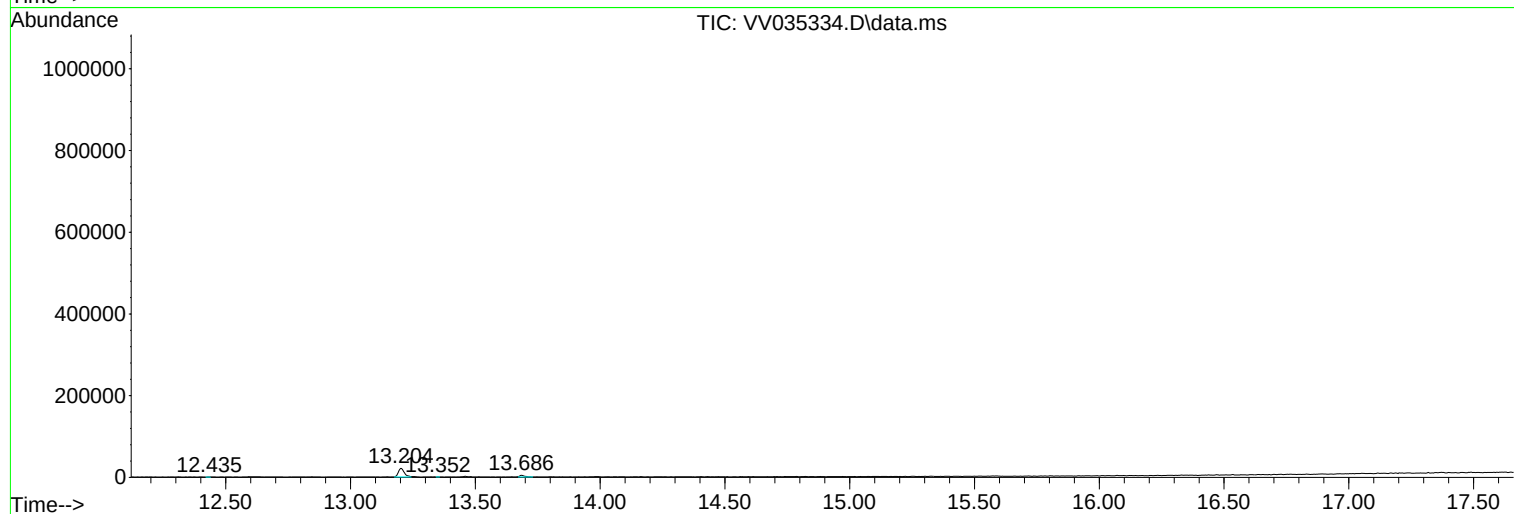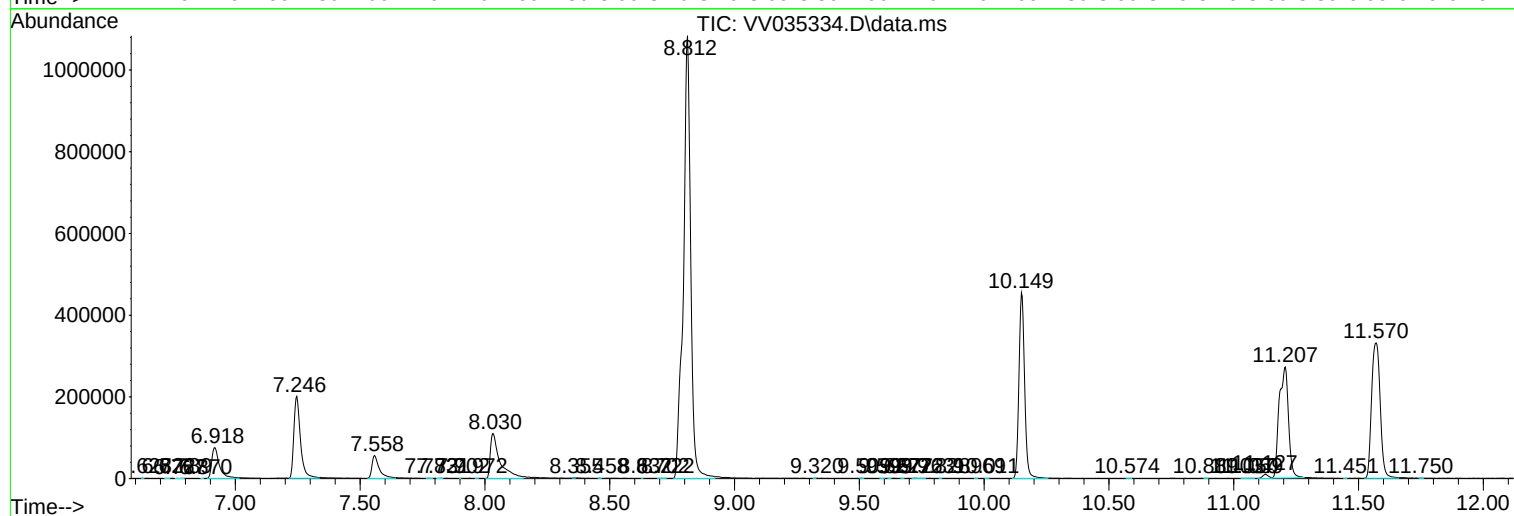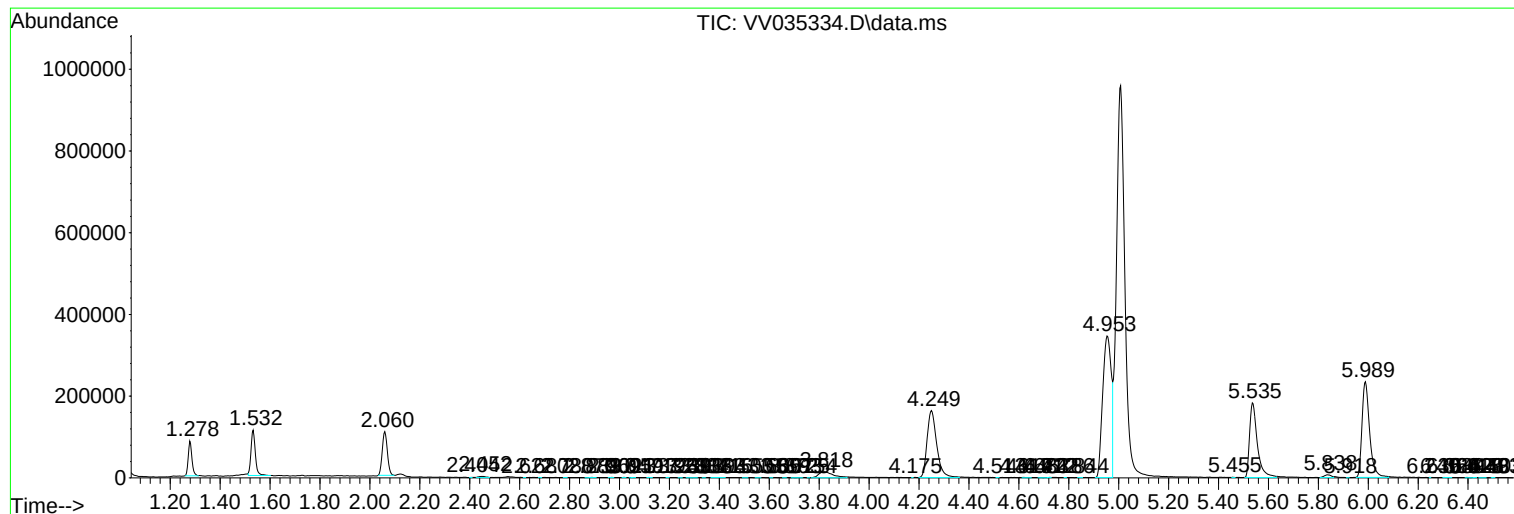

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035334.D
Acq On : 22 Apr 2024 15:39
Operator : SY/MD
Sample : P2158-04DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035334.D
Acq On : 22 Apr 2024 15:39
Operator : SY/MD
Sample : P2158-04DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------