

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035335.D
 Acq On : 22 Apr 2024 16:02
 Operator : SY/MD
 Sample : VIBLK280
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK280

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035335.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	159153	170037	12.56%	1.734%
2	1.532	146	153	170	rVB	157894	187789	13.87%	1.915%
3	2.060	308	317	333	rBV	265656	379652	28.05%	3.872%
4	2.349	400	407	429	rVB	27894	51813	3.83%	0.528%
5	2.809	548	550	553	rBV	285	203	0.01%	0.002%
6	3.072	630	632	635	rVB2	352	130	0.01%	0.001%
7	3.195	667	670	673	rBV	263	196	0.01%	0.002%
8	3.214	673	676	677	rBV2	155	90	0.01%	0.001%
9	3.371	721	725	727	rBV	386	292	0.02%	0.003%
10	3.487	759	761	765	rVB2	176	114	0.01%	0.001%
11	3.510	765	768	771	rBV2	285	186	0.01%	0.002%
12	3.529	771	774	777	rVB	189	95	0.01%	0.001%
13	3.551	777	781	784	rBV2	187	202	0.01%	0.002%
14	3.613	797	800	804	rBV	242	141	0.01%	0.001%
15	3.703	825	828	830	rVB	183	104	0.01%	0.001%
16	3.796	848	857	897	rBV	82379	262044	19.36%	2.673%
17	4.249	982	998	1031	rBV	217414	565404	41.77%	5.767%
18	4.722	1141	1145	1148	rBV3	283	303	0.02%	0.003%
19	4.741	1148	1151	1154	rBV2	507	391	0.03%	0.004%
20	4.783	1160	1164	1166	rBV2	396	251	0.02%	0.003%
21	4.957	1202	1218	1259	rBV2	499171	1353539	100.00%	13.806%
22	5.368	1344	1346	1349	rBV2	359	162	0.01%	0.002%
23	5.413	1357	1360	1362	rBV2	409	313	0.02%	0.003%
24	5.471	1375	1378	1381	rVB	376	203	0.01%	0.002%
25	5.535	1387	1398	1431	rBV	381956	815935	60.28%	8.322%
26	5.834	1482	1491	1514	rVB5	7526	18773	1.39%	0.191%
27	5.989	1526	1539	1568	rBV	305418	642858	47.49%	6.557%
28	6.259	1621	1623	1625	rBV2	264	112	0.01%	0.001%
29	6.326	1643	1644	1646	rBV2	293	88	0.01%	0.001%
30	6.381	1657	1661	1666	rBV3	324	285	0.02%	0.003%
31	6.403	1666	1668	1672	rVB2	322	179	0.01%	0.002%
32	6.445	1679	1681	1684	rBV	133	84	0.01%	0.001%
33	6.461	1684	1686	1688	rVB2	405	167	0.01%	0.002%
34	6.474	1688	1690	1691	rBV	159	43	0.00%	0.000%
35	6.490	1691	1695	1699	rVB2	292	284	0.02%	0.003%
36	6.509	1699	1701	1703	rBV	198	101	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035335.D
 Acq On : 22 Apr 2024 16:02
 Operator : SY/MD
 Sample : VIBLK280
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK280

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.587	1722	1725	1727	rBV2	240	165	0.01%	0.002%
38	6.657	1745	1747	1751	rVB2	575	358	0.03%	0.004%
39	6.680	1751	1754	1759	rVV2	381	332	0.02%	0.003%
40	6.712	1763	1764	1767	rVV3	469	271	0.02%	0.003%
41	6.741	1770	1773	1776	rVB	388	252	0.02%	0.003%
42	6.760	1776	1779	1780	rBV	208	89	0.01%	0.001%
43	6.915	1816	1827	1864	rBV	104205	212883	15.73%	2.171%
44	7.243	1918	1929	1957	rBV	497388	896612	66.24%	9.145%
45	7.554	2017	2026	2048	rBV	72546	140610	10.39%	1.434%
46	7.873	2120	2125	2127	rBV2	599	371	0.03%	0.004%
47	7.982	2156	2159	2160	rBV	178	87	0.01%	0.001%
48	8.027	2164	2173	2218	rBV2	223973	539259	39.84%	5.500%
49	8.545	2330	2334	2335	rBV	363	221	0.02%	0.002%
50	8.571	2340	2342	2343	rBV	233	88	0.01%	0.001%
51	8.654	2365	2368	2370	rBV2	294	160	0.01%	0.002%
52	8.783	2397	2408	2438	rBV	607389	1044391	77.16%	10.653%
53	9.059	2492	2494	2495	rBV	332	181	0.01%	0.002%
54	9.107	2507	2509	2513	rBV5	506	302	0.02%	0.003%
55	9.197	2535	2537	2538	rBV5	294	71	0.01%	0.001%
56	9.220	2542	2544	2545	rBV	226	69	0.01%	0.001%
57	9.255	2554	2555	2558	rBV	233	118	0.01%	0.001%
58	9.390	2594	2597	2599	rBV	214	138	0.01%	0.001%
59	9.432	2608	2610	2612	rBV	202	60	0.00%	0.001%
60	9.484	2625	2626	2628	rBV	280	99	0.01%	0.001%
61	9.574	2652	2654	2657	rVB	253	91	0.01%	0.001%
62	9.625	2668	2670	2673	rBV2	198	108	0.01%	0.001%
63	9.654	2677	2679	2681	rVB	163	65	0.00%	0.001%
64	9.667	2681	2683	2684	rBV	212	99	0.01%	0.001%
65	9.734	2701	2704	2706	rBV2	274	153	0.01%	0.002%
66	9.776	2715	2717	2723	rBV	292	331	0.02%	0.003%
67	9.821	2729	2731	2735	rBV	122	64	0.00%	0.001%
68	9.911	2756	2759	2764	rVB2	348	262	0.02%	0.003%
69	9.940	2764	2768	2774	rBV	282	290	0.02%	0.003%
70	9.992	2780	2784	2791	rVB3	340	386	0.03%	0.004%
71	10.078	2809	2811	2815	rVB2	238	164	0.01%	0.002%
72	10.149	2822	2833	2861	rBV	475220	762458	56.33%	7.777%
73	10.397	2907	2910	2913	rBV3	316	200	0.01%	0.002%
74	10.484	2934	2937	2941	rVB3	549	313	0.02%	0.003%
75	10.519	2946	2948	2950	rBV	204	110	0.01%	0.001%
76	10.561	2959	2961	2963	rBV2	262	165	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035335.D
Acq On : 22 Apr 2024 16:02
Operator : SY/MD
Sample : VIBLK280
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK280

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

77	10.644	2983	2987	2990	rBV	295	201	0.01%	0.002%
78	10.860	3052	3054	3055	rBV	409	164	0.01%	0.002%
79	11.133	3132	3139	3144	rBV5	1600	2374	0.18%	0.024%
80	11.185	3144	3155	3186	rVV	536670	872416	64.45%	8.899%
81	11.561	3259	3272	3292	rBV	522367	865294	63.93%	8.826%
82	12.014	3411	3413	3416	rBV	297	179	0.01%	0.002%
83	13.123	3755	3758	3761	rBV	473	322	0.02%	0.003%
84	13.207	3778	3784	3797	rVB5	5084	8083	0.60%	0.082%




Sum of corrected areas: 9804042

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035335.D
Acq On : 22 Apr 2024 16:02
Operator : SY/MD
Sample : VIBLK280
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK280

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

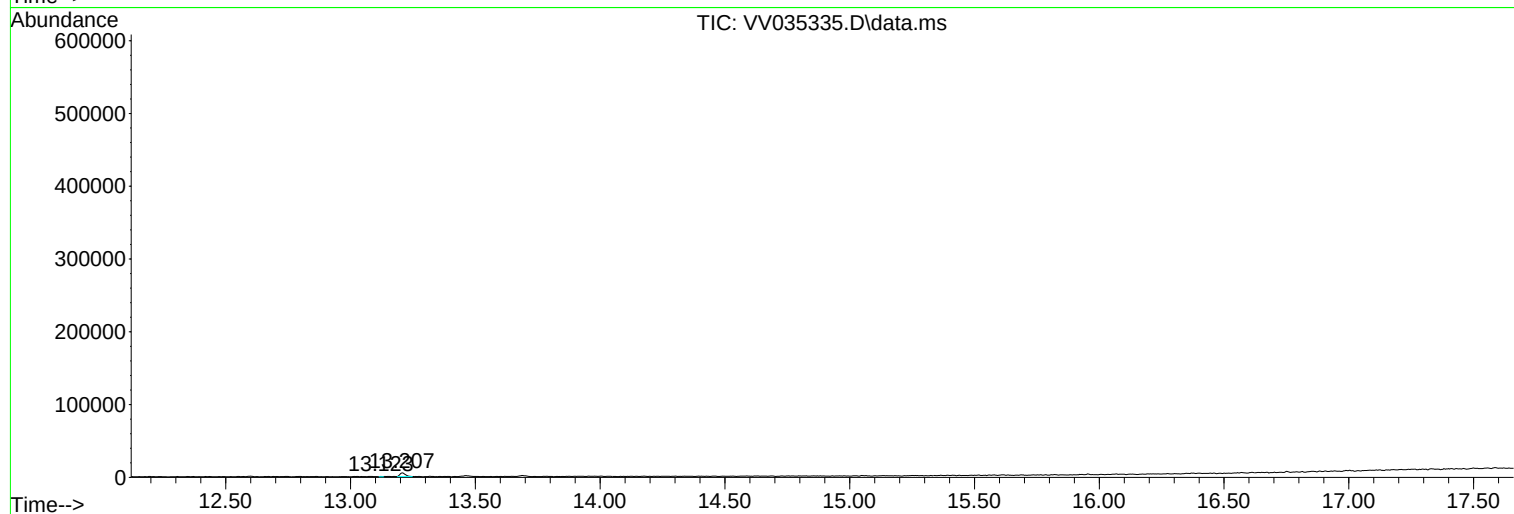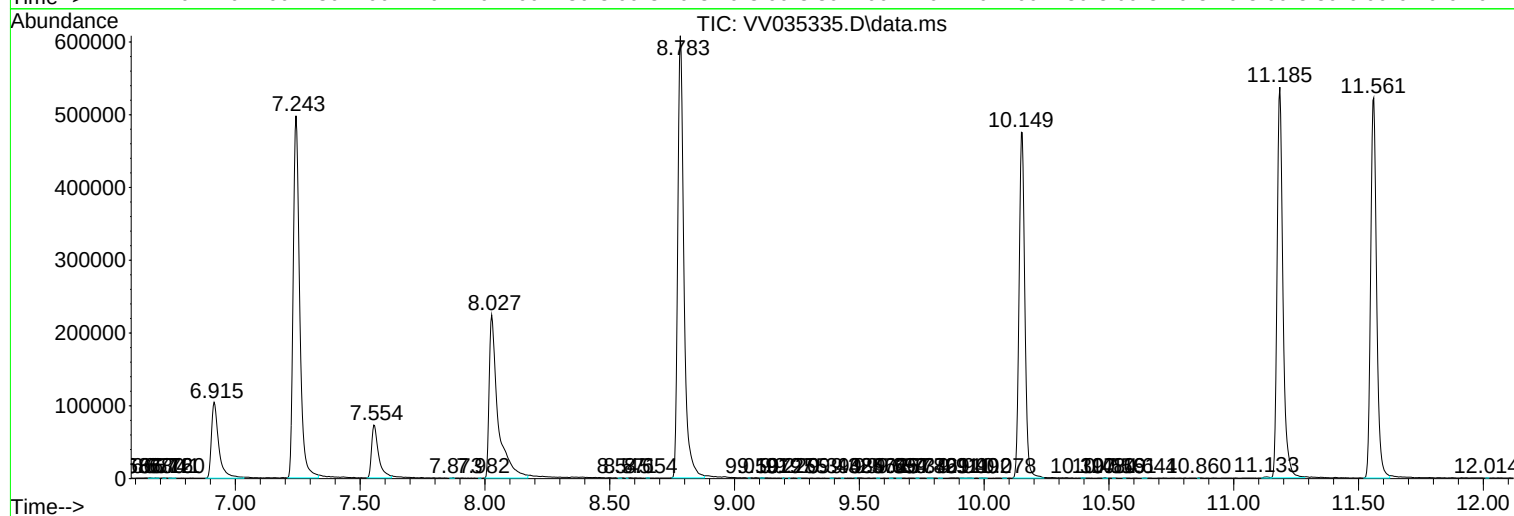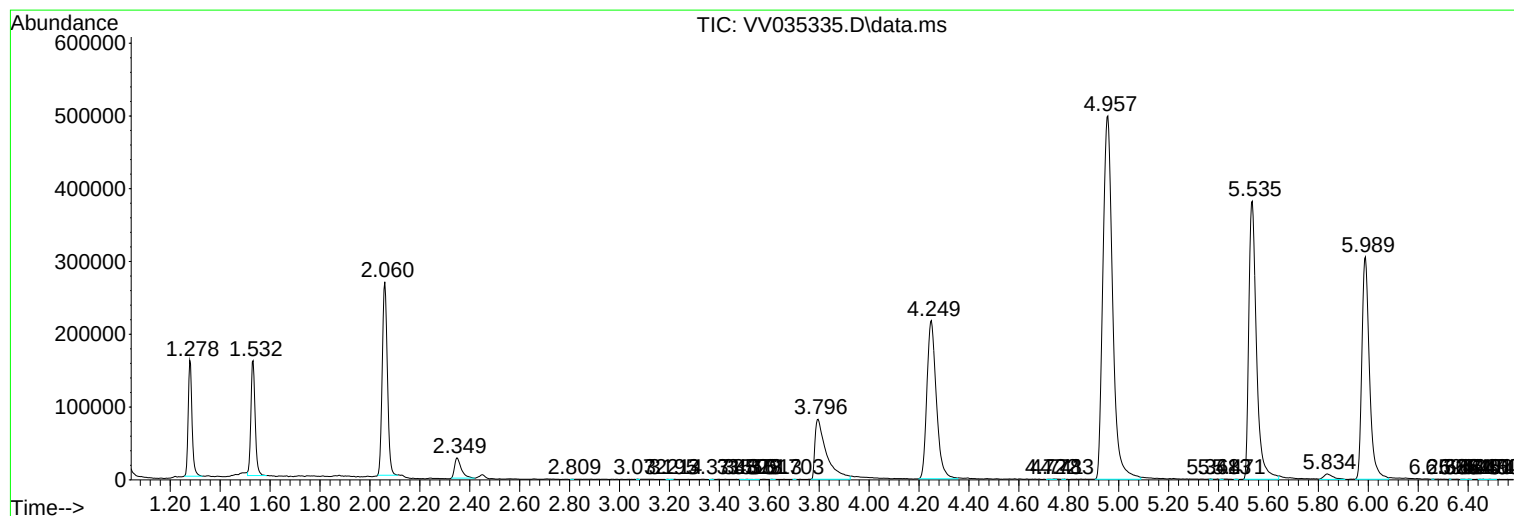

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035335.D
Acq On : 22 Apr 2024 16:02
Operator : SY/MD
Sample : VIBLK280
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK280

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035335.D
Acq On : 22 Apr 2024 16:02
Operator : SY/MD
Sample : VIBLK280
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK280

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------