

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035337.D
 Acq On : 22 Apr 2024 16:48
 Operator : SY/MD
 Sample : P2158-10DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035337.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	79729	86355	9.24%	1.260%
2	1.532	147	153	169	rVB	106510	123780	13.24%	1.805%
3	2.060	309	317	333	rVB	106513	153706	16.44%	2.242%
4	2.452	433	439	449	rVB8	2930	5089	0.54%	0.074%
5	2.658	501	503	508	rBV3	464	251	0.03%	0.004%
6	2.680	508	510	513	rBV2	287	151	0.02%	0.002%
7	2.851	560	563	565	rBV	359	216	0.02%	0.003%
8	3.002	604	610	613	rBV2	390	323	0.03%	0.005%
9	3.015	613	614	620	rVB	250	124	0.01%	0.002%
10	3.043	620	623	626	rBV2	227	202	0.02%	0.003%
11	3.188	664	668	669	rBV	158	106	0.01%	0.002%
12	3.336	710	714	716	rBV	258	216	0.02%	0.003%
13	3.368	721	724	729	rVB4	455	370	0.04%	0.005%
14	3.394	729	732	737	rBV2	195	205	0.02%	0.003%
15	3.481	756	759	763	rVB2	268	196	0.02%	0.003%
16	3.519	763	771	773	rBV2	267	271	0.03%	0.004%
17	3.645	806	810	813	rVB	257	178	0.02%	0.003%
18	3.667	813	817	822	rVB2	134	127	0.01%	0.002%
19	3.699	822	827	831	rVB	331	270	0.03%	0.004%
20	3.735	831	838	840	rBV	108	103	0.01%	0.002%
21	3.796	845	857	904	rBV2	122417	421216	45.05%	6.144%
22	4.249	982	998	1028	rBV	164906	432381	46.25%	6.306%
23	4.725	1143	1146	1148	rBV2	269	157	0.02%	0.002%
24	4.741	1148	1151	1152	rBV	342	170	0.02%	0.002%
25	4.879	1193	1194	1196	rBV	216	103	0.01%	0.002%
26	4.953	1202	1217	1230	rBV3	340511	934899	100.00%	13.636%
27	5.330	1332	1334	1336	rBV3	362	182	0.02%	0.003%
28	5.378	1347	1349	1355	rVB3	395	356	0.04%	0.005%
29	5.403	1355	1357	1362	rBV2	261	201	0.02%	0.003%
30	5.432	1362	1366	1368	rBV3	319	199	0.02%	0.003%
31	5.452	1369	1372	1374	rBV2	246	152	0.02%	0.002%
32	5.535	1388	1398	1428	rBV	181122	394305	42.18%	5.751%
33	5.838	1482	1492	1508	rBV5	5777	13704	1.47%	0.200%
34	5.989	1526	1539	1572	rBV	238921	505772	54.10%	7.377%
35	6.252	1618	1621	1625	rBV4	431	341	0.04%	0.005%
36	6.284	1628	1631	1634	rBV2	432	371	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035337.D
 Acq On : 22 Apr 2024 16:48
 Operator : SY/MD
 Sample : P2158-10DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.407	1666	1669	1670	rBV2	240	109	0.01%	0.002%
38	6.432	1675	1677	1679	rBV2	304	147	0.02%	0.002%
39	6.484	1689	1693	1696	rBV2	247	213	0.02%	0.003%
40	6.503	1696	1699	1702	rVV2	453	205	0.02%	0.003%
41	6.519	1702	1704	1710	rVB	266	178	0.02%	0.003%
42	6.561	1715	1717	1720	rBV	162	106	0.01%	0.002%
43	6.616	1731	1734	1739	rBV	242	244	0.03%	0.004%
44	6.754	1772	1777	1778	rBV2	564	364	0.04%	0.005%
45	6.825	1797	1799	1801	rVV	247	125	0.01%	0.002%
46	6.850	1805	1807	1809	rBV2	199	113	0.01%	0.002%
47	6.918	1817	1828	1863	rBV	76125	162667	17.40%	2.373%
48	7.159	1901	1903	1905	rBV	472	219	0.02%	0.003%
49	7.246	1920	1930	1960	rBV	204387	375327	40.15%	5.474%
50	7.558	2018	2027	2048	rBV	57100	113452	12.14%	1.655%
51	7.847	2113	2117	2121	rVB3	243	201	0.02%	0.003%
52	7.902	2131	2134	2138	rVB4	406	272	0.03%	0.004%
53	7.985	2154	2160	2164	rBV3	244	342	0.04%	0.005%
54	8.027	2164	2173	2228	rBV2	304796	749140	80.13%	10.927%
55	8.625	2357	2359	2360	rBV	391	107	0.01%	0.002%
56	8.680	2373	2376	2381	rVB2	400	326	0.03%	0.005%
57	8.706	2381	2384	2387	rBV2	351	273	0.03%	0.004%
58	8.744	2392	2396	2397	rBV3	473	317	0.03%	0.005%
59	8.786	2398	2409	2411	rBV	284625	350767	37.52%	5.116%
60	9.117	2509	2512	2515	rVB2	509	266	0.03%	0.004%
61	9.143	2515	2520	2522	rBV4	450	362	0.04%	0.005%
62	9.159	2523	2525	2530	rVB3	330	263	0.03%	0.004%
63	9.204	2537	2539	2541	rBV	230	124	0.01%	0.002%
64	9.220	2541	2544	2546	rBV2	321	213	0.02%	0.003%
65	9.233	2546	2548	2553	rVB2	420	312	0.03%	0.005%
66	9.278	2559	2562	2564	rBV2	318	213	0.02%	0.003%
67	9.310	2569	2572	2575	rBV2	388	337	0.04%	0.005%
68	9.336	2578	2580	2586	rVB2	382	250	0.03%	0.004%
69	9.452	2612	2616	2619	rBV	405	311	0.03%	0.005%
70	9.503	2629	2632	2635	rBV3	280	196	0.02%	0.003%
71	9.532	2639	2641	2644	rVB3	315	191	0.02%	0.003%
72	9.654	2675	2679	2683	rBV3	327	313	0.03%	0.005%
73	9.744	2705	2707	2710	rVB2	216	112	0.01%	0.002%
74	9.908	2756	2758	2765	rVB2	485	358	0.04%	0.005%
75	9.940	2765	2768	2769	rBV	206	110	0.01%	0.002%
76	10.008	2785	2789	2793	rVB4	322	261	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035337.D
 Acq On : 22 Apr 2024 16:48
 Operator : SY/MD
 Sample : P2158-10DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.072	2806	2809	2811	rBV	225	169	0.02%	0.002%
78	10.149	2822	2833	2855	rBV	461318	720903	77.11%	10.515%
79	10.336	2887	2891	2894	rBV2	365	312	0.03%	0.005%
80	10.397	2908	2910	2913	rVB2	321	139	0.01%	0.002%
81	10.500	2939	2942	2944	rBV2	261	183	0.02%	0.003%
82	10.593	2968	2971	2976	rVB2	299	243	0.03%	0.004%
83	10.628	2978	2982	2985	rBV2	164	138	0.01%	0.002%
84	10.680	2995	2998	2999	rBV	283	160	0.02%	0.002%
85	10.808	3036	3038	3042	rBV	179	140	0.01%	0.002%
86	10.873	3055	3058	3060	rBV	243	153	0.02%	0.002%
87	10.918	3069	3072	3073	rBV	254	155	0.02%	0.002%
88	10.982	3089	3092	3099	rVB3	328	366	0.04%	0.005%
89	11.124	3127	3136	3145	rBV2	18706	30636	3.28%	0.447%
90	11.185	3146	3155	3159	rBV	204132	299237	32.01%	4.365%
91	11.564	3261	3273	3301	rBV3	321553	779045	83.33%	11.363%
92	12.223	3474	3478	3482	rBV2	357	299	0.03%	0.004%
93	12.271	3491	3493	3497	rBV	285	196	0.02%	0.003%
94	12.336	3511	3513	3515	rBV	326	184	0.02%	0.003%
95	12.590	3590	3592	3594	rBV2	535	247	0.03%	0.004%
96	12.876	3676	3681	3684	rBV2	310	329	0.04%	0.005%
97	13.095	3747	3749	3751	rBV	419	208	0.02%	0.003%
98	13.197	3772	3781	3800	rBV2	84724	137206	14.68%	2.001%
99	13.538	3884	3887	3890	rBV2	510	382	0.04%	0.006%
100	13.683	3922	3932	3946	rBV3	30228	48959	5.24%	0.714%

Sum of corrected areas: 6856143




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035337.D
Acq On : 22 Apr 2024 16:48
Operator : SY/MD
Sample : P2158-10DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

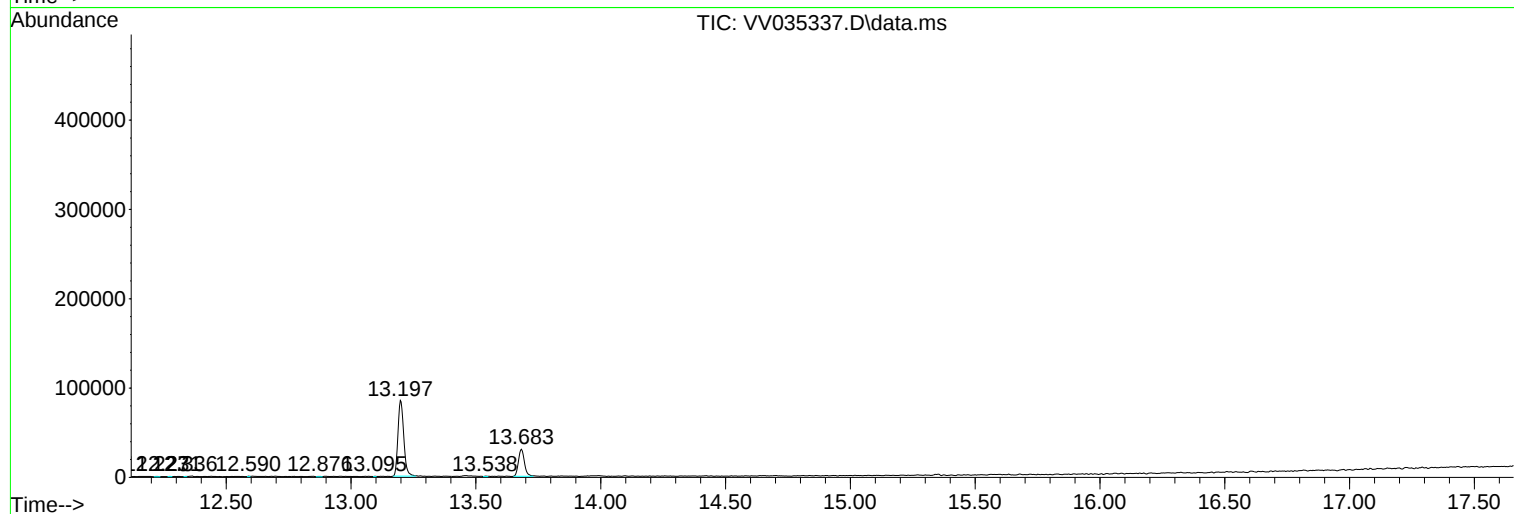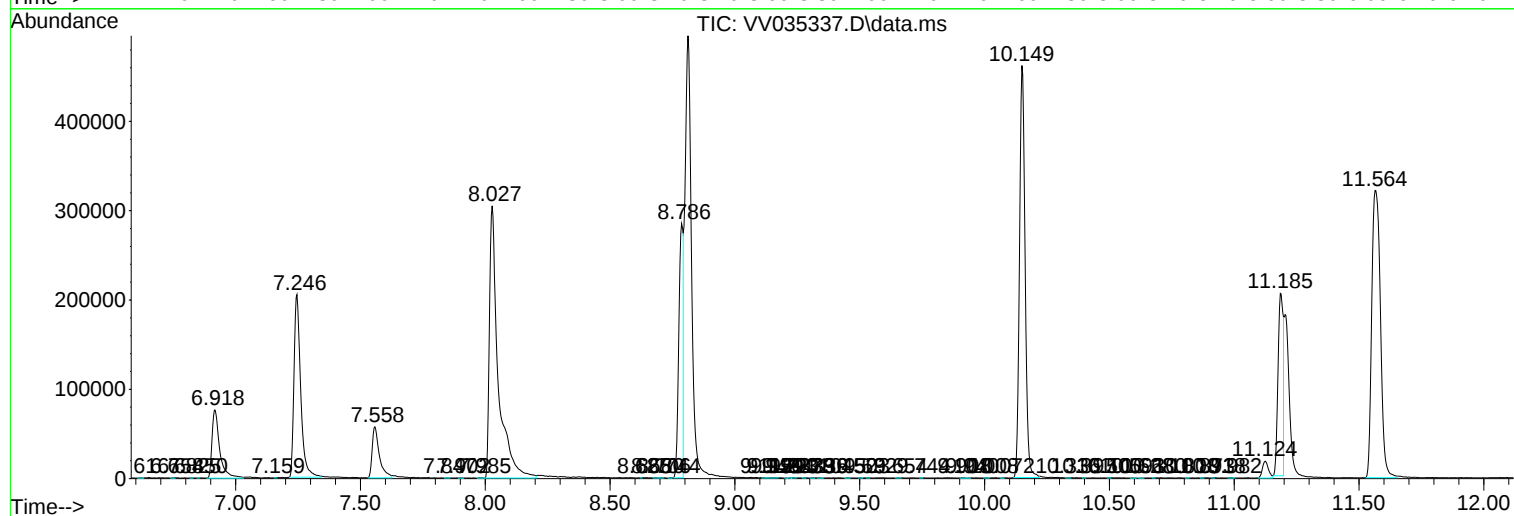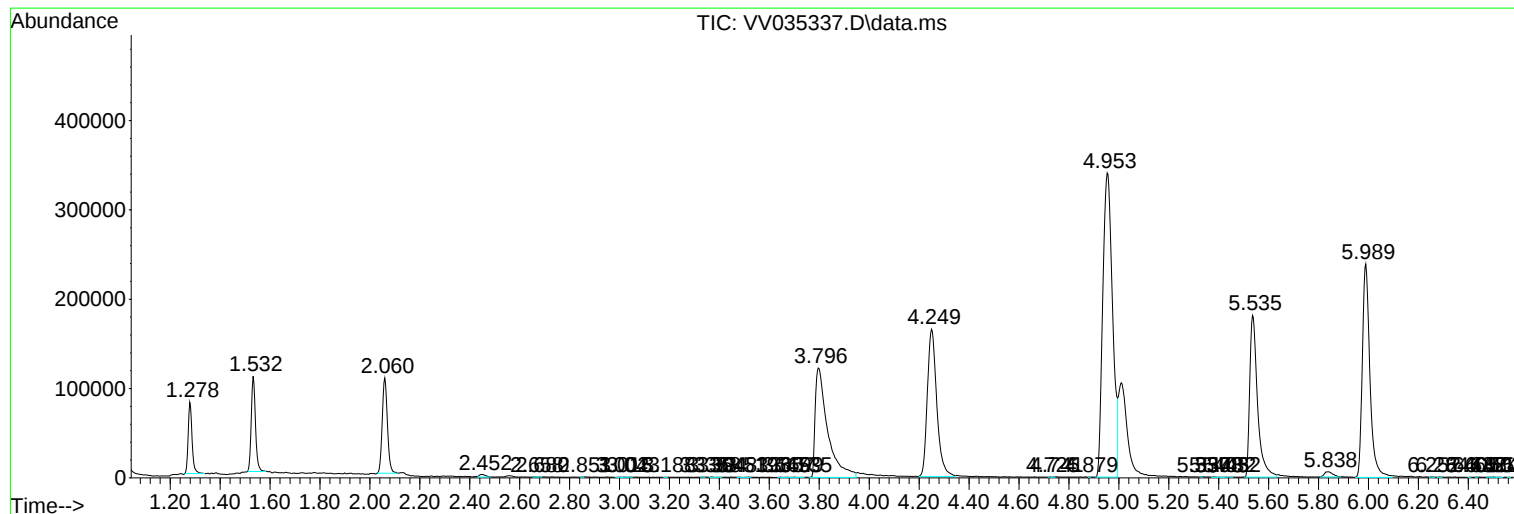

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035337.D
Acq On : 22 Apr 2024 16:48
Operator : SY/MD
Sample : P2158-10DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035337.D
Acq On : 22 Apr 2024 16:48
Operator : SY/MD
Sample : P2158-10DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc