

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035341.D
 Acq On : 22 Apr 2024 18:21
 Operator : SY/MD
 Sample : P2158-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	48	54	59	rBV	4598	5685	0.37%	0.049%
2	1.278	67	74	90	rBV	173641	187071	12.15%	1.598%
3	1.532	145	153	168	rBV	172763	204247	13.26%	1.745%
4	2.060	307	317	336	rBV	313785	453880	29.47%	3.877%
5	2.240	369	373	378	rBV2	551	534	0.03%	0.005%
6	2.388	416	419	424	rBV5	393	306	0.02%	0.003%
7	2.452	430	439	448	rVB5	1930	3232	0.21%	0.028%
8	2.497	448	453	459	rBV3	424	488	0.03%	0.004%
9	2.535	461	465	467	rBV3	333	254	0.02%	0.002%
10	2.642	492	498	502	rVB3	525	556	0.04%	0.005%
11	2.670	502	507	508	rBV	380	240	0.02%	0.002%
12	2.963	594	598	601	rVB2	291	238	0.02%	0.002%
13	3.719	830	833	836	rBV3	268	237	0.02%	0.002%
14	3.796	848	857	906	rBV	108555	357252	23.19%	3.051%
15	4.246	981	997	1029	rBV	249285	647519	42.04%	5.531%
16	4.542	1087	1089	1094	rVB3	351	224	0.01%	0.002%
17	4.690	1127	1135	1138	rBV4	531	621	0.04%	0.005%
18	4.953	1202	1217	1261	rBV2	570713	1540275	100.00%	13.156%
19	5.465	1372	1376	1379	rBV2	343	261	0.02%	0.002%
20	5.532	1386	1397	1435	rBV	436575	922704	59.91%	7.881%
21	5.838	1481	1492	1513	rVB4	8915	21253	1.38%	0.182%
22	5.985	1525	1538	1575	rBV	347375	734258	47.67%	6.272%
23	6.143	1585	1587	1593	rVB7	623	510	0.03%	0.004%
24	6.301	1633	1636	1641	rVB4	376	315	0.02%	0.003%
25	6.333	1641	1646	1649	rBV2	471	466	0.03%	0.004%
26	6.387	1661	1663	1673	rVB2	441	528	0.03%	0.005%
27	6.497	1691	1697	1701	rBV2	283	284	0.02%	0.002%
28	6.645	1738	1743	1747	rBV3	481	514	0.03%	0.004%
29	6.667	1747	1750	1755	rVV3	298	252	0.02%	0.002%
30	6.789	1784	1788	1791	rBV3	418	347	0.02%	0.003%
31	6.915	1816	1827	1861	rBV	126631	257183	16.70%	2.197%
32	7.185	1909	1911	1913	rBV3	426	230	0.01%	0.002%
33	7.243	1917	1929	1964	rBV	623637	1120796	72.77%	9.573%
34	7.555	2017	2026	2048	rBV	90134	169056	10.98%	1.444%
35	7.738	2077	2083	2084	rBV4	509	558	0.04%	0.005%
36	7.831	2105	2112	2116	rBV3	750	629	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035341.D
 Acq On : 22 Apr 2024 18:21
 Operator : SY/MD
 Sample : P2158-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	7.879	2116	2127	2137	rVB3	2218	3534	0.23%	0.030%
38	8.027	2163	2173	2220	rBV2	307734	760623	49.38%	6.497%
39	8.458	2305	2307	2311	rVB3	318	219	0.01%	0.002%
40	8.522	2325	2327	2330	rBV2	527	362	0.02%	0.003%
41	8.554	2335	2337	2340	rVB2	486	255	0.02%	0.002%
42	8.577	2340	2344	2347	rBV2	472	365	0.02%	0.003%
43	8.625	2354	2359	2361	rBV2	430	325	0.02%	0.003%
44	8.712	2383	2386	2390	rVB3	492	388	0.03%	0.003%
45	8.741	2390	2395	2397	rBV	377	310	0.02%	0.003%
46	8.783	2397	2408	2441	rBV	705952	1180312	76.63%	10.081%
47	9.185	2531	2533	2537	rVB3	335	221	0.01%	0.002%
48	9.300	2566	2569	2573	rBV3	431	273	0.02%	0.002%
49	9.400	2596	2600	2602	rVB2	397	250	0.02%	0.002%
50	9.448	2609	2615	2617	rBV	187	231	0.01%	0.002%
51	9.837	2732	2736	2742	rBV2	241	214	0.01%	0.002%
52	9.873	2742	2747	2749	rBV2	233	223	0.01%	0.002%
53	9.966	2771	2776	2780	rVB2	215	246	0.02%	0.002%
54	10.043	2798	2800	2806	rVB3	262	247	0.02%	0.002%
55	10.149	2821	2833	2861	rBV	538670	851675	55.29%	7.274%
56	10.320	2880	2886	2897	rVB3	4066	6548	0.43%	0.056%
57	10.490	2937	2939	2943	rVB3	372	233	0.02%	0.002%
58	10.519	2943	2948	2950	rBV	391	243	0.02%	0.002%
59	10.612	2976	2977	2982	rVB	427	239	0.02%	0.002%
60	10.789	3029	3032	3035	rBV	335	268	0.02%	0.002%
61	10.998	3092	3097	3100	rVV2	499	399	0.03%	0.003%
62	11.127	3130	3137	3144	rBV4	3691	5419	0.35%	0.046%
63	11.181	3144	3154	3180	rBV	641612	1025949	66.61%	8.763%
64	11.448	3235	3237	3243	rBV3	441	488	0.03%	0.004%
65	11.484	3246	3248	3252	rVB2	458	353	0.02%	0.003%
66	11.558	3258	3271	3299	rBV	697889	1119498	72.68%	9.562%
67	11.799	3344	3346	3349	rVB2	535	214	0.01%	0.002%
68	11.869	3366	3368	3371	rBV	363	250	0.02%	0.002%
69	11.911	3379	3381	3388	rBV4	338	365	0.02%	0.003%
70	11.943	3388	3391	3394	rVV	304	210	0.01%	0.002%
71	11.972	3397	3400	3405	rVB	760	557	0.04%	0.005%
72	12.005	3405	3410	3413	rBV2	408	393	0.03%	0.003%
73	12.120	3442	3446	3448	rBV2	302	221	0.01%	0.002%
74	12.191	3464	3468	3478	rVB3	775	1179	0.08%	0.010%
75	12.287	3494	3498	3502	rBV3	384	271	0.02%	0.002%
76	12.339	3512	3514	3517	rBV	354	252	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035341.D
 Acq On : 22 Apr 2024 18:21
 Operator : SY/MD
 Sample : P2158-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	12.355	3517	3519	3521	rVV	434	212	0.01%	0.002%
78	12.516	3563	3569	3577	rBV2	538	743	0.05%	0.006%
79	12.603	3588	3596	3597	rBV4	707	952	0.06%	0.008%
80	12.702	3624	3627	3632	rBV3	320	314	0.02%	0.003%
81	12.789	3651	3654	3656	rBV2	333	268	0.02%	0.002%
82	12.821	3660	3664	3668	rVB2	648	488	0.03%	0.004%
83	12.988	3713	3716	3719	rVB	290	222	0.01%	0.002%
84	13.075	3740	3743	3749	rVB2	359	340	0.02%	0.003%
85	13.201	3772	3782	3797	rVV2	47527	76058	4.94%	0.650%
86	13.323	3816	3820	3823	rBV4	389	370	0.02%	0.003%
87	13.387	3837	3840	3844	rBV2	410	325	0.02%	0.003%
88	13.564	3893	3895	3900	rVB	376	232	0.02%	0.002%
89	13.590	3900	3903	3905	rBV3	420	229	0.01%	0.002%
90	13.683	3923	3932	3945	rVV	16534	26106	1.69%	0.223%
91	13.840	3978	3981	3983	rBV2	421	279	0.02%	0.002%
92	13.975	4019	4023	4027	rBV3	582	470	0.03%	0.004%
93	14.001	4027	4031	4034	rBV4	704	523	0.03%	0.004%
94	14.056	4044	4048	4053	rBV3	776	660	0.04%	0.006%
95	14.082	4054	4056	4059	rBV2	501	319	0.02%	0.003%
96	14.220	4096	4099	4102	rBV3	421	297	0.02%	0.003%
97	14.316	4127	4129	4131	rBV2	377	227	0.01%	0.002%
98	14.802	4278	4280	4284	rBV3	552	456	0.03%	0.004%
99	14.934	4317	4321	4325	rBV	536	468	0.03%	0.004%
100	14.988	4336	4338	4342	rBV3	473	388	0.03%	0.003%




Sum of corrected areas: 11707771

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035341.D
Acq On : 22 Apr 2024 18:21
Operator : SY/MD
Sample : P2158-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

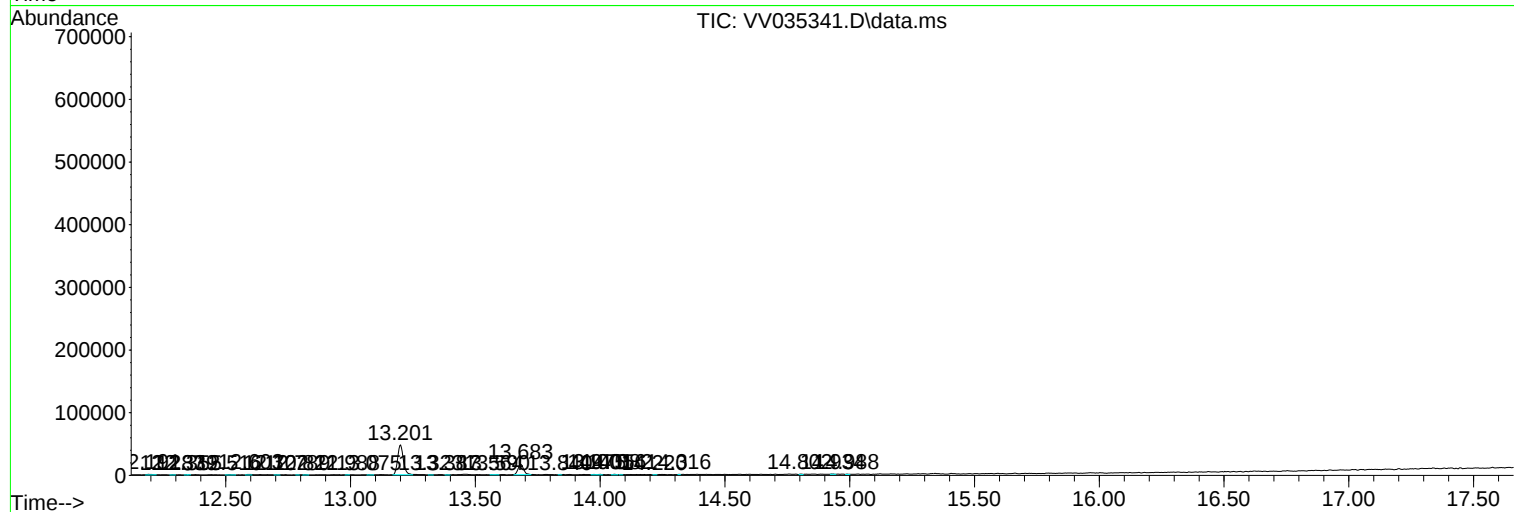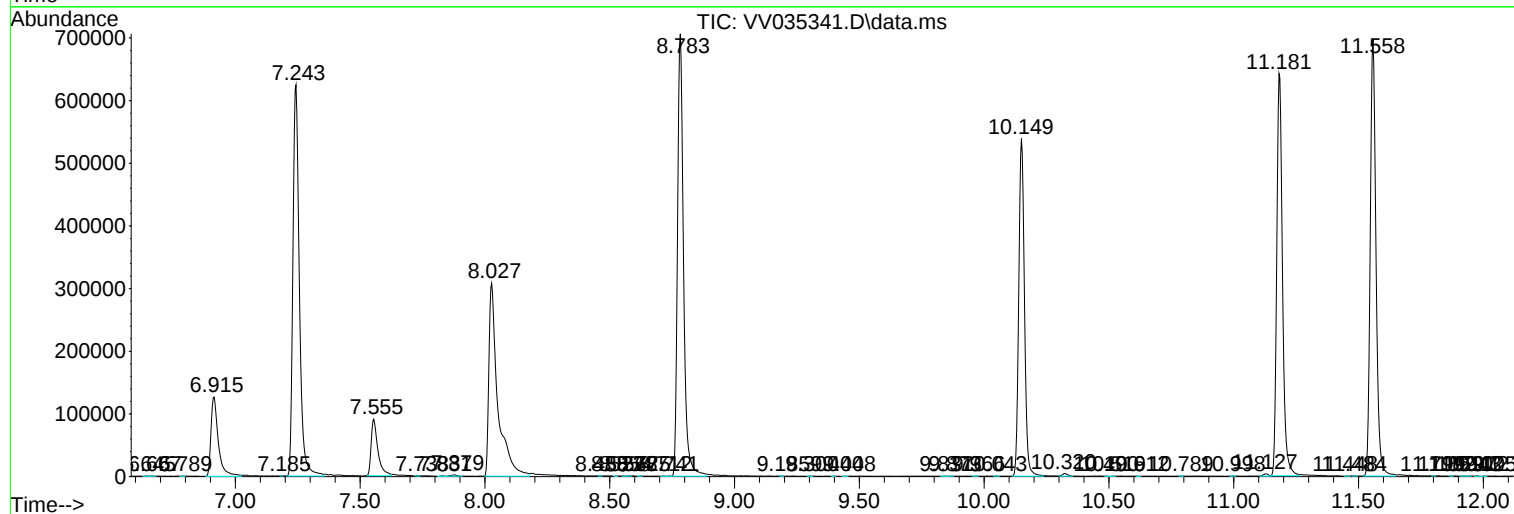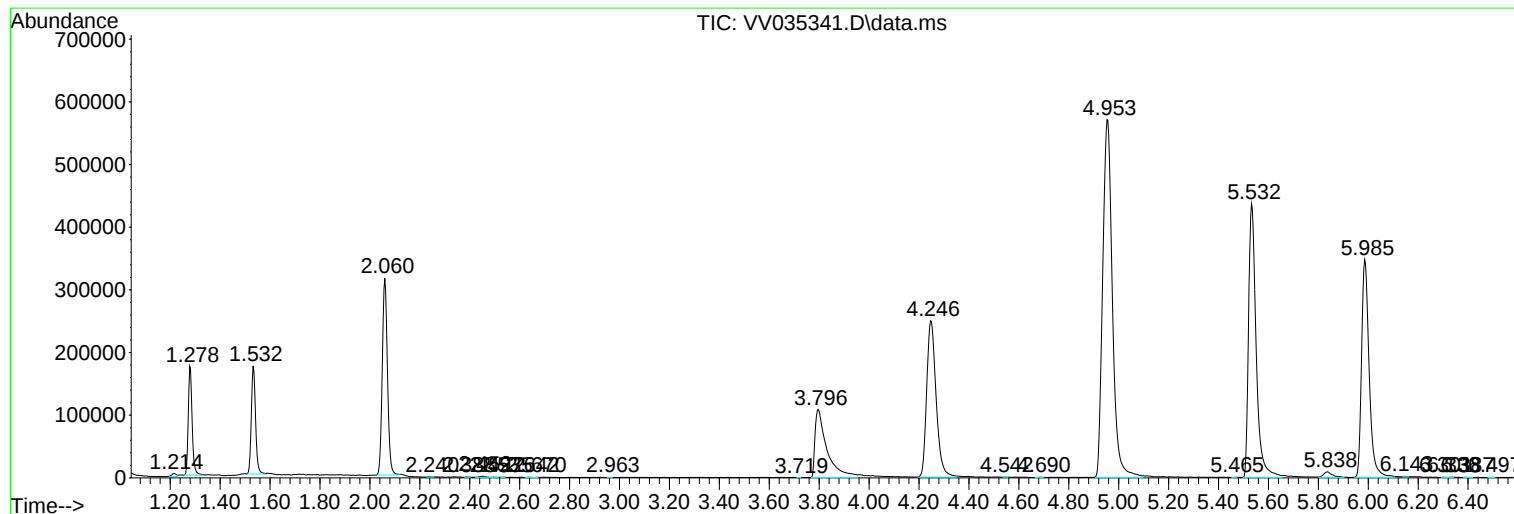

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035341.D
Acq On : 22 Apr 2024 18:21
Operator : SY/MD
Sample : P2158-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035341.D
Acq On : 22 Apr 2024 18:21
Operator : SY/MD
Sample : P2158-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
