

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035343.D
 Acq On : 22 Apr 2024 19:07
 Operator : SY/MD
 Sample : P2157-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035343.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	151068	162815	11.31%	1.538%
2	1.532	147	153	169	rVB	158028	184731	12.84%	1.745%
3	2.060	308	317	331	rBV	264978	382931	26.61%	3.617%
4	2.484	447	449	453	rBV2	449	425	0.03%	0.004%
5	2.526	461	462	464	rBV	221	58	0.00%	0.001%
6	2.539	464	466	468	rBV2	531	233	0.02%	0.002%
7	2.551	468	470	472	rBV2	276	131	0.01%	0.001%
8	2.622	488	492	494	rBV3	507	312	0.02%	0.003%
9	2.670	506	507	510	rBV	248	141	0.01%	0.001%
10	2.857	562	565	567	rBV2	219	119	0.01%	0.001%
11	2.892	572	576	580	rBV2	329	313	0.02%	0.003%
12	2.947	587	593	595	rBV	198	198	0.01%	0.002%
13	3.031	617	619	621	rBV2	103	47	0.00%	0.000%
14	3.082	630	635	639	rBV3	228	229	0.02%	0.002%
15	3.166	660	661	664	rBV	209	109	0.01%	0.001%
16	3.217	675	677	678	rVB	152	44	0.00%	0.000%
17	3.230	678	681	682	rBV2	90	49	0.00%	0.000%
18	3.265	691	692	693	rBV	162	37	0.00%	0.000%
19	3.278	695	696	697	rVB	192	40	0.00%	0.000%
20	3.310	704	706	707	rBV	109	44	0.00%	0.000%
21	3.346	715	717	718	rBV	157	51	0.00%	0.000%
22	3.394	730	732	736	rBV3	215	121	0.01%	0.001%
23	3.413	736	738	741	rBV2	332	185	0.01%	0.002%
24	3.432	741	744	750	rVB	216	147	0.01%	0.001%
25	3.461	750	753	754	rBV	104	58	0.00%	0.001%
26	3.526	770	773	775	rBV2	126	87	0.01%	0.001%
27	3.555	779	782	785	rVB2	272	207	0.01%	0.002%
28	3.632	803	806	807	rBV	144	74	0.01%	0.001%
29	3.796	848	857	891	rBV	110046	352099	24.47%	3.325%
30	4.249	982	998	1040	rBV	232712	605733	42.10%	5.721%
31	4.857	1183	1187	1191	rBV3	441	378	0.03%	0.004%
32	4.953	1201	1217	1260	rBV2	528924	1438943	100.00%	13.590%
33	5.481	1378	1381	1383	rBV2	197	155	0.01%	0.001%
34	5.532	1387	1397	1438	rVV	380400	808027	56.15%	7.631%
35	5.834	1482	1491	1516	rVB4	7733	19948	1.39%	0.188%
36	5.921	1516	1518	1520	rBV	166	72	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035343.D
 Acq On : 22 Apr 2024 19:07
 Operator : SY/MD
 Sample : P2157-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.985	1527	1538	1569	rBV	325345	684659	47.58%	6.466%
38	6.252	1620	1621	1624	rVB3	539	201	0.01%	0.002%
39	6.291	1630	1633	1637	rVB4	813	585	0.04%	0.006%
40	6.317	1637	1641	1647	rVB4	533	576	0.04%	0.005%
41	6.355	1651	1653	1658	rVB3	462	349	0.02%	0.003%
42	6.384	1658	1662	1665	rBV2	403	341	0.02%	0.003%
43	6.410	1668	1670	1673	rVB3	362	194	0.01%	0.002%
44	6.426	1673	1675	1676	rBV	172	76	0.01%	0.001%
45	6.448	1680	1682	1685	rBV	162	80	0.01%	0.001%
46	6.471	1687	1689	1694	rVB2	335	161	0.01%	0.002%
47	6.542	1708	1711	1713	rBV2	94	56	0.00%	0.001%
48	6.551	1713	1714	1715	rVB	132	25	0.00%	0.000%
49	6.596	1724	1728	1730	rBV	378	240	0.02%	0.002%
50	6.622	1733	1736	1739	rVV3	589	387	0.03%	0.004%
51	6.648	1741	1744	1746	rVV3	405	235	0.02%	0.002%
52	6.690	1755	1757	1760	rBV	354	208	0.01%	0.002%
53	6.815	1791	1796	1800	rBV	298	265	0.02%	0.003%
54	6.834	1800	1802	1803	rBV	115	55	0.00%	0.001%
55	6.915	1817	1827	1860	rBV2	117931	238739	16.59%	2.255%
56	7.101	1883	1885	1890	rVB3	561	265	0.02%	0.003%
57	7.172	1905	1907	1912	rVB5	544	405	0.03%	0.004%
58	7.243	1917	1929	1968	rBV	547507	980510	68.14%	9.261%
59	7.554	2017	2026	2054	rBV	83814	161876	11.25%	1.529%
60	7.853	2118	2119	2120	rBV	386	143	0.01%	0.001%
61	7.950	2147	2149	2151	rVB	342	90	0.01%	0.001%
62	7.992	2161	2162	2163	rBV	157	54	0.00%	0.001%
63	8.027	2163	2173	2209	rBV2	313877	780615	54.25%	7.373%
64	8.654	2364	2368	2369	rBV	440	334	0.02%	0.003%
65	8.715	2384	2387	2392	rVB2	323	214	0.01%	0.002%
66	8.738	2392	2394	2397	rVB	274	107	0.01%	0.001%
67	8.783	2397	2408	2439	rBV	599900	1026337	71.33%	9.693%
68	9.107	2506	2509	2511	rBB	473	187	0.01%	0.002%
69	9.204	2538	2539	2541	rBV	211	107	0.01%	0.001%
70	9.271	2558	2560	2562	rBV	161	68	0.00%	0.001%
71	9.320	2572	2575	2576	rBV2	337	156	0.01%	0.001%
72	9.410	2601	2603	2606	rBV2	270	168	0.01%	0.002%
73	9.487	2625	2627	2629	rBV	181	73	0.01%	0.001%
74	9.513	2633	2635	2638	rBV3	307	177	0.01%	0.002%
75	9.590	2656	2659	2660	rBV	253	113	0.01%	0.001%
76	9.625	2667	2670	2671	rBV	209	101	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
 Data File : VV035343.D
 Acq On : 22 Apr 2024 19:07
 Operator : SY/MD
 Sample : P2157-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.702	2691	2694	2698	rVB	198	109	0.01%	0.001%
78	9.725	2698	2701	2706	rBV2	303	179	0.01%	0.002%
79	9.850	2737	2740	2743	rVB2	583	350	0.02%	0.003%
80	9.863	2743	2744	2745	rBV2	201	66	0.00%	0.001%
81	10.011	2786	2790	2791	rBV	215	135	0.01%	0.001%
82	10.046	2798	2801	2802	rBV	305	189	0.01%	0.002%
83	10.149	2821	2833	2859	rBV	540435	848714	58.98%	8.016%
84	10.323	2879	2887	2892	rBV3	1397	1845	0.13%	0.017%
85	10.535	2950	2953	2956	rVB	364	225	0.02%	0.002%
86	10.599	2966	2973	2975	rBV2	297	334	0.02%	0.003%
87	10.673	2994	2996	2997	rBV	198	65	0.00%	0.001%
88	10.947	3079	3081	3082	rBV	178	79	0.01%	0.001%
89	11.130	3132	3138	3143	rBV5	2442	3077	0.21%	0.029%
90	11.185	3144	3155	3187	rVV	545044	886446	61.60%	8.372%
91	11.558	3256	3271	3298	rBV	607373	986972	68.59%	9.322%
92	12.024	3414	3416	3419	rBV2	218	158	0.01%	0.001%
93	12.117	3440	3445	3448	rBV3	498	476	0.03%	0.004%
94	12.435	3542	3544	3547	rVB	361	168	0.01%	0.002%
95	12.863	3673	3677	3680	rBV2	411	338	0.02%	0.003%
96	13.072	3740	3742	3743	rBV2	241	89	0.01%	0.001%
97	13.204	3775	3783	3793	rBV3	10130	16024	1.11%	0.151%
98	13.689	3927	3934	3942	rVB6	2006	3219	0.22%	0.030%




Sum of corrected areas: 10588080

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035343.D
Acq On : 22 Apr 2024 19:07
Operator : SY/MD
Sample : P2157-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

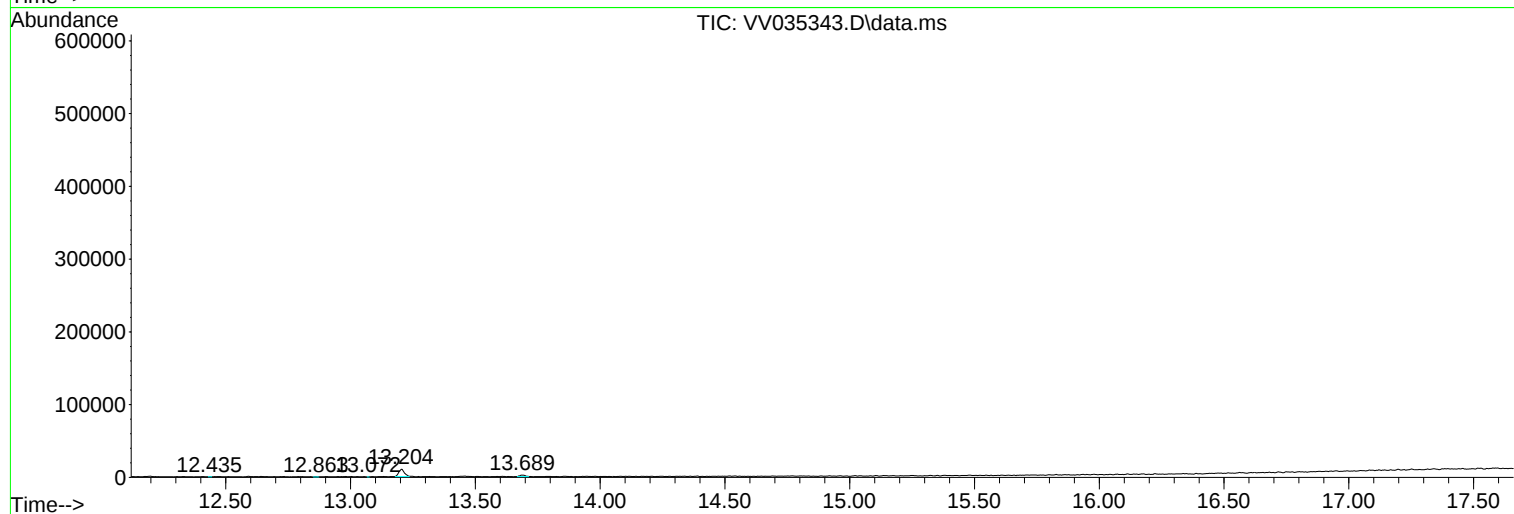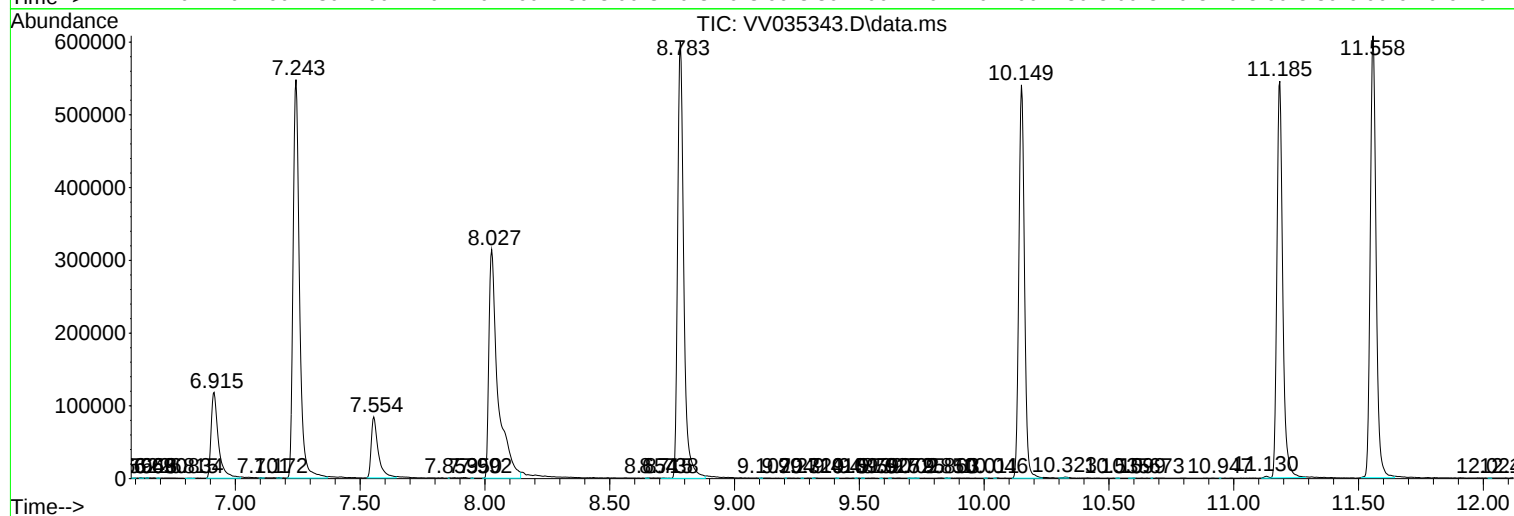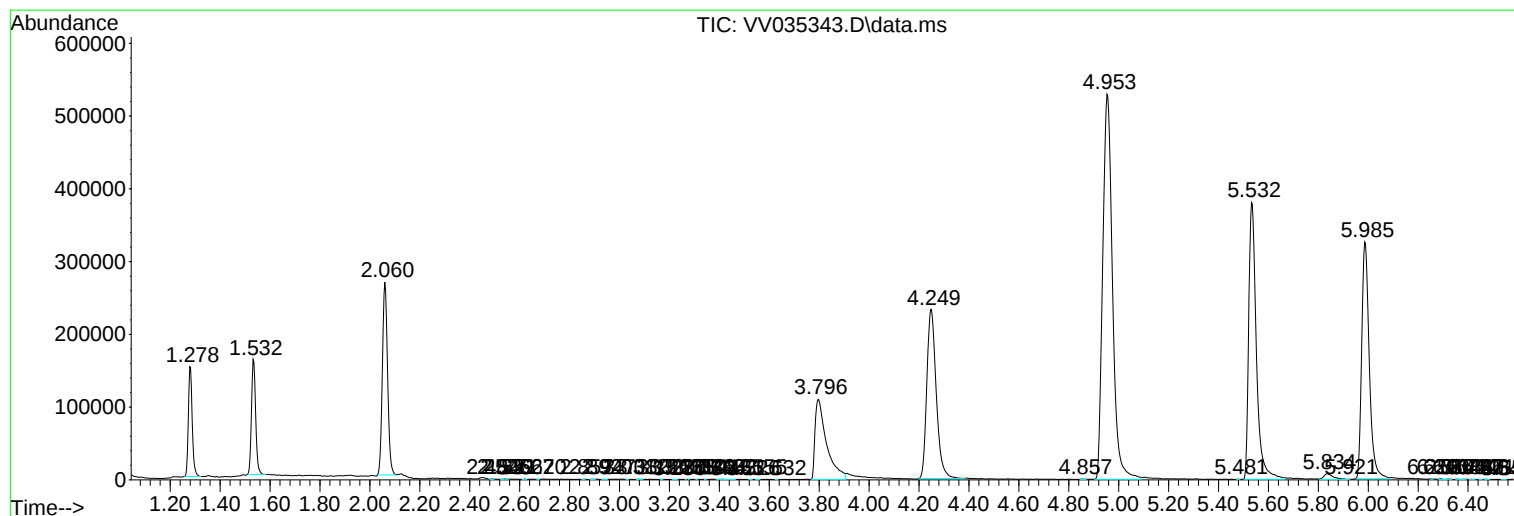

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035343.D
Acq On : 22 Apr 2024 19:07
Operator : SY/MD
Sample : P2157-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035343.D
Acq On : 22 Apr 2024 19:07
Operator : SY/MD
Sample : P2157-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc