


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042224\
Data File : VV035321.D
Acq On : 22 Apr 2024 08:50
Operator : SY/MD
Sample : BFB288
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB288

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis
Last Update : Fri Apr 26 01:37:05 2024

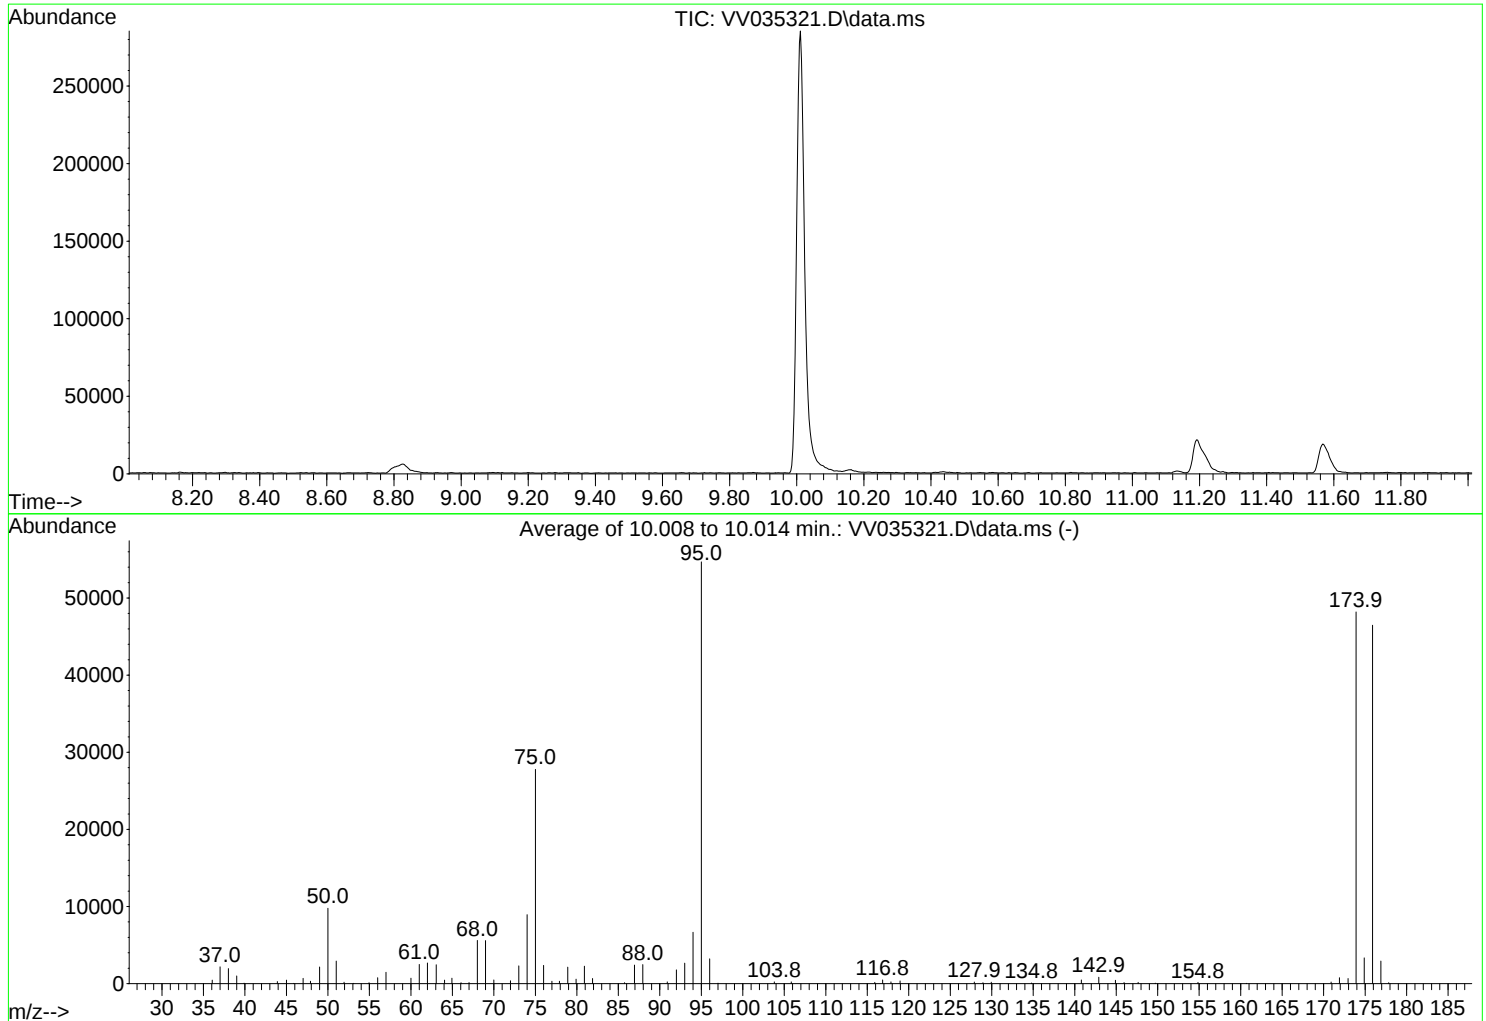

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	9769	PASS
75	95	30	80	50.8	27789	PASS
95	95	100	100	100.0	54691	PASS
96	95	5	9	5.9	3219	PASS
173	174	0.00	2	1.4	667	PASS
174	95	50	120	88.1	48200	PASS
175	174	5	9	6.9	3340	PASS
176	174	95	105	96.4	46480	PASS
177	176	5	10	6.3	2929	PASS

m/z	Abundance
39.90	199.0
43.90	394.0

Instrument :
MSVOA_V
ClientSampleId :
BFB288

m/z	Abundance
36.10	427.0
37.00	2315.0
38.00	2014.0
39.00	1021.0
40.00	272.0
43.90	670.0
45.00	484.0
45.90	109.0
47.00	759.0
47.90	350.0
49.00	2218.0
50.00	10067.0
51.00	2932.0
52.00	210.0
54.90	111.0
56.00	900.0
57.00	1513.0
60.00	728.0
61.00	2446.0
62.00	2747.0
63.00	2406.0
64.00	450.0
65.00	743.0
66.10	127.0
67.00	129.0
68.00	5737.0
69.00	5690.0
70.00	535.0
72.00	387.0
73.00	2347.0
74.00	9226.0
75.00	28384.0
76.00	2532.0
77.00	370.0
77.90	333.0
78.90	2145.0
79.90	602.0
80.90	2202.0
81.90	649.0
85.70	120.0
86.90	2620.0
88.00	2365.0
90.90	234.0
92.00	1890.0
93.00	2577.0
94.00	6395.0
95.00	55688.0
96.00	3350.0
103.80	242.0
105.80	240.0
115.90	139.0
116.90	464.0
117.90	234.0
118.90	388.0
127.90	199.0
129.00	144.0
130.00	232.0
134.80	135.0
140.80	469.0
142.90	824.0
144.90	411.0
146.00	155.0
147.70	134.0
154.80	162.0
170.90	214.0
171.90	743.0
172.90	659.0
173.90	47008.0
174.90	3280.0
175.90	45656.0
176.90	2994.0
177.90	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB288

m/z	Abundance
36.10	475.0
37.00	2249.0
38.00	1992.0
39.00	1004.0
39.90	261.0
43.90	674.0
45.00	472.0
47.00	692.0
47.90	328.0
49.00	2200.0
50.00	10027.0
51.00	3001.0
52.00	182.0
55.00	134.0
56.00	795.0
57.00	1498.0
60.00	748.0
61.00	2547.0
62.00	2713.0
63.00	2555.0
64.10	490.0
65.00	724.0
66.10	117.0
67.00	160.0
68.00	5838.0
69.00	5722.0
70.00	497.0
72.00	376.0
73.00	2375.0
74.00	9202.0
75.00	28768.0
76.00	2435.0
77.00	312.0
77.90	311.0
78.90	2175.0
79.90	596.0
80.90	2288.0
81.90	680.0
85.70	141.0
86.90	2451.0
87.90	2572.0
90.90	249.0
92.00	1888.0
93.00	2793.0
94.00	6861.0
95.00	56472.0
96.00	3317.0
97.00	105.0
103.80	253.0
105.80	219.0
115.90	153.0
116.90	484.0
117.80	240.0
118.90	372.0
127.90	207.0
128.90	134.0
130.00	189.0
134.80	123.0
140.80	480.0
142.90	872.0
144.90	470.0
145.90	145.0
147.70	184.0
149.70	103.0
154.90	157.0
160.70	102.0
170.90	223.0
171.90	766.0
172.90	691.0
173.90	49920.0
174.90	3460.0
175.90	47976.0
176.90	2984.0
177.80	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB288

m/z	Abundance
36.00	486.0
37.00	2004.0
38.00	1844.0
39.00	961.0
40.00	252.0
44.00	636.0
45.00	390.0
47.00	577.0
47.90	261.0
49.00	2039.0
50.00	9213.0
51.00	2836.0
51.90	156.0
53.10	128.0
55.00	151.0
56.00	636.0
57.00	1406.0
60.00	667.0
61.00	2497.0
62.00	2543.0
63.10	2407.0
64.00	449.0
64.90	643.0
66.00	103.0
67.00	171.0
68.00	5205.0
69.00	5337.0
70.00	387.0
72.00	334.0
73.00	2181.0
74.00	8392.0
75.00	26216.0
76.00	2115.0
77.00	269.0
77.90	288.0
78.90	2104.0
79.90	557.0
80.90	2289.0
81.90	651.0
85.80	135.0
87.00	2135.0
87.90	2453.0
90.90	221.0
92.00	1561.0
93.00	2570.0
94.00	6710.0
95.00	51912.0
96.00	2990.0
97.00	114.0
103.80	211.0
105.90	209.0
115.90	194.0
116.80	471.0
117.90	221.0
119.00	329.0
127.90	224.0
128.90	112.0
129.90	160.0
140.80	474.0
142.90	772.0
144.90	420.0
145.90	126.0
147.60	205.0
149.70	101.0
154.90	161.0
170.90	193.0
171.90	770.0
173.00	650.0
173.90	47672.0
174.90	3281.0
175.90	45808.0
176.90	2810.0
177.80	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB288