


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV042320\
 Data File : VV015650.D
 Acq On : 23 Apr 2020 09:35
 Operator : SY/MD
 Sample : BFB41
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB41

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Apr 24 03:28:15 2020

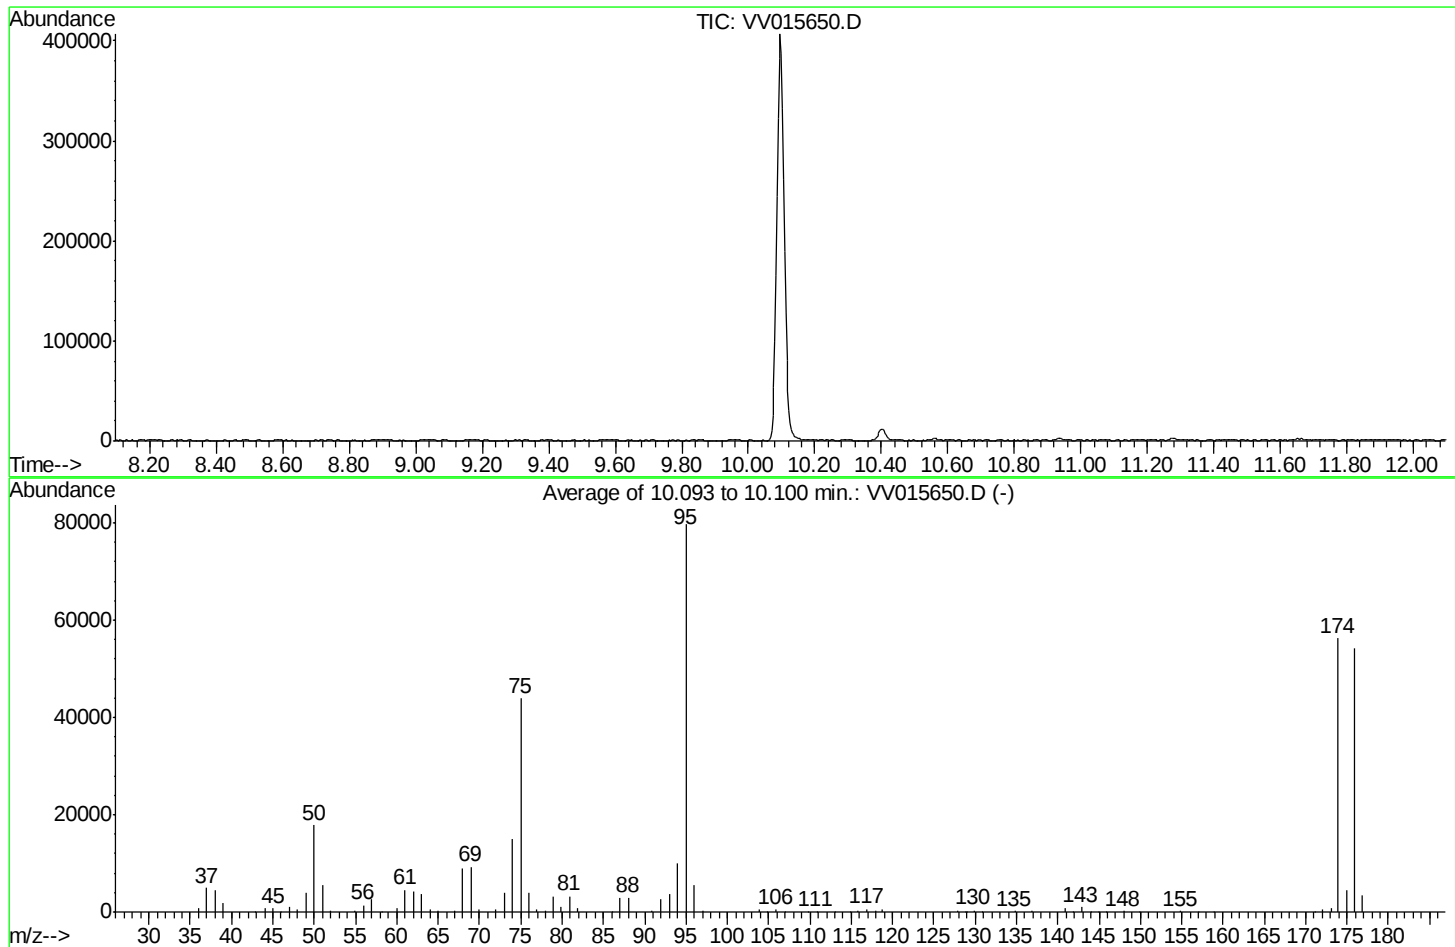

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	17810	PASS
75	95	30	80	55.0	43845	PASS
95	95	100	100	100.0	79669	PASS
96	95	5	9	6.9	5527	PASS
173	174	0.00	2	1.5	824	PASS
174	95	50	120	70.6	56226	PASS
175	174	5	9	7.8	4380	PASS
176	174	95	101	96.6	54306	PASS
177	176	5	9	6.5	3516	PASS

m/z	Abundance
35.90	766.0
37.00	4899.0
38.00	4541.0
39.00	1833.0
40.00	305.0
42.80	123.0
44.00	928.0
45.10	730.0
47.00	1000.0
48.00	601.0
49.00	4034.0
50.00	17416.0
51.00	5398.0
52.00	248.0
55.00	309.0
56.00	1423.0
57.00	2780.0
58.10	103.0
60.00	931.0
61.00	4565.0
62.00	4180.0
63.00	3599.0
64.00	497.0
65.00	360.0
67.00	272.0
68.00	8728.0
69.00	9134.0
70.00	672.0
72.00	606.0
73.00	3984.0
74.00	14852.0
75.00	42832.0
76.00	3833.0
76.90	403.0
77.90	327.0
78.90	3067.0
79.90	984.0
80.90	3122.0
81.90	686.0
86.90	2930.0
88.00	2708.0
90.90	363.0
92.00	2521.0
93.00	3543.0
94.00	9955.0
95.00	78192.0
96.00	5538.0
97.00	181.0
103.80	510.0
104.90	150.0
105.90	446.0
106.90	129.0
109.80	107.0
110.80	117.0
114.90	127.0
115.80	274.0
116.90	672.0
117.90	307.0
118.80	491.0
127.80	270.0
128.80	126.0
129.90	288.0
130.80	126.0
134.80	152.0
136.80	187.0
140.90	866.0
141.70	121.0
142.90	986.0
144.90	125.0
145.90	134.0
148.00	162.0
149.80	103.0
154.90	209.0
157.00	108.0
158.80	119.0
171.20	112.0
171.90	420.0
173.10	717.0
173.90	53424.0
175.00	4227.0
176.00	51944.0
176.90	3480.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

m/z	Abundance
35.90	781.0
37.00	5121.0
38.00	4710.0
39.00	1922.0
40.00	302.0
42.80	119.0
44.00	1007.0
45.00	769.0
47.00	1213.0
48.00	600.0
49.00	4028.0
50.00	18512.0
51.00	5556.0
52.00	253.0
55.00	278.0
56.00	1431.0
57.00	2679.0
60.00	948.0
61.00	4638.0
62.00	4500.0
63.00	3802.0
64.00	463.0
65.00	362.0
66.90	309.0
68.00	9237.0
69.00	9625.0
70.00	694.0
72.00	688.0
73.00	4148.0
74.00	15489.0
75.00	45560.0
76.00	3995.0
76.90	461.0
77.90	325.0
78.90	3176.0
79.90	1006.0
80.90	3366.0
81.90	712.0
86.00	130.0
87.00	2945.0
88.00	3036.0
90.90	385.0
92.00	2614.0
93.00	3766.0
94.00	10424.0
95.00	82656.0
96.00	5781.0
97.00	173.0
103.80	499.0
104.90	134.0
105.90	507.0
106.90	139.0
109.80	110.0
110.80	117.0
114.80	120.0
115.80	299.0
116.90	662.0
117.90	357.0
118.80	543.0
127.80	310.0
128.80	126.0
129.00	127.0
129.80	300.0
130.70	136.0
134.80	180.0
136.80	172.0
140.90	937.0
141.80	135.0
142.90	1013.0
144.90	142.0
145.80	126.0
148.00	202.0
149.80	123.0
154.90	219.0
157.10	139.0
158.80	133.0
171.10	122.0
171.90	449.0
173.10	854.0
173.90	58264.0
175.00	4579.0
176.00	56248.0
176.90	3614.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

m/z	Abundance
36.00	767.0
37.00	4771.0
38.00	4149.0
39.00	1781.0
40.00	307.0
42.90	106.0
44.00	996.0
45.00	794.0
46.00	106.0
47.00	1175.0
47.90	589.0
49.00	3658.0
50.00	17504.0
51.00	5292.0
52.00	243.0
54.90	235.0
56.00	1305.0
57.00	2404.0
60.00	885.0
61.00	4244.0
62.00	4281.0
63.00	3461.0
64.00	393.0
65.10	328.0
66.90	309.0
68.00	8820.0
69.00	8974.0
70.00	634.0
72.00	633.0
73.00	3846.0
74.00	14428.0
75.00	43144.0
76.00	3731.0
76.90	491.0
78.00	322.0
78.90	2946.0
79.90	889.0
80.90	3198.0
81.90	654.0
86.00	142.0
87.00	2734.0
88.00	2973.0
90.90	371.0
92.00	2534.0
93.00	3700.0
94.00	9856.0
95.00	78160.0
96.00	5262.0
97.10	175.0
103.80	444.0
104.80	107.0
105.90	505.0
107.00	109.0
110.80	111.0
113.00	109.0
114.70	143.0
115.90	331.0
116.90	641.0
117.90	370.0
118.80	537.0
127.90	312.0
129.00	137.0
129.80	318.0
130.70	132.0
134.80	177.0
136.80	141.0
140.90	908.0
141.80	126.0
142.90	986.0
144.00	106.0
144.90	150.0
148.00	208.0
149.80	121.0
154.90	193.0
157.00	158.0
158.80	131.0
171.10	115.0
172.00	449.0
173.10	903.0
174.00	56992.0
175.00	4334.0
175.90	54728.0
176.90	3456.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

Scan 2788 (10.055 min): VV015650.D
BFB41

m/z	Abundance
40.00	353.0
44.00	292.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41