

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021112.D
 Acq On : 23 Apr 2021 12:17
 Operator : SY/MD
 Sample : VV0423WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 24 03:43:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 24 03:42:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	688821	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	681055	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	313437	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.311	65	234509	41.43	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.86%
7) Chloroethane-d5	1.571	69	188223	45.20	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.40%
11) 1,1-Dichloroethene-d2	2.111	63	341061	32.67	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.34%
21) 2-Butanone-d5	3.896	46	273754	99.04	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.04%
24) Chloroform-d	4.352	84	468135	46.39	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.78%
26) 1,2-Dichloroethane-d4	5.037	65	324750	50.63	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.26%
32) Benzene-d6	5.053	84	874365	48.21	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.42%
36) 1,2-Dichloropropane-d6	6.072	67	268045	49.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.02%
41) Toluene-d8	7.320	98	809352	46.11	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.22%
43) trans-1,3-Dichloroprop...	7.625	79	139850	47.27	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.54%
47) 2-Hexanone-d5	8.095	63	219183	102.07	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	102.07%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	380610	46.61	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.22%
66) 1,2-Dichlorobenzene-d4	11.632	152	331465	53.54	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.08%
Target Compounds						
48) 2-Hexanone	8.095	43	23469	5.29	ug/L	Qvalue # 56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021112.D
Acq On : 23 Apr 2021 12:17
Operator : SY/MD
Sample : VV0423WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Apr 24 03:43:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 24 03:42:40 2021
Response via : Initial Calibration

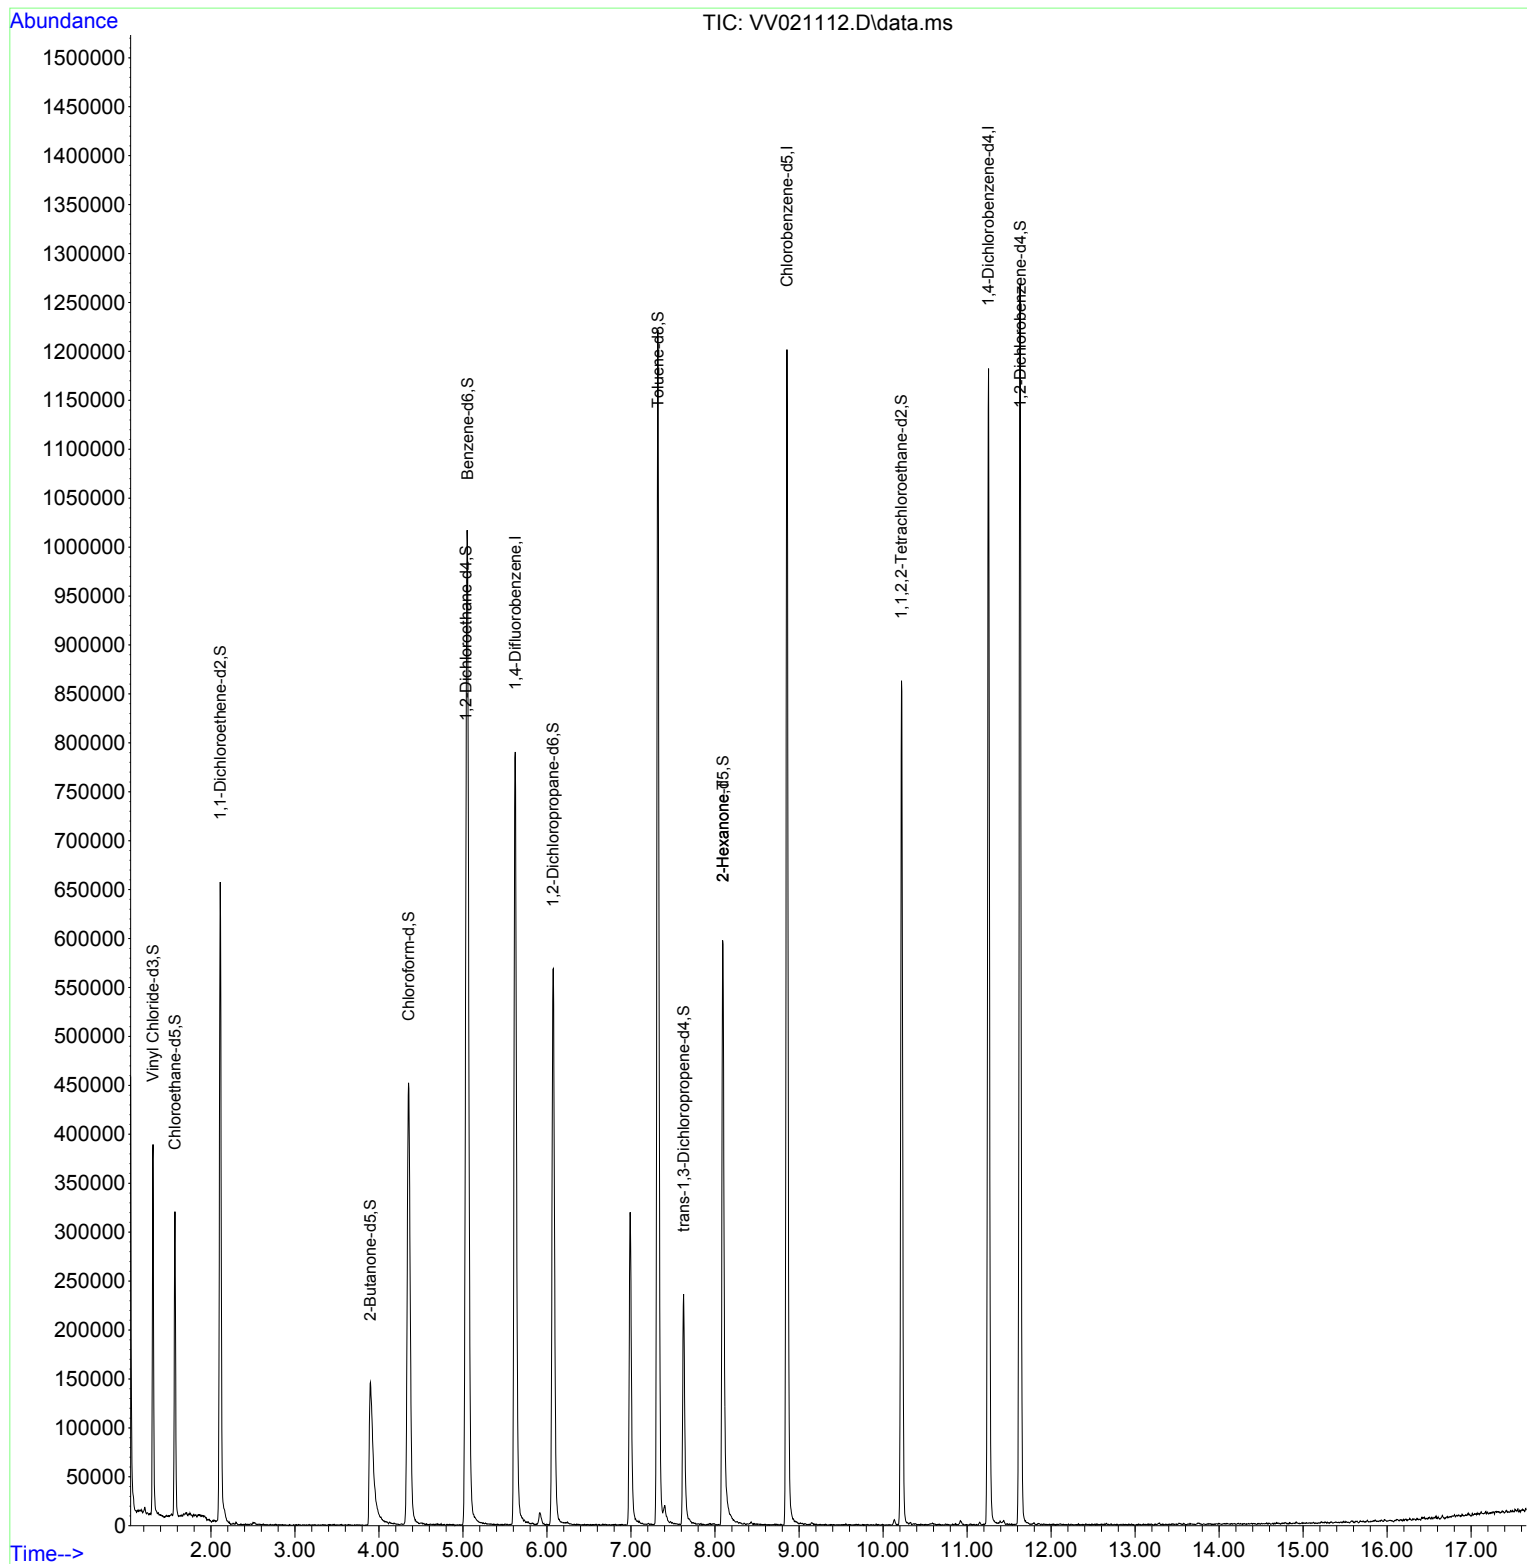

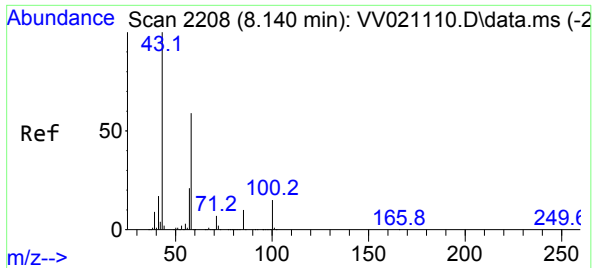

#48
2-Hexanone
Concen: 5.29 ug/L
RT: 8.095 min Scan# 2194
Delta R.T. -0.045 min
Lab File: VV021112.D
Acq: 23 Apr 2021 12:17

Instrument :
MSVOA_V
ClientSampleId :

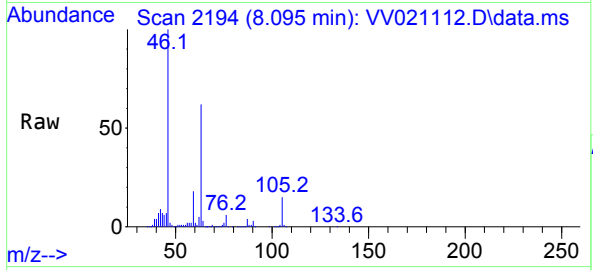

Tgt Ion: 43 Resp: 23469

Ion	Ratio	Lower	Upper
43	100		
58	18.1	46.8	70.2#
57	32.9	17.6	26.4#
100	1.2	12.0	18.0#

