

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021132.D
 Acq On : 23 Apr 2021 20:34
 Operator : SY/MD
 Sample : M2123-07 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 24 03:47:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 24 03:42:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	689163	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	671356	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	320674	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	169750	29.98	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	59.96%#		
7) Chloroethane-d5	1.571	69	143262	34.39	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	68.78%#		
11) 1,1-Dichloroethene-d2	2.108	63	266361	25.50	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	51.00%#		
21) 2-Butanone-d5	3.915	46	228605	82.67	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	82.67%		
24) Chloroform-d	4.352	84	393254	38.95	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	77.90%		
26) 1,2-Dichloroethane-d4	5.037	65	275122	42.87	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.74%		
32) Benzene-d6	5.053	84	694872	38.86	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	77.72%		
36) 1,2-Dichloropropane-d6	6.075	67	221743	41.55	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	83.10%		
41) Toluene-d8	7.320	98	637885	36.86	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	73.72%#		
43) trans-1,3-Dichloroprop...	7.625	79	111221	38.13	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	76.26%		
47) 2-Hexanone-d5	8.095	63	214645	101.40	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	101.40%		
56) 1,1,2,2-Tetrachloroeth...	10.220	84	342743	42.58	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	85.16%		
66) 1,2-Dichlorobenzene-d4	11.632	152	281669	44.47	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.94%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.625	75	6115	0.79	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021132.D
Acq On : 23 Apr 2021 20:34
Operator : SY/MD
Sample : M2123-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Apr 24 03:47:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 24 03:42:40 2021
Response via : Initial Calibration

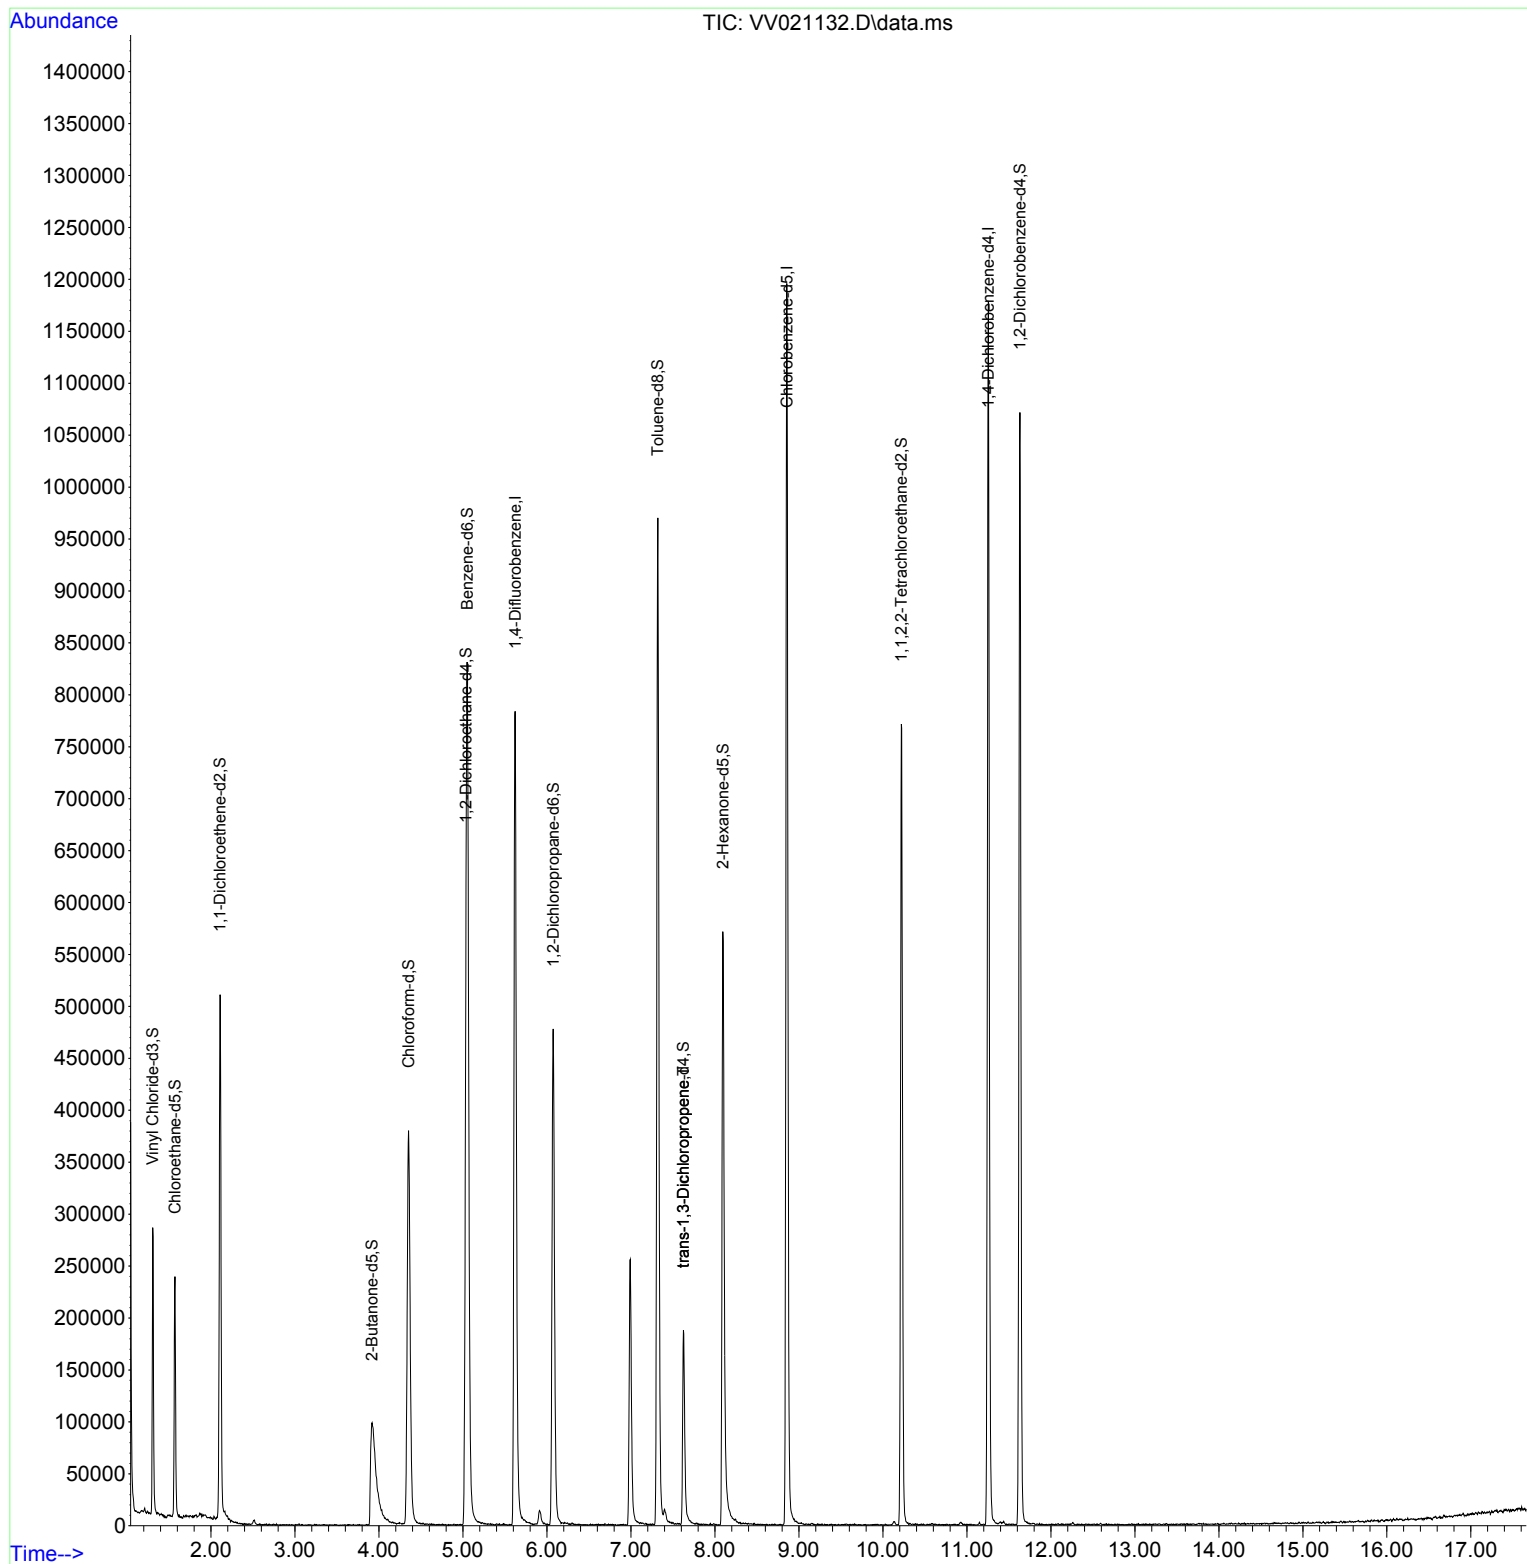

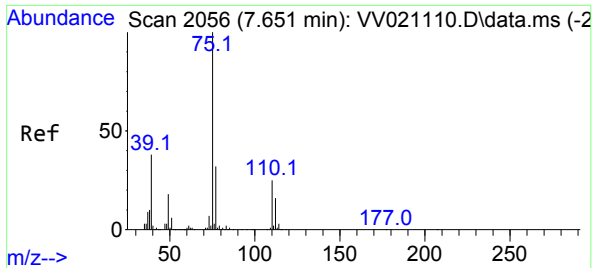

#44
trans-1,3-Dichloropropene
Concen: 0.79 ug/L
RT: 7.625 min Scan# 2048
Delta R.T. -0.026 min
Lab File: VV021132.D
Acq: 23 Apr 2021 20:34

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 75 Resp: 6115
Ion Ratio Lower Upper
75 100
77 39.1 21.8 40.6

