

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021111.D
 Acq On : 23 Apr 2021 11:54
 Operator : SY/MD
 Sample : VV0423MBL01
 Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK169

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021111.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	98	rBV	402844	421312	15.46%	2.016%
2	1.571	158	165	175	rBV	323201	360344	13.22%	1.725%
3	2.108	322	332	365	rVB	712103	1058546	38.84%	5.066%
4	2.349	405	407	410	rBV	818	391	0.01%	0.002%
5	2.510	452	457	464	rBV7	3235	3894	0.14%	0.019%
6	2.584	476	480	483	rBV3	1183	925	0.03%	0.004%
7	2.725	523	524	525	rBV	430	159	0.01%	0.001%
8	2.818	549	553	558	rBV3	1233	1182	0.04%	0.006%
9	2.841	558	560	562	rBV	419	198	0.01%	0.001%
10	2.931	586	588	590	rBV	346	231	0.01%	0.001%
11	2.941	590	591	592	rVV	399	104	0.00%	0.000%
12	3.098	638	640	645	rBV3	466	374	0.01%	0.002%
13	3.240	682	684	686	rBV	684	282	0.01%	0.001%
14	3.262	686	691	693	rBV3	635	575	0.02%	0.003%
15	3.310	702	706	709	rBV2	1059	718	0.03%	0.003%
16	3.326	709	711	713	rVV2	353	135	0.00%	0.001%
17	3.371	720	725	727	rBV2	425	401	0.01%	0.002%
18	3.404	732	735	738	rBV2	592	433	0.02%	0.002%
19	3.526	770	773	774	rBV	287	152	0.01%	0.001%
20	3.535	774	776	779	rVB2	887	380	0.01%	0.002%
21	3.648	809	811	816	rVB2	928	685	0.03%	0.003%
22	3.686	816	823	827	rBV3	1227	1435	0.05%	0.007%
23	3.725	833	835	840	rVB	622	389	0.01%	0.002%
24	3.748	840	842	844	rBV2	709	389	0.01%	0.002%
25	3.796	855	857	859	rBV2	444	218	0.01%	0.001%
26	3.818	861	864	867	rBV4	471	366	0.01%	0.002%
27	3.857	872	876	878	rBV2	664	463	0.02%	0.002%
28	3.899	878	889	925	rBV2	128692	489543	17.96%	2.343%
29	4.349	1014	1029	1057	rBV2	469395	1161780	42.62%	5.560%
30	4.657	1122	1125	1127	rBV	807	528	0.02%	0.003%
31	4.783	1161	1164	1166	rBV3	638	387	0.01%	0.002%
32	4.854	1184	1186	1189	rBV2	406	174	0.01%	0.001%
33	4.940	1210	1213	1216	rBV	887	556	0.02%	0.003%
34	5.047	1229	1246	1275	rBV2	1049253	2725599	100.00%	13.044%
35	5.490	1380	1384	1387	rVB3	1093	790	0.03%	0.004%
36	5.510	1387	1390	1394	rBV4	1072	669	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021111.D
 Acq On : 23 Apr 2021 11:54
 Operator : SY/MD
 Sample : VV0423MBL01
 Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK169

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	5.548	1400	1402	1406	rVB4	1266	715	0.03%	0.003%
38	5.616	1409	1423	1449	rBV	846066	1703707	62.51%	8.153%
39	6.069	1551	1564	1587	rBV	595511	1214629	44.56%	5.813%
40	6.352	1649	1652	1654	rBV2	994	575	0.02%	0.003%
41	6.429	1673	1676	1679	rBV3	753	571	0.02%	0.003%
42	6.474	1688	1690	1691	rBV	541	289	0.01%	0.001%
43	6.506	1696	1700	1703	rBV4	1461	1080	0.04%	0.005%
44	6.680	1752	1754	1758	rVB3	1028	562	0.02%	0.003%
45	6.699	1758	1760	1764	rBV3	757	497	0.02%	0.002%
46	6.789	1786	1788	1793	rBV2	756	722	0.03%	0.003%
47	6.863	1808	1811	1814	rBV2	694	462	0.02%	0.002%
48	6.940	1833	1835	1837	rBV2	774	346	0.01%	0.002%
49	6.985	1837	1849	1877	rBV	334770	624683	22.92%	2.990%
50	7.156	1898	1902	1905	rBV2	1165	918	0.03%	0.004%
51	7.204	1914	1917	1921	rBV3	1217	926	0.03%	0.004%
52	7.230	1924	1925	1927	rBV2	562	309	0.01%	0.001%
53	7.317	1940	1952	1970	rBV	1270632	2174551	79.78%	10.407%
54	7.622	2038	2047	2069	rBV	237119	416453	15.28%	1.993%
55	7.815	2104	2107	2111	rBV4	1096	1063	0.04%	0.005%
56	7.982	2157	2159	2164	rVB5	1814	1176	0.04%	0.006%
57	8.091	2183	2193	2234	rBV	601344	1100124	40.36%	5.265%
58	8.571	2337	2342	2344	rBV4	1468	938	0.03%	0.004%
59	8.722	2387	2389	2392	rBV	899	400	0.01%	0.002%
60	8.783	2406	2408	2410	rBV	629	364	0.01%	0.002%
61	8.853	2418	2430	2458	rBV	1251513	2049983	75.21%	9.811%
62	9.127	2512	2515	2518	rBV3	1213	895	0.03%	0.004%
63	9.149	2519	2522	2525	rVV4	2201	1571	0.06%	0.008%
64	9.390	2594	2597	2598	rBV	497	321	0.01%	0.002%
65	9.500	2629	2631	2634	rBV2	690	494	0.02%	0.002%
66	9.580	2654	2656	2657	rBV2	790	389	0.01%	0.002%
67	9.770	2713	2715	2717	rBV2	732	388	0.01%	0.002%
68	9.796	2721	2723	2725	rVB2	618	271	0.01%	0.001%
69	9.808	2725	2727	2729	rBV2	607	382	0.01%	0.002%
70	9.853	2739	2741	2743	rBV	456	141	0.01%	0.001%
71	10.001	2785	2787	2790	rBV3	943	547	0.02%	0.003%
72	10.040	2798	2799	2802	rBV2	509	195	0.01%	0.001%
73	10.220	2843	2855	2876	rBV	880048	1375726	50.47%	6.584%
74	10.480	2934	2936	2939	rBV2	765	418	0.02%	0.002%
75	10.709	3003	3007	3009	rBV2	626	521	0.02%	0.002%
76	10.921	3068	3073	3082	rVB7	5844	8056	0.30%	0.039%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021111.D
 Acq On : 23 Apr 2021 11:54
 Operator : SY/MD
 Sample : VV0423MBL01
 Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK169

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

77	11.027	3104	3106	3107	rBV	899	360	0.01%	0.002%
78	11.037	3107	3109	3115	rVB5	1340	1176	0.04%	0.006%
79	11.255	3165	3177	3196	rBV	1253849	1930971	70.85%	9.241%
80	11.480	3245	3247	3250	rVB3	1652	756	0.03%	0.004%
81	11.529	3257	3262	3263	rBV2	1058	822	0.03%	0.004%
82	11.628	3281	3293	3313	rBV	1278280	2034183	74.63%	9.735%
83	12.027	3415	3417	3419	rBV2	687	416	0.02%	0.002%
84	12.699	3624	3626	3628	rBV2	638	321	0.01%	0.002%
85	13.178	3773	3775	3776	rBV	999	390	0.01%	0.002%
86	13.213	3784	3786	3789	rVB3	915	389	0.01%	0.002%
87	13.519	3876	3881	3882	rBV4	2749	2417	0.09%	0.012%
88	13.631	3913	3916	3918	rBV2	1229	756	0.03%	0.004%
89	13.918	4002	4005	4007	rBV4	1103	630	0.02%	0.003%
90	14.239	4103	4105	4110	rBV4	1295	886	0.03%	0.004%




Sum of corrected areas: 20895538

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021111.D
Acq On : 23 Apr 2021 11:54
Operator : SY/MD
Sample : VV0423MBL01
Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK169

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

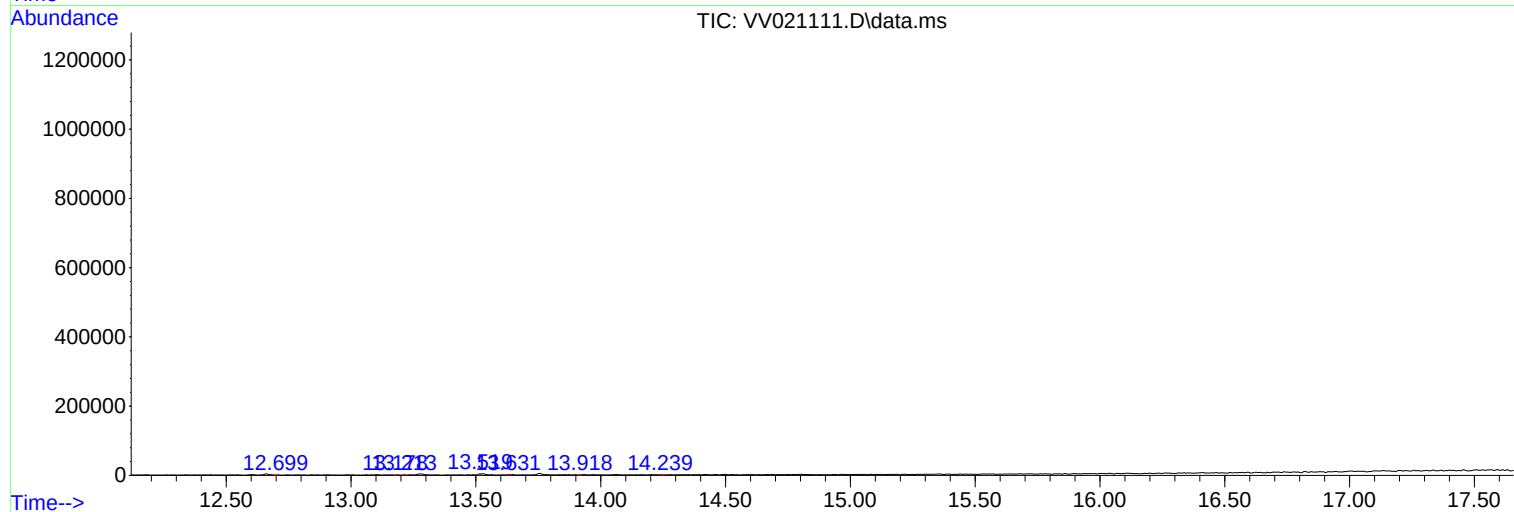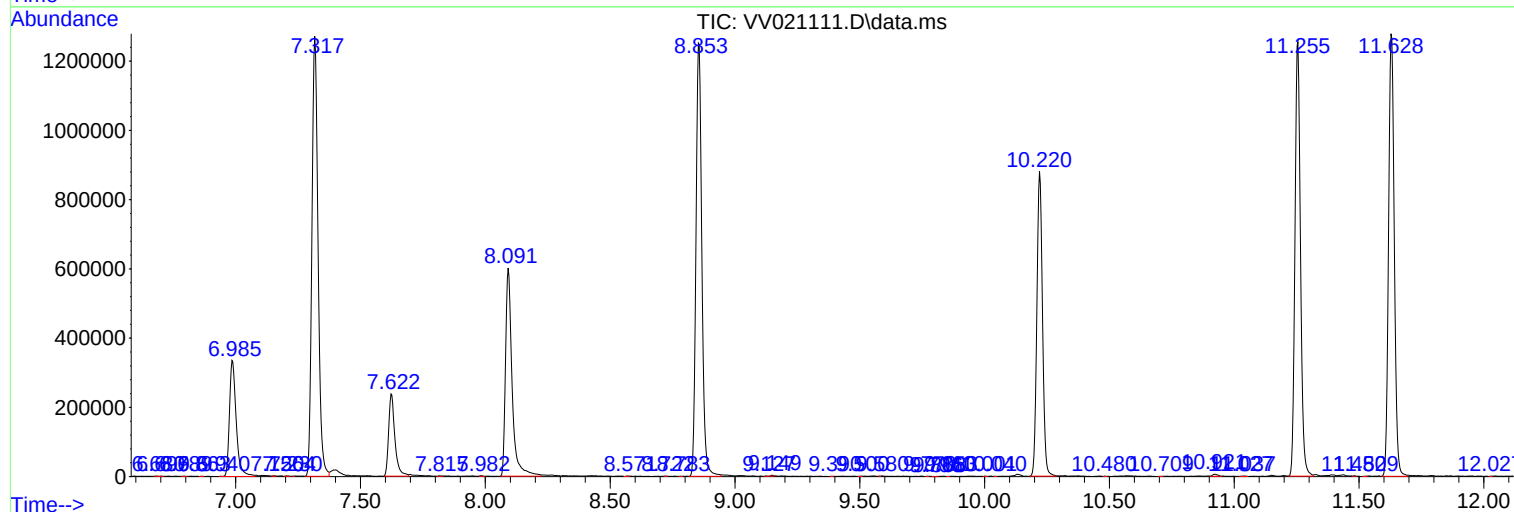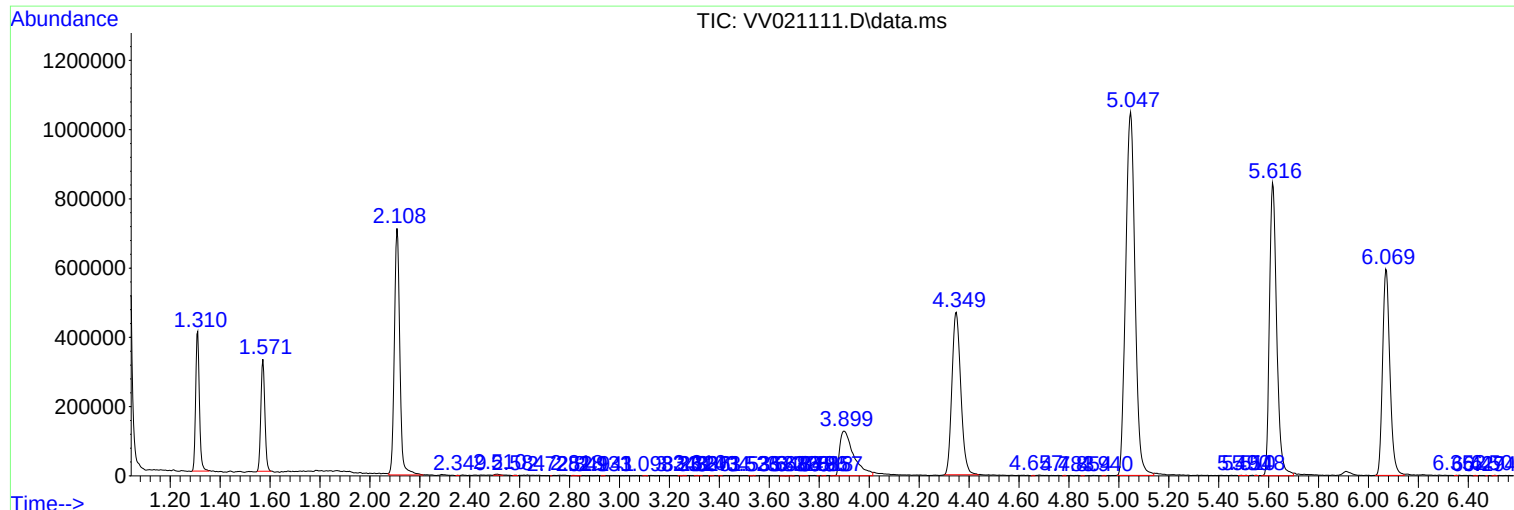

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021111.D
Acq On : 23 Apr 2021 11:54
Operator : SY/MD
Sample : VV0423MBL01
Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK169

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021111.D
Acq On : 23 Apr 2021 11:54
Operator : SY/MD
Sample : VV0423MBL01
Misc : 5.00G/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK169

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
