

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021112.D
 Acq On : 23 Apr 2021 12:17
 Operator : SY/MD
 Sample : VV0423WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK170

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021112.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	77	84	101	rVB	377361	387577	14.84%	1.934%
2	1.571	158	165	180	rVB	311400	348907	13.36%	1.741%
3	2.111	323	333	358	rVB	652921	964438	36.94%	4.813%
4	2.410	422	426	429	rBV4	1225	957	0.04%	0.005%
5	2.767	533	537	538	rBV3	963	653	0.03%	0.003%
6	2.847	560	562	566	rVB	764	533	0.02%	0.003%
7	2.870	566	569	571	rBV	415	251	0.01%	0.001%
8	2.931	586	588	590	rBV2	990	521	0.02%	0.003%
9	3.011	610	613	615	rBV2	785	494	0.02%	0.002%
10	3.044	618	623	626	rBV2	915	840	0.03%	0.004%
11	3.114	643	645	648	rVB2	501	192	0.01%	0.001%
12	3.169	657	662	665	rBV4	827	545	0.02%	0.003%
13	3.236	679	683	688	rBV4	625	519	0.02%	0.003%
14	3.384	725	729	730	rBV	409	271	0.01%	0.001%
15	3.426	740	742	745	rBV	614	402	0.02%	0.002%
16	3.452	748	750	751	rBV	490	184	0.01%	0.001%
17	3.484	758	760	762	rBV	418	182	0.01%	0.001%
18	3.568	784	786	788	rBV	342	112	0.00%	0.001%
19	3.638	804	808	809	rBV4	530	351	0.01%	0.002%
20	3.680	819	821	824	rVB2	521	217	0.01%	0.001%
21	3.693	824	825	826	rBV2	312	97	0.00%	0.000%
22	3.709	828	830	834	rVB2	607	307	0.01%	0.002%
23	3.728	834	836	838	rBV2	641	375	0.01%	0.002%
24	3.761	844	846	849	rBV	522	307	0.01%	0.002%
25	3.786	852	854	856	rBV2	421	255	0.01%	0.001%
26	3.831	866	868	869	rBV	244	129	0.00%	0.001%
27	3.851	872	874	877	rBV2	536	323	0.01%	0.002%
28	3.899	878	889	926	rBV	145981	489759	18.76%	2.444%
29	4.352	1015	1030	1054	rBV	449571	1113648	42.65%	5.557%
30	4.915	1202	1205	1206	rBV	741	478	0.02%	0.002%
31	4.979	1222	1225	1228	rBV2	649	493	0.02%	0.002%
32	5.050	1229	1247	1269	rBV2	1016567	2610956	100.00%	13.029%
33	5.468	1375	1377	1379	rVB	577	162	0.01%	0.001%
34	5.622	1413	1425	1456	rBV	788244	1591990	60.97%	7.944%
35	5.995	1537	1541	1544	rBV3	1002	990	0.04%	0.005%
36	6.076	1551	1566	1586	rBV	568429	1172356	44.90%	5.850%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021112.D
 Acq On : 23 Apr 2021 12:17
 Operator : SY/MD
 Sample : VV0423WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK170

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	6.349	1649	1651	1652	rBV	644	209	0.01%	0.001%
38	6.519	1700	1704	1706	rVB3	878	619	0.02%	0.003%
39	6.535	1706	1709	1710	rBV	663	311	0.01%	0.002%
40	6.664	1745	1749	1751	rBV3	1013	732	0.03%	0.004%
41	6.783	1780	1786	1788	rBV5	785	806	0.03%	0.004%
42	6.892	1818	1820	1826	rVB3	955	585	0.02%	0.003%
43	6.915	1826	1827	1830	rBV	317	154	0.01%	0.001%
44	6.989	1839	1850	1869	rBV2	319265	587362	22.50%	2.931%
45	7.320	1941	1953	1971	rBV	1219844	2096612	80.30%	10.462%
46	7.625	2038	2048	2066	rBV	235204	408899	15.66%	2.040%
47	7.857	2117	2120	2122	rBV3	1137	616	0.02%	0.003%
48	8.014	2168	2169	2174	rVB4	628	420	0.02%	0.002%
49	8.037	2174	2176	2181	rBV3	705	571	0.02%	0.003%
50	8.092	2183	2193	2220	rBV	597363	1097733	42.04%	5.478%
51	8.461	2305	2308	2309	rBV	1179	562	0.02%	0.003%
52	8.638	2361	2363	2366	rVB3	661	329	0.01%	0.002%
53	8.857	2419	2431	2453	rBV	1201099	1967401	75.35%	9.818%
54	9.198	2535	2537	2539	rBV2	675	339	0.01%	0.002%
55	9.317	2571	2574	2578	rVB5	917	578	0.02%	0.003%
56	9.403	2600	2601	2604	rBV	564	291	0.01%	0.001%
57	9.664	2679	2682	2685	rBV2	456	331	0.01%	0.002%
58	9.680	2685	2687	2691	rVV2	777	684	0.03%	0.003%
59	9.709	2694	2696	2701	rVB2	806	453	0.02%	0.002%
60	9.754	2708	2710	2712	rBV2	700	283	0.01%	0.001%
61	9.921	2759	2762	2764	rVB2	1018	556	0.02%	0.003%
62	9.976	2777	2779	2783	rBV	398	308	0.01%	0.002%
63	9.995	2783	2785	2788	rBV2	838	502	0.02%	0.003%
64	10.030	2794	2796	2797	rBV2	350	161	0.01%	0.001%
65	10.072	2806	2809	2811	rBV2	526	278	0.01%	0.001%
66	10.133	2821	2828	2836	rVB5	5471	7912	0.30%	0.039%
67	10.169	2837	2839	2842	rVB2	803	302	0.01%	0.002%
68	10.220	2842	2855	2874	rBV	863007	1353917	51.86%	6.756%
69	10.445	2923	2925	2926	rBV	747	226	0.01%	0.001%
70	10.654	2984	2990	2992	rBV2	784	931	0.04%	0.005%
71	10.709	3004	3007	3010	rBV2	747	553	0.02%	0.003%
72	10.828	3041	3044	3047	rBV3	943	688	0.03%	0.003%
73	11.114	3131	3133	3136	rVB2	606	326	0.01%	0.002%
74	11.149	3138	3144	3152	rBV7	2915	3757	0.14%	0.019%
75	11.255	3166	3177	3202	rBV	1180351	1826626	69.96%	9.115%
76	11.545	3265	3267	3272	rBV3	1056	999	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021112.D
 Acq On : 23 Apr 2021 12:17
 Operator : SY/MD
 Sample : VV0423WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK170

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	11.632	3282	3294	3312	rBV	1267340	1975242	75.65%	9.857%
78	11.882	3370	3372	3374	rBV	870	567	0.02%	0.003%
79	12.024	3414	3416	3420	rVB3	1102	634	0.02%	0.003%
80	12.066	3427	3429	3432	rBV2	846	560	0.02%	0.003%
81	12.239	3479	3483	3487	rBV5	931	943	0.04%	0.005%
82	12.326	3508	3510	3513	rBV2	1083	477	0.02%	0.002%
83	12.378	3524	3526	3530	rBV4	891	577	0.02%	0.003%
84	12.413	3535	3537	3539	rBV2	796	355	0.01%	0.002%
85	12.487	3556	3560	3564	rBV2	1272	1285	0.05%	0.006%
86	12.548	3575	3579	3582	rVB2	1132	844	0.03%	0.004%
87	12.641	3606	3608	3609	rBV2	700	199	0.01%	0.001%
88	12.815	3658	3662	3663	rBV2	594	422	0.02%	0.002%
89	13.021	3723	3726	3729	rBV	655	485	0.02%	0.002%
90	13.040	3729	3732	3734	rBV	955	566	0.02%	0.003%
91	13.236	3790	3793	3795	rBV	1054	689	0.03%	0.003%




Sum of corrected areas: 20039538

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021112.D
Acq On : 23 Apr 2021 12:17
Operator : SY/MD
Sample : VV0423WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK170

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

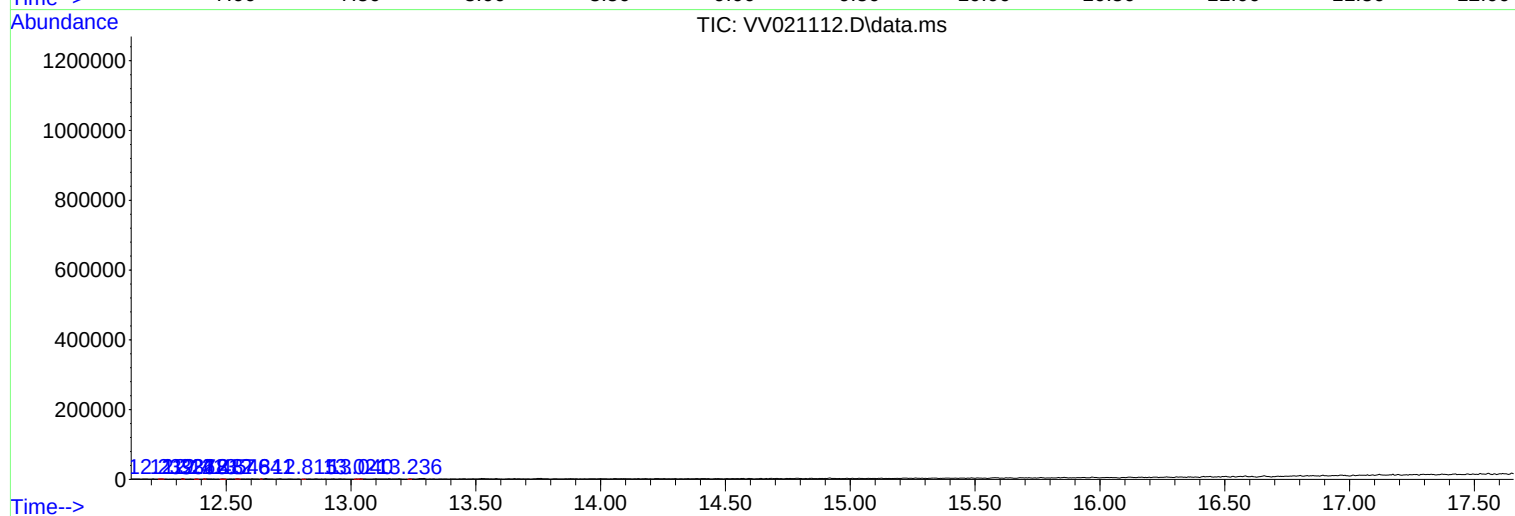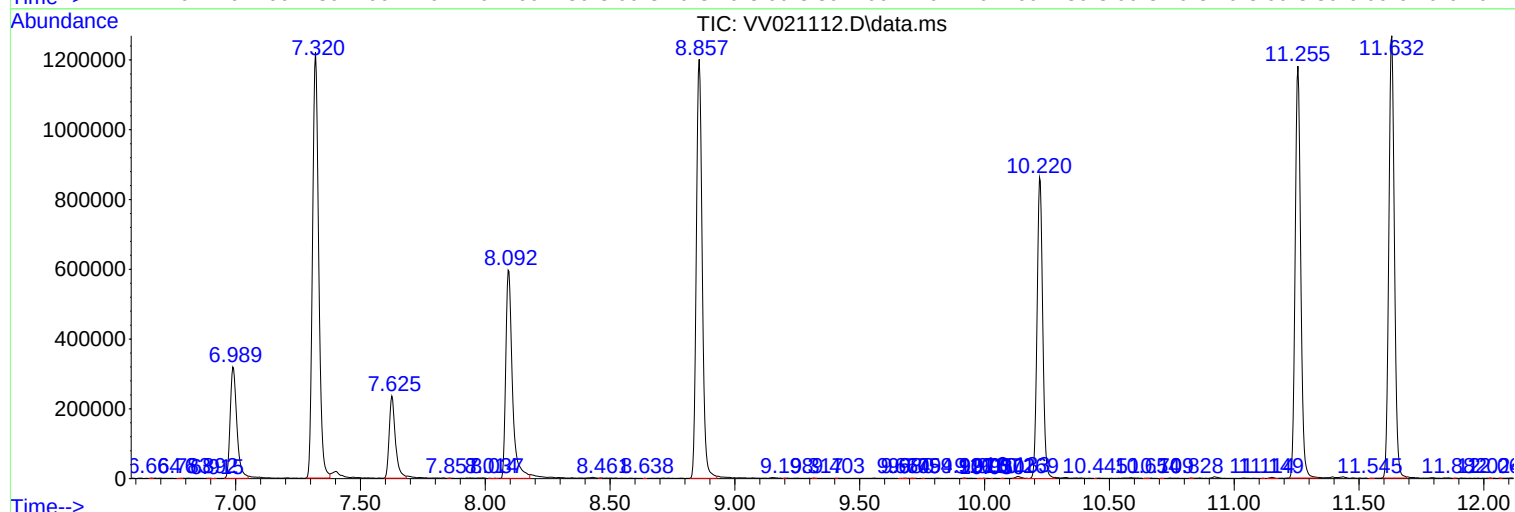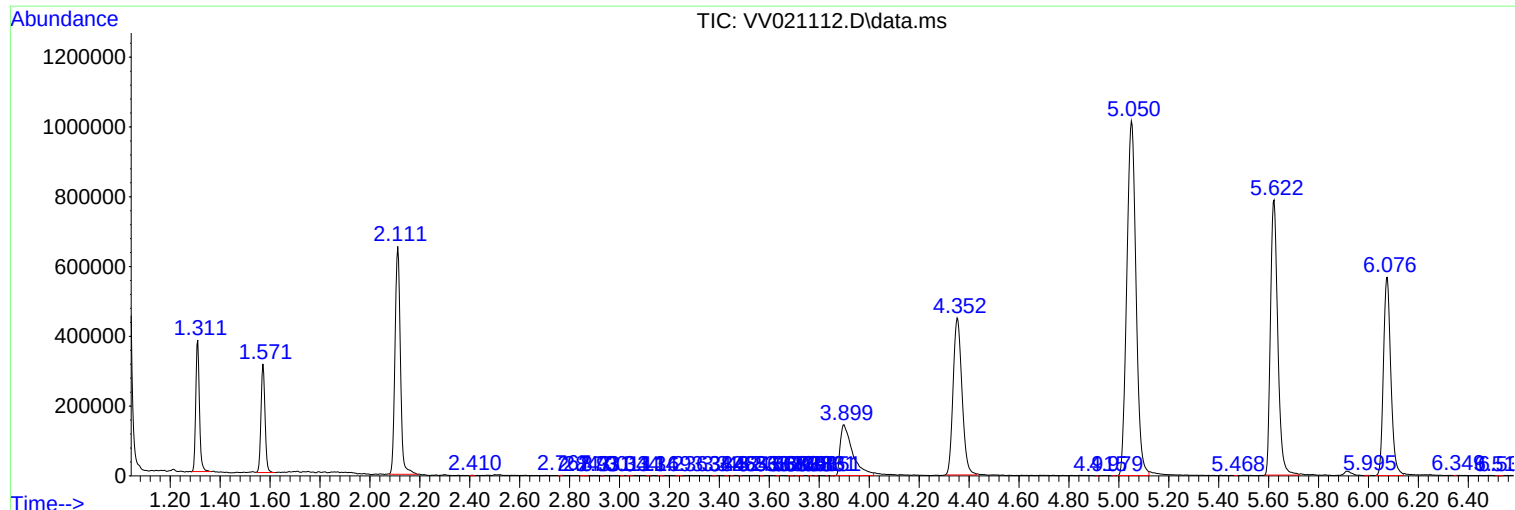

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021112.D
Acq On : 23 Apr 2021 12:17
Operator : SY/MD
Sample : VV0423WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK170

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021112.D
Acq On : 23 Apr 2021 12:17
Operator : SY/MD
Sample : VV0423WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK170

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
