

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021114.D
 Acq On : 23 Apr 2021 13:07
 Operator : SY/MD
 Sample : M2144-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	99	rVB	345350	361035	14.36%	1.856%
2	1.571	158	165	181	rVB	287458	326293	12.98%	1.677%
3	2.111	323	333	346	rBV	622003	904176	35.96%	4.648%
4	2.497	451	453	456	rBV2	1425	1110	0.04%	0.006%
5	2.761	532	535	537	rBV4	1253	754	0.03%	0.004%
6	2.857	561	565	567	rBV3	486	375	0.01%	0.002%
7	3.002	607	610	612	rBV2	561	311	0.01%	0.002%
8	3.040	620	622	624	rBV3	657	374	0.01%	0.002%
9	3.079	629	634	636	rBV4	601	436	0.02%	0.002%
10	3.111	641	644	647	rBV4	889	673	0.03%	0.003%
11	3.153	655	657	659	rBV	590	355	0.01%	0.002%
12	3.243	683	685	688	rBV	638	324	0.01%	0.002%
13	3.330	710	712	714	rVB	678	260	0.01%	0.001%
14	3.484	756	760	761	rBV	504	327	0.01%	0.002%
15	3.568	782	786	788	rBV3	709	493	0.02%	0.003%
16	3.622	799	803	804	rBV2	763	616	0.02%	0.003%
17	3.719	832	833	839	rVB2	1077	502	0.02%	0.003%
18	3.748	839	842	845	rBV	645	427	0.02%	0.002%
19	3.863	873	878	879	rBV	701	409	0.02%	0.002%
20	3.905	879	891	927	rBV	128485	454202	18.06%	2.335%
21	4.352	1014	1030	1055	rBV	437316	1079867	42.95%	5.551%
22	4.693	1131	1136	1139	rBV3	1103	1142	0.05%	0.006%
23	4.854	1183	1186	1189	rBV2	1284	798	0.03%	0.004%
24	4.873	1189	1192	1194	rVV2	532	328	0.01%	0.002%
25	4.908	1199	1203	1205	rBV2	374	292	0.01%	0.002%
26	4.921	1205	1207	1210	rBV2	552	371	0.01%	0.002%
27	4.937	1210	1212	1215	rBV4	431	262	0.01%	0.001%
28	4.986	1224	1227	1229	rVB	1098	621	0.02%	0.003%
29	5.050	1229	1247	1273	rBV2	977655	2514458	100.00%	12.926%
30	5.378	1347	1349	1351	rBV2	981	487	0.02%	0.003%
31	5.478	1377	1380	1384	rBV5	1794	1385	0.06%	0.007%
32	5.526	1392	1395	1399	rBV2	855	645	0.03%	0.003%
33	5.622	1411	1425	1455	rBV	770561	1570588	62.46%	8.074%
34	5.912	1508	1515	1534	rVB2	24518	49511	1.97%	0.255%
35	6.076	1551	1566	1594	rBV	554853	1131876	45.01%	5.819%
36	6.330	1643	1645	1649	rVB2	1208	789	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021114.D
 Acq On : 23 Apr 2021 13:07
 Operator : SY/MD
 Sample : M2144-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	6.400	1662	1667	1671	rBV4	1021	994	0.04%	0.005%
38	6.423	1671	1674	1675	rBV2	899	528	0.02%	0.003%
39	6.622	1733	1736	1737	rBV	614	353	0.01%	0.002%
40	6.638	1737	1741	1742	rBV2	909	726	0.03%	0.004%
41	6.690	1754	1757	1759	rBV2	791	592	0.02%	0.003%
42	6.719	1763	1766	1769	rVB2	762	363	0.01%	0.002%
43	6.822	1796	1798	1801	rVB2	666	351	0.01%	0.002%
44	6.989	1839	1850	1876	rBV	307050	574869	22.86%	2.955%
45	7.320	1941	1953	1972	rBV	1168644	2022280	80.43%	10.396%
46	7.625	2038	2048	2077	rBV	219603	390987	15.55%	2.010%
47	7.911	2135	2137	2138	rBV	695	337	0.01%	0.002%
48	7.931	2141	2143	2145	rBV2	1166	774	0.03%	0.004%
49	8.021	2169	2171	2173	rBV2	811	359	0.01%	0.002%
50	8.053	2179	2181	2182	rBV	822	379	0.02%	0.002%
51	8.095	2183	2194	2217	rBV	575562	1042060	41.44%	5.357%
52	8.439	2299	2301	2303	rBV3	777	341	0.01%	0.002%
53	8.477	2312	2313	2318	rVB3	526	285	0.01%	0.001%
54	8.503	2318	2321	2322	rBV2	960	529	0.02%	0.003%
55	8.619	2354	2357	2361	rBV3	1223	722	0.03%	0.004%
56	8.706	2379	2384	2385	rBV2	948	730	0.03%	0.004%
57	8.805	2412	2415	2418	rVB3	638	383	0.02%	0.002%
58	8.857	2418	2431	2455	rBV	1180312	1930335	76.77%	9.923%
59	9.069	2495	2497	2500	rBV3	1001	567	0.02%	0.003%
60	9.117	2509	2512	2518	rBV4	1121	1247	0.05%	0.006%
61	9.146	2518	2521	2522	rBV	1095	553	0.02%	0.003%
62	9.220	2542	2544	2546	rBV	645	315	0.01%	0.002%
63	9.268	2557	2559	2563	rBV4	746	465	0.02%	0.002%
64	9.358	2584	2587	2590	rBV2	843	545	0.02%	0.003%
65	9.384	2593	2595	2599	rVV2	761	464	0.02%	0.002%
66	9.455	2615	2617	2620	rVB	603	285	0.01%	0.001%
67	9.487	2620	2627	2628	rBV4	924	987	0.04%	0.005%
68	9.628	2666	2671	2674	rBV4	782	671	0.03%	0.003%
69	9.648	2674	2677	2678	rBV	786	415	0.02%	0.002%
70	9.825	2730	2732	2736	rVV5	636	376	0.01%	0.002%
71	10.037	2793	2798	2800	rBV3	2020	1997	0.08%	0.010%
72	10.133	2824	2828	2836	rVB3	4533	4872	0.19%	0.025%
73	10.220	2843	2855	2877	rBV	786845	1266895	50.38%	6.513%
74	10.390	2903	2908	2913	rBV4	2306	2203	0.09%	0.011%
75	10.484	2934	2937	2938	rBV2	585	325	0.01%	0.002%
76	10.661	2989	2992	2996	rBV3	1230	985	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021114.D
 Acq On : 23 Apr 2021 13:07
 Operator : SY/MD
 Sample : M2144-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	10.712	3006	3008	3009	rBV	540	287	0.01%	0.001%
78	10.738	3014	3016	3018	rBV	735	435	0.02%	0.002%
79	10.808	3035	3038	3040	rBV2	671	386	0.02%	0.002%
80	10.921	3068	3073	3086	rVB9	5118	9129	0.36%	0.047%
81	11.156	3140	3146	3149	rBV6	2817	3886	0.15%	0.020%
82	11.255	3166	3177	3198	rBV	1147043	1798483	71.53%	9.246%
83	11.542	3257	3266	3281	rBV6	12774	25539	1.02%	0.131%
84	11.632	3282	3294	3316	rVV	1219455	1927087	76.64%	9.907%
85	11.927	3383	3386	3387	rBV2	626	312	0.01%	0.002%
86	12.043	3417	3422	3424	rBV4	1459	1362	0.05%	0.007%
87	12.358	3513	3520	3531	rVB8	8790	14414	0.57%	0.074%
88	12.493	3559	3562	3566	rBV3	841	664	0.03%	0.003%
89	12.606	3593	3597	3601	rBV3	1562	1450	0.06%	0.007%
90	12.751	3641	3642	3645	rVB	653	320	0.01%	0.002%
91	12.860	3673	3676	3679	rBV2	1305	837	0.03%	0.004%
92	12.972	3709	3711	3714	rVB2	745	396	0.02%	0.002%
93	13.037	3729	3731	3733	rBV2	817	468	0.02%	0.002%
94	13.075	3737	3743	3746	rBV4	1144	1507	0.06%	0.008%
95	13.124	3756	3758	3764	rVB3	927	724	0.03%	0.004%
96	13.349	3826	3828	3831	rVB2	875	356	0.01%	0.002%
97	13.442	3855	3857	3859	rBV	760	379	0.02%	0.002%
98	13.606	3903	3908	3912	rBV3	986	1183	0.05%	0.006%
99	13.654	3920	3923	3924	rBV3	939	506	0.02%	0.003%
100	14.593	4212	4215	4222	rBV5	1719	2045	0.08%	0.011%




Sum of corrected areas: 19452471

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021114.D
Acq On : 23 Apr 2021 13:07
Operator : SY/MD
Sample : M2144-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

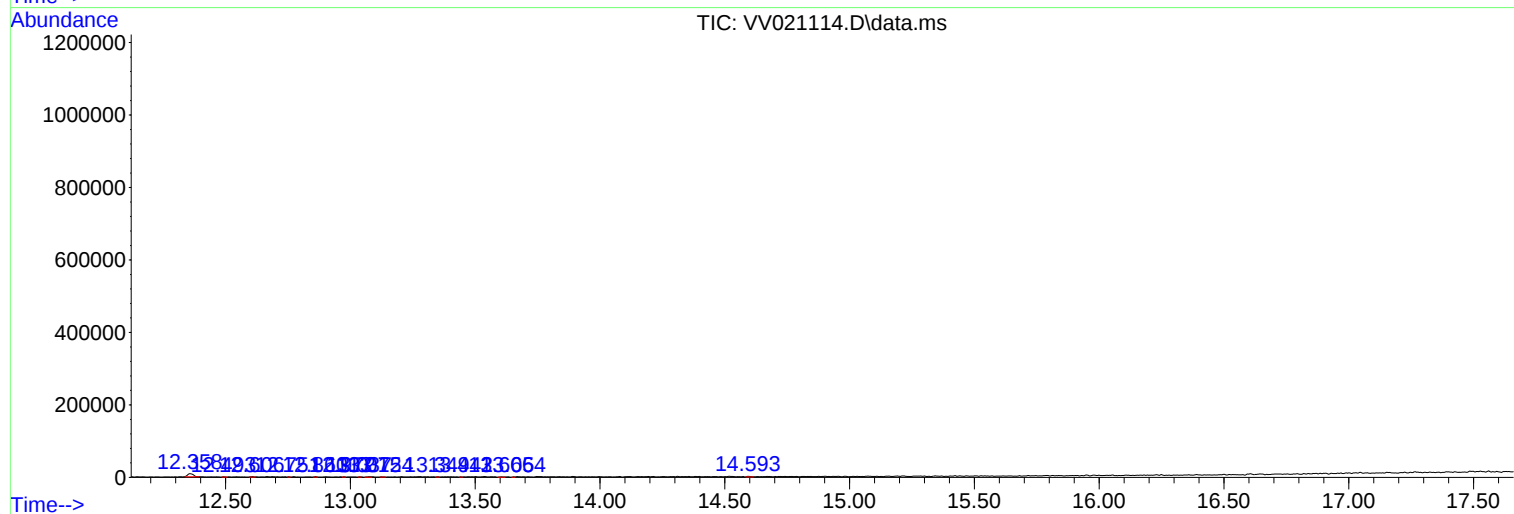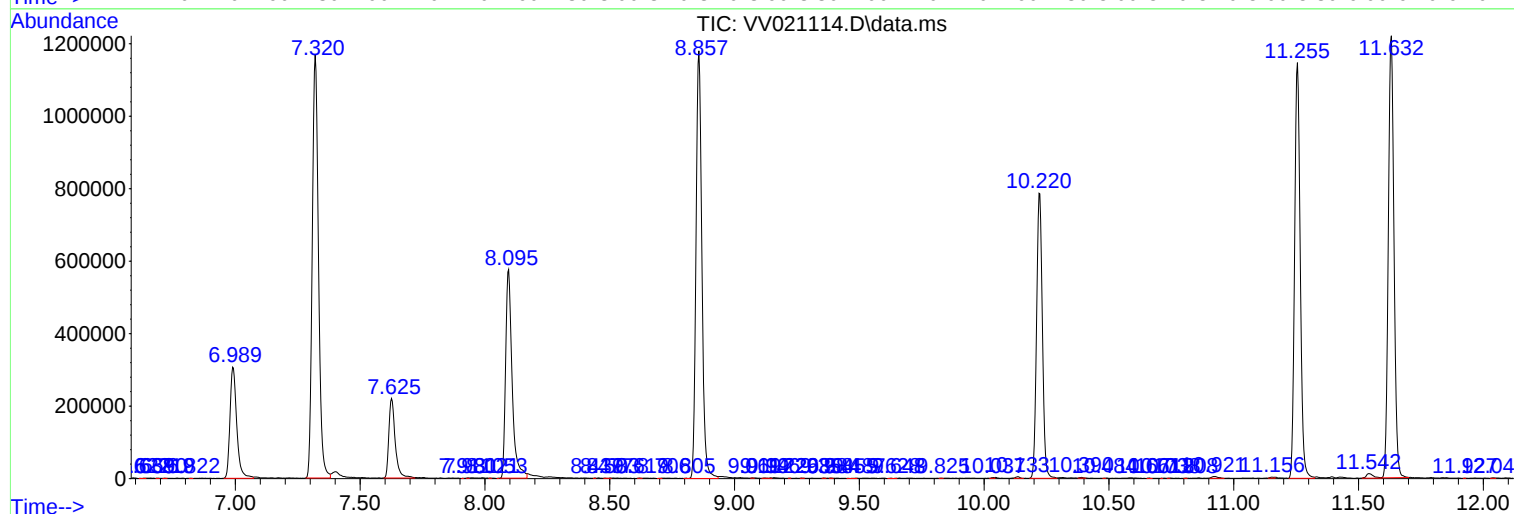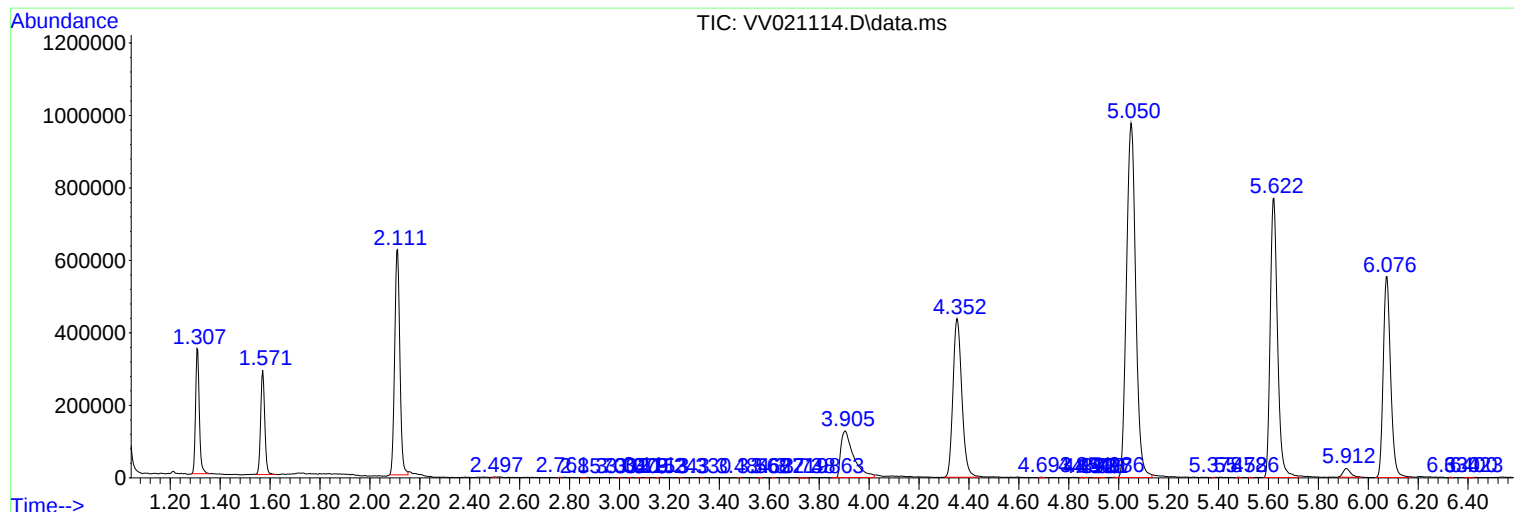

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021114.D
Acq On : 23 Apr 2021 13:07
Operator : SY/MD
Sample : M2144-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021114.D
Acq On : 23 Apr 2021 13:07
Operator : SY/MD
Sample : M2144-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
