

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021115.D
 Acq On : 23 Apr 2021 13:30
 Operator : SY/MD
 Sample : M2144-01DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021115.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	98	rVB	347271	356005	7.64%	1.470%
2	1.571	158	165	175	rVB	285751	320546	6.88%	1.323%
3	2.111	323	333	350	rBV	606846	891398	19.13%	3.680%
4	2.375	413	415	419	rBV3	811	471	0.01%	0.002%
5	2.674	507	508	509	rBV	557	127	0.00%	0.001%
6	2.757	532	534	535	rBV	471	182	0.00%	0.001%
7	2.786	539	543	545	rBV2	703	538	0.01%	0.002%
8	2.889	571	575	578	rBV2	564	478	0.01%	0.002%
9	2.915	581	583	585	rBV3	615	287	0.01%	0.001%
10	2.950	593	594	598	rVB	487	264	0.01%	0.001%
11	2.992	603	607	609	rBV2	571	386	0.01%	0.002%
12	3.005	609	611	612	rBV	469	176	0.00%	0.001%
13	3.169	660	662	664	rBV	445	259	0.01%	0.001%
14	3.191	666	669	671	rVB	927	553	0.01%	0.002%
15	3.207	671	674	676	rBV	276	162	0.00%	0.001%
16	3.220	676	678	681	rBV	505	325	0.01%	0.001%
17	3.236	681	683	686	rVB2	535	229	0.00%	0.001%
18	3.352	715	719	721	rBV	764	473	0.01%	0.002%
19	3.397	729	733	737	rVB2	772	633	0.01%	0.003%
20	3.420	737	740	742	rBV2	500	290	0.01%	0.001%
21	3.432	742	744	745	rBV	199	74	0.00%	0.000%
22	3.461	751	753	755	rBV	330	111	0.00%	0.000%
23	3.532	773	775	778	rBV2	602	298	0.01%	0.001%
24	3.577	787	789	793	rBV2	475	368	0.01%	0.002%
25	3.651	808	812	814	rBV3	614	409	0.01%	0.002%
26	3.664	814	816	818	rVV2	293	120	0.00%	0.000%
27	3.680	818	821	822	rBV	302	145	0.00%	0.001%
28	3.744	837	841	845	rBV3	312	396	0.01%	0.002%
29	3.825	864	866	867	rBV	422	173	0.00%	0.001%
30	3.838	867	870	872	rVV2	647	403	0.01%	0.002%
31	3.899	879	889	929	rBV2	139247	485006	10.41%	2.002%
32	4.211	983	986	988	rBV	914	574	0.01%	0.002%
33	4.352	1015	1030	1060	rBV	430189	1055098	22.64%	4.356%
34	4.696	1135	1137	1141	rVB4	1016	456	0.01%	0.002%
35	4.773	1156	1161	1163	rBV3	1030	781	0.02%	0.003%
36	4.815	1172	1174	1179	rBV4	491	436	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021115.D
 Acq On : 23 Apr 2021 13:30
 Operator : SY/MD
 Sample : M2144-01DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	4.879	1192	1194	1197	rBV3	489	228	0.00%	0.001%
38	4.982	1221	1226	1230	rBV3	1013	958	0.02%	0.004%
39	5.050	1230	1247	1286	rBV2	967151	2524834	54.17%	10.424%
40	5.532	1394	1397	1400	rVB2	957	476	0.01%	0.002%
41	5.619	1410	1424	1453	rBV	777453	1579146	33.88%	6.520%
42	6.072	1553	1565	1594	rBV	542360	1103308	23.67%	4.555%
43	6.429	1674	1676	1677	rBV	447	188	0.00%	0.001%
44	6.545	1710	1712	1714	rBV2	764	405	0.01%	0.002%
45	6.558	1714	1716	1718	rBV	647	350	0.01%	0.001%
46	6.606	1726	1731	1736	rVB2	672	689	0.01%	0.003%
47	6.641	1739	1742	1743	rBV	636	247	0.01%	0.001%
48	6.802	1789	1792	1793	rBV	228	94	0.00%	0.000%
49	6.815	1793	1796	1798	rBV	658	401	0.01%	0.002%
50	6.831	1798	1801	1805	rBV3	1159	930	0.02%	0.004%
51	6.931	1829	1832	1834	rVB2	583	259	0.01%	0.001%
52	6.992	1839	1851	1875	rBV	311064	569347	12.22%	2.351%
53	7.249	1929	1931	1934	rVB3	977	424	0.01%	0.002%
54	7.320	1941	1953	1972	rBV	1153473	2003917	43.00%	8.273%
55	7.625	2039	2048	2074	rBV	220334	381333	8.18%	1.574%
56	7.931	2139	2143	2155	rBV7	1923	4054	0.09%	0.017%
57	8.091	2183	2193	2229	rBV	604710	1089884	23.39%	4.500%
58	8.599	2349	2351	2355	rBV3	515	394	0.01%	0.002%
59	8.638	2359	2363	2364	rBV2	501	405	0.01%	0.002%
60	8.696	2375	2381	2383	rBV3	1041	1111	0.02%	0.005%
61	8.857	2419	2431	2437	rBV	1213179	2046289	43.91%	8.448%
62	9.143	2517	2520	2521	rBV2	1110	576	0.01%	0.002%
63	9.188	2531	2534	2539	rBV6	1029	819	0.02%	0.003%
64	9.310	2569	2572	2580	rVB5	1505	1573	0.03%	0.006%
65	9.342	2580	2582	2583	rBV	273	101	0.00%	0.000%
66	9.361	2583	2588	2591	rBV4	1128	839	0.02%	0.003%
67	9.419	2603	2606	2607	rBV3	958	378	0.01%	0.002%
68	9.500	2627	2631	2633	rBV2	629	503	0.01%	0.002%
69	9.612	2665	2666	2669	rBV2	373	197	0.00%	0.001%
70	9.683	2686	2688	2690	rBV3	693	315	0.01%	0.001%
71	9.998	2781	2786	2788	rBV3	957	933	0.02%	0.004%
72	10.066	2804	2807	2808	rBV2	536	318	0.01%	0.001%
73	10.220	2843	2855	2877	rBV	839685	1308892	28.08%	5.404%
74	10.442	2920	2924	2925	rBV2	798	485	0.01%	0.002%
75	10.857	3050	3053	3056	rBV2	1125	956	0.02%	0.004%
76	10.924	3067	3074	3084	rVB6	4803	7031	0.15%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021115.D
 Acq On : 23 Apr 2021 13:30
 Operator : SY/MD
 Sample : M2144-01DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

77	11.152	3138	3145	3148	rBV6	2251	2598	0.06%	0.011%
78	11.191	3148	3157	3166	rVV2	69986	108033	2.32%	0.446%
79	11.255	3166	3177	3199	rVV2	1301424	2932237	62.92%	12.106%
80	11.500	3251	3253	3254	rBV2	712	204	0.00%	0.001%
81	11.644	3282	3298	3319	rBV2	2057637	4660602	100.00%	19.241%
82	12.348	3515	3517	3519	rBV	888	519	0.01%	0.002%
83	12.490	3558	3561	3562	rBV2	706	315	0.01%	0.001%
84	12.593	3591	3593	3596	rBV2	838	461	0.01%	0.002%
85	12.657	3608	3613	3620	rBV7	4192	5877	0.13%	0.024%
86	12.731	3632	3636	3639	rBV4	884	896	0.02%	0.004%
87	12.902	3687	3689	3692	rVB2	987	449	0.01%	0.002%
88	12.982	3712	3714	3715	rBV	655	248	0.01%	0.001%
89	13.268	3793	3803	3818	rBV	340510	529817	11.37%	2.187%
90	13.754	3943	3954	3968	rBV	150955	227382	4.88%	0.939%




Sum of corrected areas: 24221855

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021115.D
Acq On : 23 Apr 2021 13:30
Operator : SY/MD
Sample : M2144-01DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

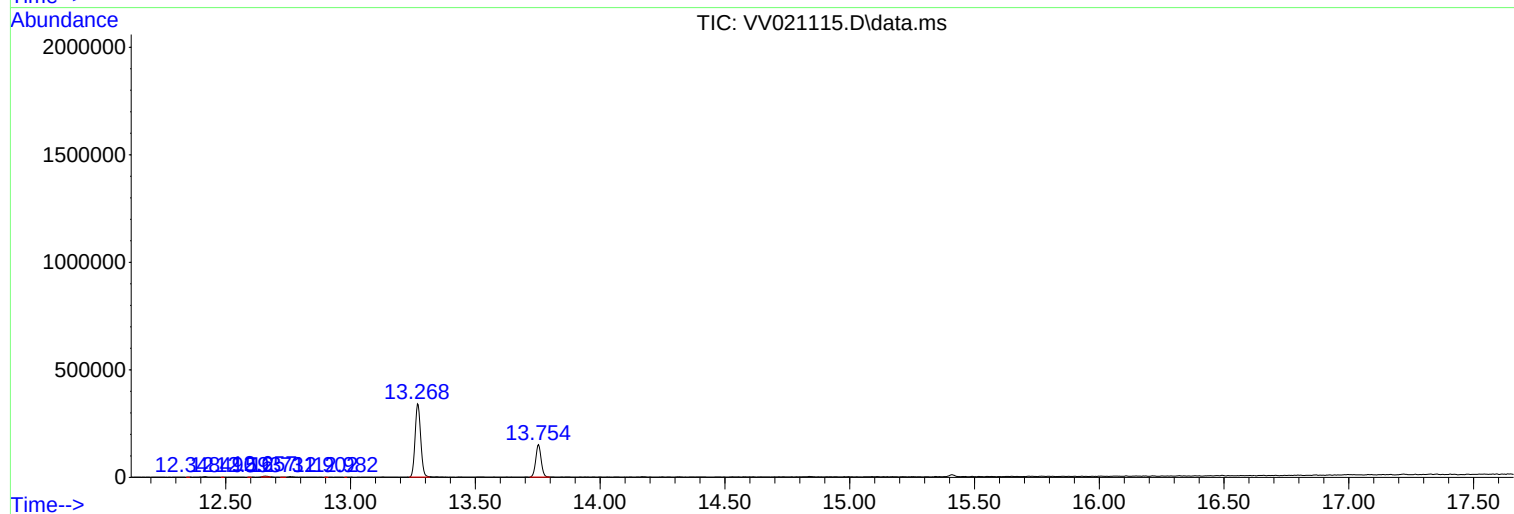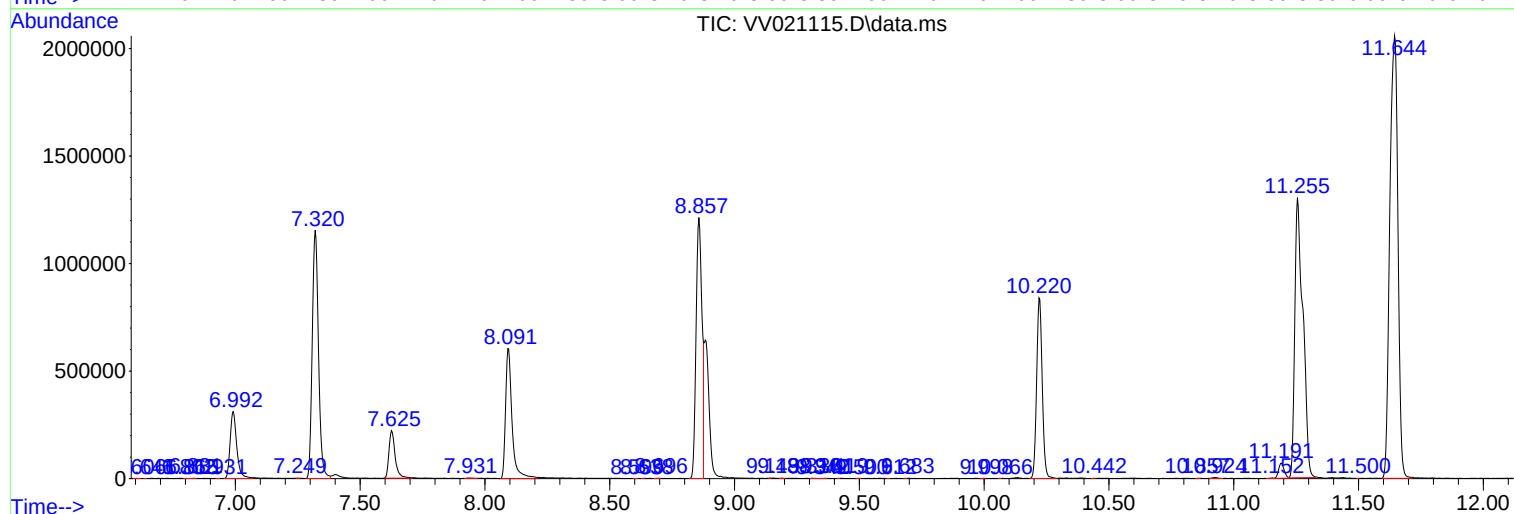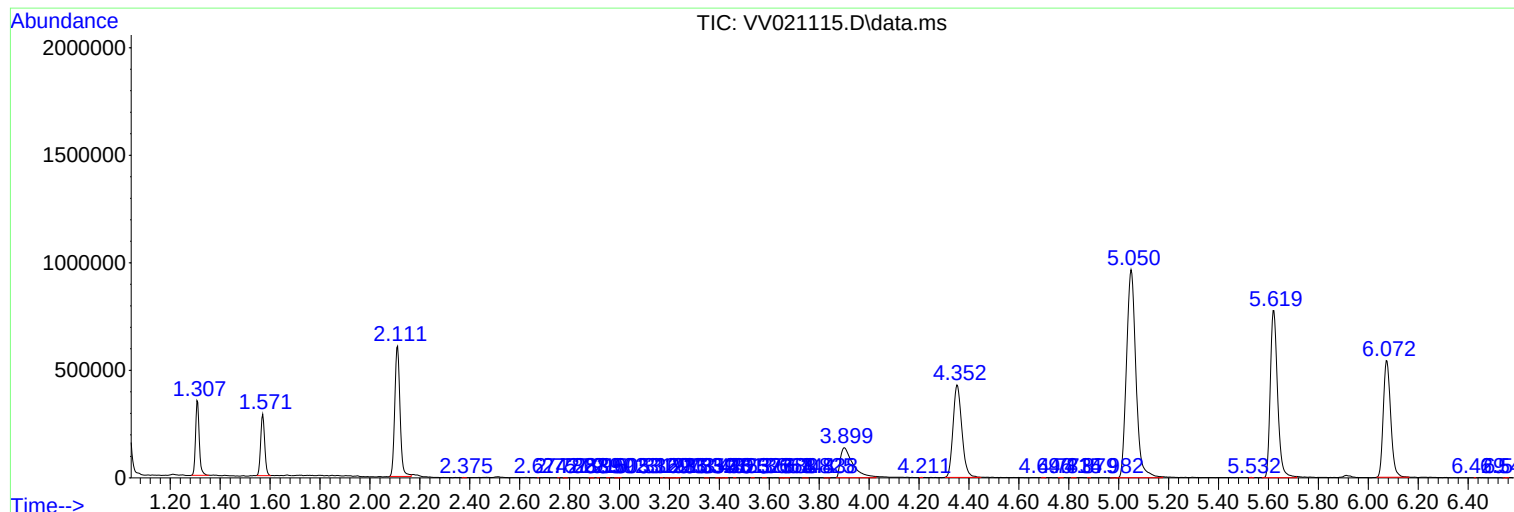

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021115.D
Acq On : 23 Apr 2021 13:30
Operator : SY/MD
Sample : M2144-01DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021115.D
Acq On : 23 Apr 2021 13:30
Operator : SY/MD
Sample : M2144-01DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------