

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021116.D
 Acq On : 23 Apr 2021 13:54
 Operator : SY/MD
 Sample : M2144-05DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	345836	346377	7.57%	1.552%
2	1.571	158	165	180	rVB	282389	323676	7.08%	1.450%
3	2.108	323	332	363	rVB	611115	917582	20.06%	4.110%
4	2.282	382	386	388	rBV4	1043	983	0.02%	0.004%
5	2.391	416	420	424	rVB2	420	332	0.01%	0.001%
6	2.429	428	432	435	rBV4	883	776	0.02%	0.003%
7	2.507	449	456	470	rVB6	4587	8637	0.19%	0.039%
8	2.664	501	505	507	rBV	902	796	0.02%	0.004%
9	2.748	527	531	532	rBV3	712	496	0.01%	0.002%
10	2.809	546	550	555	rBV5	623	666	0.01%	0.003%
11	2.892	574	576	579	rBV	528	313	0.01%	0.001%
12	2.918	581	584	588	rVV3	759	653	0.01%	0.003%
13	2.966	598	599	604	rVB3	907	665	0.01%	0.003%
14	2.999	604	609	611	rBV2	613	575	0.01%	0.003%
15	3.018	611	615	616	rBV	790	454	0.01%	0.002%
16	3.082	632	635	637	rBV3	618	397	0.01%	0.002%
17	3.127	644	649	650	rBV	447	346	0.01%	0.002%
18	3.188	663	668	671	rVV2	786	753	0.02%	0.003%
19	3.352	717	719	725	rVB3	563	458	0.01%	0.002%
20	3.558	780	783	788	rBV2	546	378	0.01%	0.002%
21	3.622	797	803	805	rBV2	433	443	0.01%	0.002%
22	3.899	878	889	924	rBV	138813	462445	10.11%	2.071%
23	4.352	1013	1030	1058	rBV	428374	1062547	23.23%	4.760%
24	4.661	1124	1126	1129	rVB3	1018	500	0.01%	0.002%
25	4.806	1166	1171	1174	rBV4	1056	1187	0.03%	0.005%
26	4.876	1190	1193	1195	rVB2	898	448	0.01%	0.002%
27	4.899	1197	1200	1202	rVB3	1029	489	0.01%	0.002%
28	4.957	1214	1218	1222	rBV4	910	915	0.02%	0.004%
29	4.976	1222	1224	1226	rBV	980	393	0.01%	0.002%
30	5.050	1230	1247	1259	rBV2	951776	2482655	54.28%	11.121%
31	5.368	1345	1346	1349	rBV2	711	439	0.01%	0.002%
32	5.506	1383	1389	1392	rBV5	1932	1891	0.04%	0.008%
33	5.574	1407	1410	1413	rBV2	769	615	0.01%	0.003%
34	5.619	1413	1424	1451	rBV	750039	1519943	33.23%	6.808%
35	5.912	1506	1515	1524	rBV5	9843	20591	0.45%	0.092%
36	6.072	1551	1565	1588	rBV	531616	1097982	24.01%	4.918%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042321\
 Data File : VW021116.D
 Acq On : 23 Apr 2021 13:54
 Operator : SY/MD
 Sample : M2144-05DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	6.291	1631	1633	1638	rBV3	773	432	0.01%	0.002%
38	6.365	1653	1656	1657	rBV2	1031	530	0.01%	0.002%
39	6.433	1672	1677	1680	rBV7	738	589	0.01%	0.003%
40	6.542	1708	1711	1712	rBV4	758	487	0.01%	0.002%
41	6.661	1742	1748	1752	rBV6	1115	1318	0.03%	0.006%
42	6.693	1756	1758	1761	rBV2	973	647	0.01%	0.003%
43	6.732	1767	1770	1775	rVV5	1047	620	0.01%	0.003%
44	6.934	1829	1833	1835	rBV2	690	522	0.01%	0.002%
45	6.989	1839	1850	1882	rVV2	302063	558954	12.22%	2.504%
46	7.320	1941	1953	1972	rBV	1145945	1967114	43.01%	8.811%
47	7.590	2035	2037	2038	rBV	808	346	0.01%	0.002%
48	7.625	2038	2048	2073	rVV	216873	391500	8.56%	1.754%
49	7.844	2113	2116	2119	rBV3	1067	832	0.02%	0.004%
50	7.918	2135	2139	2140	rBV3	1151	662	0.01%	0.003%
51	8.092	2183	2193	2225	rBV	611648	1095693	23.96%	4.908%
52	8.429	2292	2298	2300	rBV4	1189	1241	0.03%	0.006%
53	8.519	2323	2326	2332	rBV4	882	835	0.02%	0.004%
54	8.545	2332	2334	2341	rVB4	940	692	0.02%	0.003%
55	8.645	2362	2365	2367	rBV	904	496	0.01%	0.002%
56	8.686	2376	2378	2382	rVB3	645	484	0.01%	0.002%
57	8.709	2382	2385	2386	rBV2	609	364	0.01%	0.002%
58	8.748	2394	2397	2401	rVB4	799	544	0.01%	0.002%
59	8.770	2401	2404	2407	rBV3	571	345	0.01%	0.002%
60	8.786	2407	2409	2413	rBV3	589	406	0.01%	0.002%
61	8.857	2418	2431	2433	rBV	1263764	1541389	33.70%	6.904%
62	9.246	2550	2552	2553	rBV	1143	479	0.01%	0.002%
63	9.358	2583	2587	2589	rBV4	1437	1129	0.02%	0.005%
64	9.477	2621	2624	2626	rVB3	911	526	0.01%	0.002%
65	9.497	2628	2630	2634	rBV2	595	501	0.01%	0.002%
66	9.580	2654	2656	2661	rVB3	535	446	0.01%	0.002%
67	9.609	2661	2665	2669	rBV2	1104	809	0.02%	0.004%
68	9.825	2731	2732	2741	rVB3	1196	836	0.02%	0.004%
69	10.127	2817	2826	2839	rBV7	4567	7807	0.17%	0.035%
70	10.223	2843	2856	2875	rBV	827205	1299333	28.41%	5.820%
71	10.381	2903	2905	2909	rBV2	1315	1058	0.02%	0.005%
72	10.426	2917	2919	2922	rBV2	743	326	0.01%	0.001%
73	10.558	2958	2960	2962	rBV3	618	344	0.01%	0.002%
74	10.583	2962	2968	2973	rBV5	1765	2230	0.05%	0.010%
75	10.632	2981	2983	2988	rBV3	892	652	0.01%	0.003%
76	10.696	3000	3003	3004	rBV	675	397	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021116.D
 Acq On : 23 Apr 2021 13:54
 Operator : SY/MD
 Sample : M2144-05DL 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

77	10.818	3035	3041	3043	rVB3	1046	983	0.02%	0.004%
78	10.841	3045	3048	3052	rBV3	1009	1022	0.02%	0.005%
79	10.989	3089	3094	3096	rBV3	833	605	0.01%	0.003%
80	11.040	3106	3110	3118	rVB6	1253	1432	0.03%	0.006%
81	11.072	3118	3120	3122	rBV	737	365	0.01%	0.002%
82	11.149	3135	3144	3146	rBV4	2483	2887	0.06%	0.013%
83	11.188	3147	3156	3166	rBV	150296	227417	4.97%	1.019%
84	11.255	3167	3177	3180	rBV	1333952	1840001	40.23%	8.242%
85	11.500	3251	3253	3254	rBV2	1039	445	0.01%	0.002%
86	11.577	3275	3277	3280	rBV2	768	436	0.01%	0.002%
87	11.645	3282	3298	3321	rBV2	2049023	4573413	100.00%	20.486%
88	11.918	3378	3383	3385	rBV3	1273	924	0.02%	0.004%
89	12.014	3410	3413	3414	rBV2	1217	673	0.01%	0.003%
90	12.349	3514	3517	3521	rBV4	1155	901	0.02%	0.004%
91	12.448	3546	3548	3550	rBV	900	509	0.01%	0.002%
92	12.596	3590	3594	3597	rBV5	1351	1456	0.03%	0.007%
93	12.760	3640	3645	3651	rBV4	1684	1928	0.04%	0.009%
94	13.198	3778	3781	3787	rVB4	1143	923	0.02%	0.004%
95	13.271	3792	3804	3815	rBV	273977	419252	9.17%	1.878%
96	13.619	3906	3912	3914	rBV2	1156	1156	0.03%	0.005%
97	13.754	3945	3954	3965	rBV2	65001	102564	2.24%	0.459%
98	13.860	3984	3987	3989	rBV2	1060	642	0.01%	0.003%
99	14.117	4063	4067	4070	rBV5	1168	1081	0.02%	0.005%
100	14.178	4084	4086	4089	rBV3	1090	945	0.02%	0.004%




Sum of corrected areas: 22324671

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021116.D
Acq On : 23 Apr 2021 13:54
Operator : SY/MD
Sample : M2144-05DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

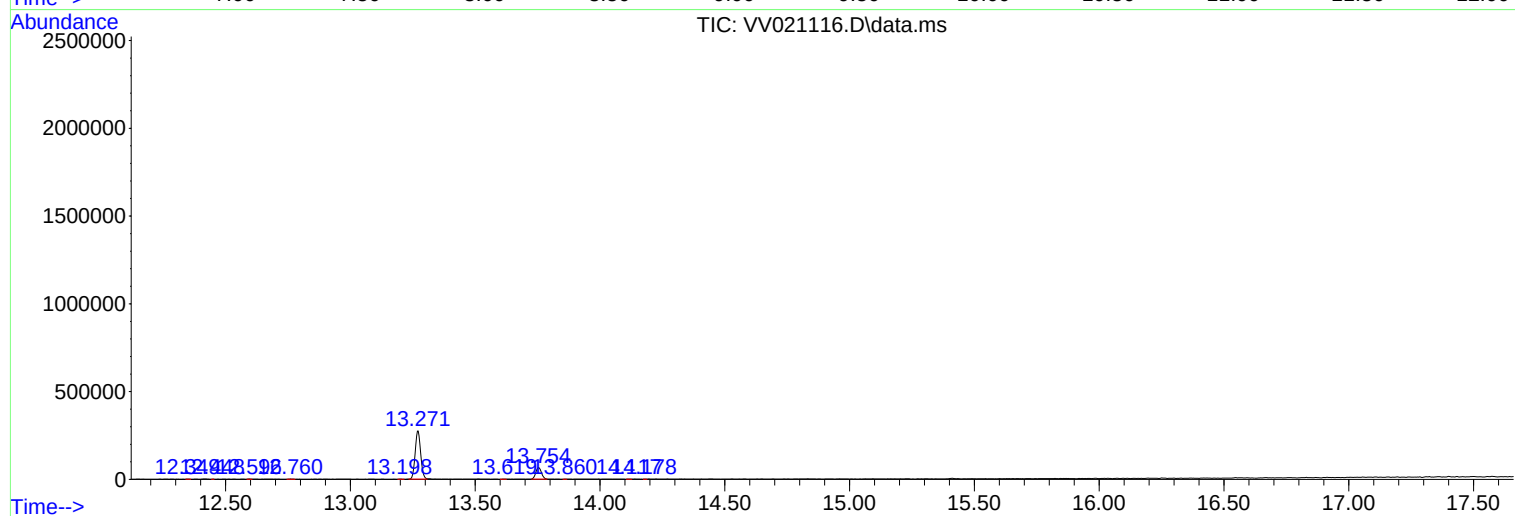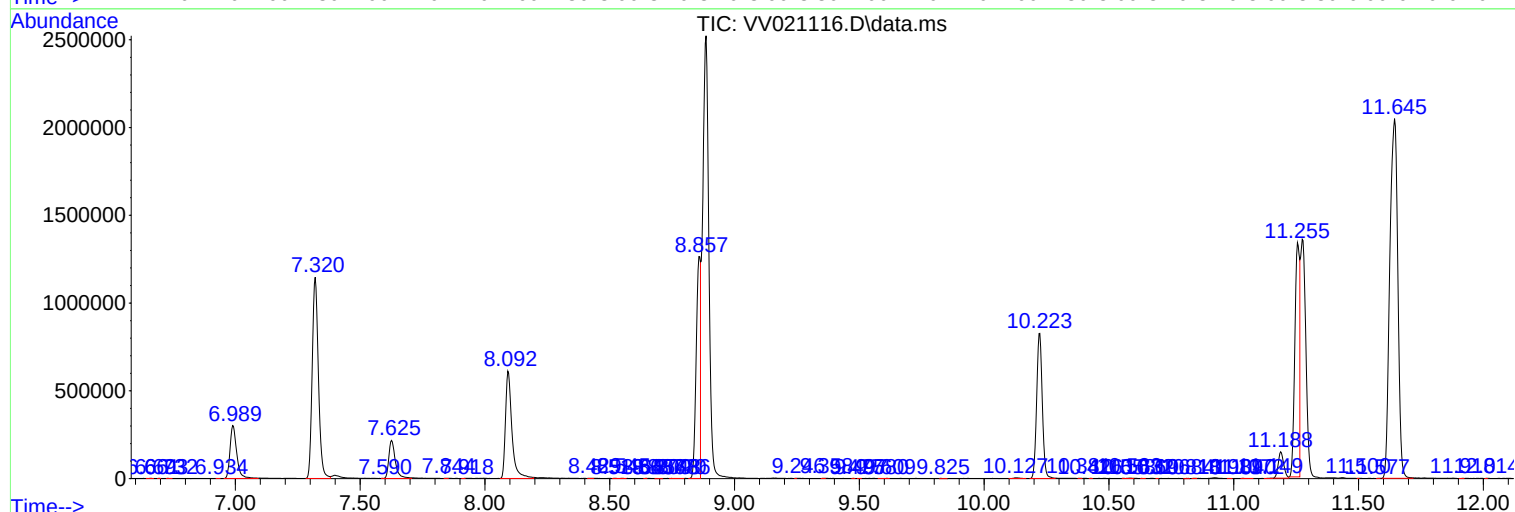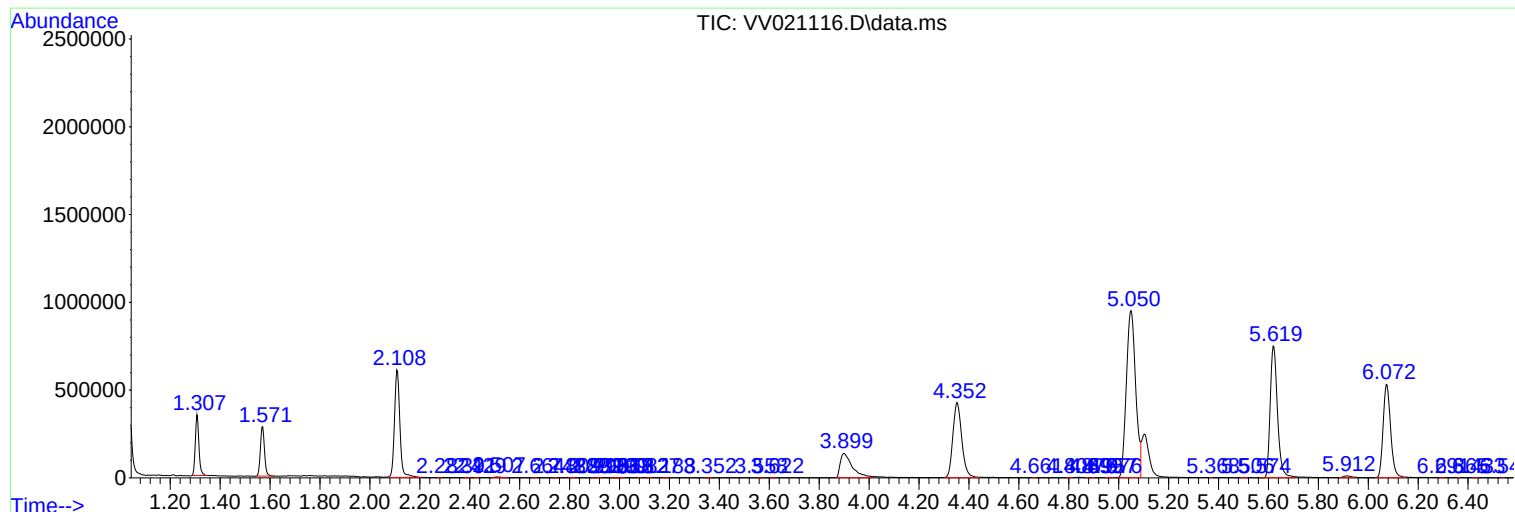

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021116.D
Acq On : 23 Apr 2021 13:54
Operator : SY/MD
Sample : M2144-05DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021116.D
Acq On : 23 Apr 2021 13:54
Operator : SY/MD
Sample : M2144-05DL 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
