

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021118.D
 Acq On : 23 Apr 2021 14:41
 Operator : SY/MD
 Sample : M2144-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	336063	347886	14.23%	1.812%
2	1.571	158	165	175	rVB	282809	314216	12.85%	1.636%
3	2.111	323	333	345	rBV	597953	858742	35.13%	4.472%
4	2.561	469	473	475	rBV3	647	449	0.02%	0.002%
5	2.587	475	481	483	rBV2	1032	976	0.04%	0.005%
6	2.625	483	493	502	rBV4	4406	9654	0.39%	0.050%
7	2.690	510	513	516	rBV2	819	531	0.02%	0.003%
8	2.748	529	531	534	rBV4	589	374	0.02%	0.002%
9	2.805	547	549	552	rVB	519	214	0.01%	0.001%
10	2.838	557	559	565	rVB2	571	520	0.02%	0.003%
11	2.873	565	570	571	rBV2	450	408	0.02%	0.002%
12	2.921	583	585	587	rBV	513	213	0.01%	0.001%
13	2.979	598	603	606	rBV2	606	505	0.02%	0.003%
14	3.101	635	641	643	rBV2	766	695	0.03%	0.004%
15	3.233	680	682	684	rBV2	612	317	0.01%	0.002%
16	3.249	685	687	691	rVV2	651	459	0.02%	0.002%
17	3.272	691	694	698	rVV	613	362	0.01%	0.002%
18	3.301	698	703	705	rBV	614	438	0.02%	0.002%
19	3.394	729	732	735	rBV	362	223	0.01%	0.001%
20	3.455	748	751	754	rVB2	428	230	0.01%	0.001%
21	3.471	754	756	758	rBV	416	247	0.01%	0.001%
22	3.596	789	795	801	rVB4	648	815	0.03%	0.004%
23	3.680	818	821	823	rBV2	626	394	0.02%	0.002%
24	3.719	831	833	835	rVB	715	274	0.01%	0.001%
25	3.748	840	842	846	rBV	434	317	0.01%	0.002%
26	3.812	859	862	864	rBV	593	371	0.02%	0.002%
27	3.828	864	867	870	rVB	893	480	0.02%	0.002%
28	3.857	873	876	878	rBV2	417	243	0.01%	0.001%
29	3.905	878	891	943	rBV3	165073	667899	27.32%	3.478%
30	4.352	1016	1030	1058	rBV	424433	1104296	45.17%	5.750%
31	4.690	1131	1135	1139	rBV3	1365	1033	0.04%	0.005%
32	4.741	1148	1151	1153	rBV2	909	508	0.02%	0.003%
33	4.773	1160	1161	1164	rBV	706	315	0.01%	0.002%
34	4.838	1178	1181	1183	rVB2	1018	470	0.02%	0.002%
35	5.050	1229	1247	1279	rBV3	938930	2444705	100.00%	12.730%
36	5.445	1368	1370	1372	rVB	661	248	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021118.D
 Acq On : 23 Apr 2021 14:41
 Operator : SY/MD
 Sample : M2144-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	5.500	1381	1387	1394	rBV8	1441	2012	0.08%	0.010%
38	5.532	1394	1397	1399	rBV3	881	470	0.02%	0.002%
39	5.622	1413	1425	1451	rBV	745861	1512139	61.85%	7.874%
40	5.911	1505	1515	1533	rBV5	23077	52877	2.16%	0.275%
41	6.001	1541	1543	1547	rVB5	1123	690	0.03%	0.004%
42	6.075	1552	1566	1588	rBV	541106	1106089	45.24%	5.760%
43	6.378	1658	1660	1662	rBV	902	611	0.02%	0.003%
44	6.497	1695	1697	1700	rBV2	751	417	0.02%	0.002%
45	6.754	1773	1777	1778	rBV2	774	391	0.02%	0.002%
46	6.908	1822	1825	1826	rBV2	1062	575	0.02%	0.003%
47	6.937	1832	1834	1838	rVB2	794	512	0.02%	0.003%
48	6.989	1838	1850	1871	rBV2	303374	556244	22.75%	2.896%
49	7.204	1914	1917	1918	rBV	1187	632	0.03%	0.003%
50	7.268	1935	1937	1941	rBV3	932	570	0.02%	0.003%
51	7.320	1941	1953	1972	rBV	1146649	1956045	80.01%	10.186%
52	7.625	2037	2048	2070	rBV	217127	382136	15.63%	1.990%
53	7.866	2120	2123	2127	rBV5	1214	868	0.04%	0.005%
54	7.911	2135	2137	2139	rBV2	914	394	0.02%	0.002%
55	8.034	2171	2175	2177	rBV2	1261	928	0.04%	0.005%
56	8.095	2183	2194	2225	rBV	593468	1097730	44.90%	5.716%
57	8.509	2321	2323	2325	rBV	723	400	0.02%	0.002%
58	8.554	2331	2337	2343	rVB5	1122	1171	0.05%	0.006%
59	8.583	2343	2346	2348	rBV2	989	546	0.02%	0.003%
60	8.638	2359	2363	2364	rBV3	765	463	0.02%	0.002%
61	8.702	2381	2383	2384	rBV	701	234	0.01%	0.001%
62	8.718	2385	2388	2391	rVV4	837	618	0.03%	0.003%
63	8.802	2411	2414	2417	rVB	695	455	0.02%	0.002%
64	8.857	2417	2431	2461	rBV	1144225	1857142	75.97%	9.670%
65	9.217	2540	2543	2544	rBV2	669	378	0.02%	0.002%
66	9.307	2567	2571	2575	rBV4	529	574	0.02%	0.003%
67	9.615	2666	2667	2670	rVB2	609	281	0.01%	0.001%
68	9.632	2670	2672	2675	rBV2	306	212	0.01%	0.001%
69	9.661	2678	2681	2684	rVB2	833	532	0.02%	0.003%
70	9.718	2696	2699	2700	rBV2	750	392	0.02%	0.002%
71	9.857	2740	2742	2744	rBV	836	472	0.02%	0.002%
72	9.988	2780	2783	2785	rBV	368	259	0.01%	0.001%
73	10.082	2809	2812	2814	rBV2	647	431	0.02%	0.002%
74	10.133	2819	2828	2837	rVV5	4824	6942	0.28%	0.036%
75	10.223	2843	2856	2881	rBV	802854	1274376	52.13%	6.636%
76	10.429	2919	2920	2923	rVB	557	247	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021118.D
 Acq On : 23 Apr 2021 14:41
 Operator : SY/MD
 Sample : M2144-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	10.448	2923	2926	2931	rBV4	735	611	0.02%	0.003%
78	10.522	2947	2949	2953	rBV3	644	378	0.02%	0.002%
79	10.587	2966	2969	2972	rBV3	1730	1223	0.05%	0.006%
80	10.622	2977	2980	2981	rBV	628	398	0.02%	0.002%
81	10.757	3020	3022	3024	rBV	750	333	0.01%	0.002%
82	10.821	3038	3042	3046	rBV3	829	842	0.03%	0.004%
83	10.908	3065	3069	3070	rBV2	1323	913	0.04%	0.005%
84	10.931	3070	3076	3083	rVB9	3893	5428	0.22%	0.028%
85	10.976	3088	3090	3093	rVB	832	408	0.02%	0.002%
86	11.014	3096	3102	3105	rBV3	876	973	0.04%	0.005%
87	11.066	3115	3118	3120	rBV	571	322	0.01%	0.002%
88	11.255	3166	3177	3205	rBV	1113278	1727691	70.67%	8.996%
89	11.541	3262	3266	3275	rBV8	3600	4994	0.20%	0.026%
90	11.631	3282	3294	3314	rBV	1210179	1875510	76.72%	9.766%
91	11.931	3385	3387	3388	rBV	825	347	0.01%	0.002%
92	12.435	3542	3544	3546	rBV2	845	358	0.01%	0.002%
93	12.467	3551	3554	3557	rBV2	658	545	0.02%	0.003%
94	12.725	3630	3634	3636	rBV3	1094	804	0.03%	0.004%
95	12.805	3657	3659	3661	rBV	1049	521	0.02%	0.003%
96	12.988	3714	3716	3717	rBV	548	226	0.01%	0.001%
97	13.082	3742	3745	3747	rBV2	1065	622	0.03%	0.003%
98	13.217	3784	3787	3789	rBV3	946	660	0.03%	0.003%
99	13.683	3930	3932	3936	rVB3	1524	1016	0.04%	0.005%
100	13.824	3972	3976	3977	rBV3	722	605	0.02%	0.003%


Sum of corrected areas: 19204210

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021118.D
Acq On : 23 Apr 2021 14:41
Operator : SY/MD
Sample : M2144-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

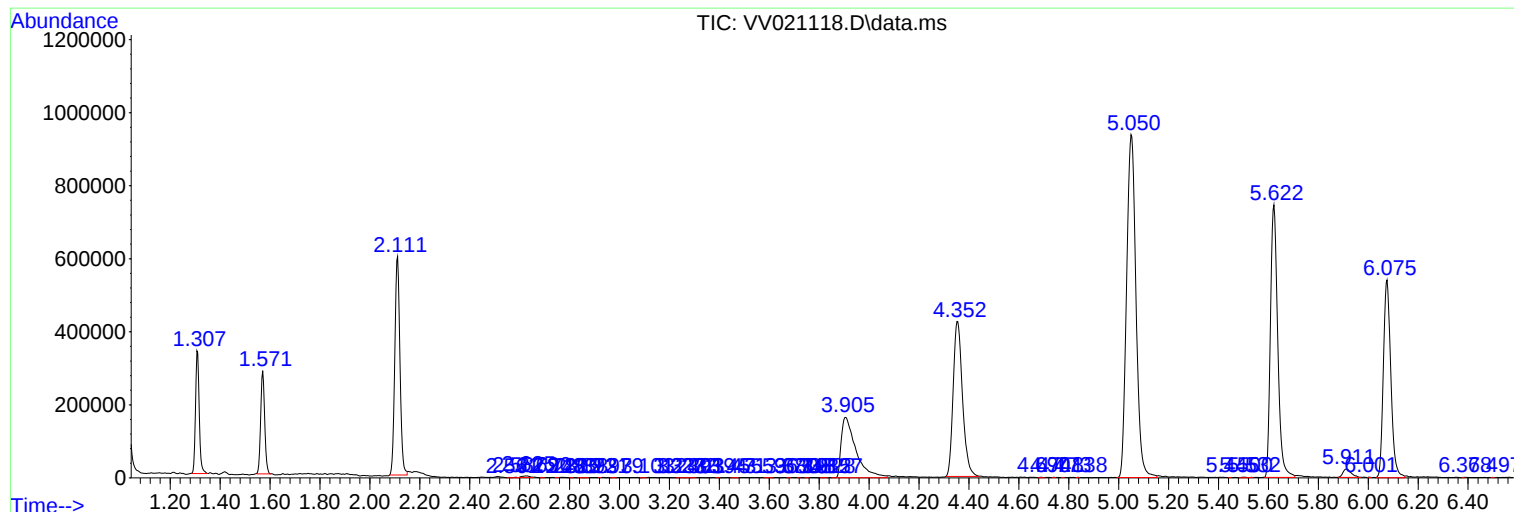

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021118.D
Acq On : 23 Apr 2021 14:41
Operator : SY/MD
Sample : M2144-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021118.D
Acq On : 23 Apr 2021 14:41
Operator : SY/MD
Sample : M2144-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
