

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021124.D
 Acq On : 23 Apr 2021 17:02
 Operator : SY/MD
 Sample : M2144-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021124.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	95	rBV	302250	309365	1.05%	0.387%
2	1.571	158	165	178	rVB	254246	284322	0.97%	0.355%
3	2.108	323	332	345	rBV	555503	797238	2.71%	0.996%
4	2.912	576	582	585	rBV3	922	863	0.00%	0.001%
5	2.950	591	594	596	rBV3	665	437	0.00%	0.001%
6	2.982	600	604	606	rVB3	943	644	0.00%	0.001%
7	3.082	633	635	639	rVB2	636	396	0.00%	0.000%
8	3.111	640	644	647	rBV3	768	668	0.00%	0.001%
9	3.192	664	669	670	rBV2	376	306	0.00%	0.000%
10	3.278	693	696	698	rBV2	591	343	0.00%	0.000%
11	3.388	728	730	735	rVB3	674	499	0.00%	0.001%
12	3.413	735	738	740	rBV2	504	360	0.00%	0.000%
13	3.452	746	750	753	rBV2	783	470	0.00%	0.001%
14	3.478	753	758	761	rBV	323	282	0.00%	0.000%
15	3.536	772	776	778	rBV	437	272	0.00%	0.000%
16	3.568	783	786	788	rBV2	652	418	0.00%	0.001%
17	3.674	816	819	821	rVB	1154	518	0.00%	0.001%
18	3.751	840	843	847	rBV2	585	461	0.00%	0.001%
19	3.806	858	860	866	rVB2	412	359	0.00%	0.000%
20	3.921	878	896	942	rBV3	120182	612014	2.08%	0.765%
21	4.352	1016	1030	1054	rBV	394470	984667	3.34%	1.230%
22	4.683	1131	1133	1137	rVB2	749	516	0.00%	0.001%
23	4.735	1147	1149	1151	rBV	573	298	0.00%	0.000%
24	4.786	1164	1165	1169	rVB3	791	458	0.00%	0.001%
25	4.809	1169	1172	1176	rVB4	1045	700	0.00%	0.001%
26	4.886	1194	1196	1199	rBV2	689	502	0.00%	0.001%
27	4.950	1213	1216	1217	rBV2	629	358	0.00%	0.000%
28	4.986	1222	1227	1230	rBV3	670	554	0.00%	0.001%
29	5.050	1230	1247	1259	rBV3	889816	2272946	7.72%	2.840%
30	5.378	1346	1349	1352	rBV4	1017	729	0.00%	0.001%
31	5.622	1412	1425	1453	rBV	783709	1589621	5.40%	1.986%
32	5.912	1506	1515	1535	rVB4	18833	40503	0.14%	0.051%
33	6.076	1549	1566	1591	rBV	494817	1033482	3.51%	1.291%
34	6.285	1629	1631	1633	rBV2	815	336	0.00%	0.000%
35	6.333	1644	1646	1649	rBV2	771	464	0.00%	0.001%
36	6.349	1649	1651	1654	rVV4	883	486	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021124.D
 Acq On : 23 Apr 2021 17:02
 Operator : SY/MD
 Sample : M2144-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	6.397	1663	1666	1667	rBV2	673	358	0.00%	0.000%
38	6.407	1667	1669	1673	rVV	781	318	0.00%	0.000%
39	6.436	1676	1678	1679	rBV	575	248	0.00%	0.000%
40	6.529	1705	1707	1711	rVB3	1271	748	0.00%	0.001%
41	6.551	1711	1714	1715	rBV	859	418	0.00%	0.001%
42	6.786	1784	1787	1792	rVB3	813	614	0.00%	0.001%
43	6.834	1800	1802	1805	rVB2	710	264	0.00%	0.000%
44	6.851	1805	1807	1810	rBV2	463	259	0.00%	0.000%
45	6.886	1816	1818	1821	rBV	337	277	0.00%	0.000%
46	6.899	1821	1822	1828	rVB2	568	339	0.00%	0.000%
47	6.992	1839	1851	1876	rBV	278187	518469	1.76%	0.648%
48	7.320	1940	1953	1971	rBV	1046366	1826948	6.20%	2.283%
49	7.625	2037	2048	2067	rBV	206256	359534	1.22%	0.449%
50	7.944	2134	2147	2155	rBV2	4668	7828	0.03%	0.010%
51	7.979	2155	2158	2160	rBV3	1581	942	0.00%	0.001%
52	8.095	2180	2194	2218	rBV	586627	1058321	3.59%	1.322%
53	8.426	2295	2297	2300	rBV2	1306	520	0.00%	0.001%
54	8.567	2337	2341	2342	rBV4	619	466	0.00%	0.001%
55	8.693	2379	2380	2385	rBV2	423	353	0.00%	0.000%
56	8.764	2398	2402	2405	rBV5	1279	1188	0.00%	0.001%
57	8.886	2416	2440	2483	rBV2	6156189	11775698	39.99%	14.712%
58	9.227	2543	2546	2553	rBV6	1842	1946	0.01%	0.002%
59	9.442	2610	2613	2615	rVB3	1535	790	0.00%	0.001%
60	9.484	2624	2626	2634	rVB4	897	926	0.00%	0.001%
61	9.635	2668	2673	2676	rBV2	1437	1255	0.00%	0.002%
62	9.677	2682	2686	2687	rBV2	840	583	0.00%	0.001%
63	9.712	2694	2697	2699	rVB	791	379	0.00%	0.000%
64	9.735	2699	2704	2705	rBV2	770	447	0.00%	0.001%
65	9.812	2723	2728	2733	rBV4	885	1193	0.00%	0.001%
66	9.902	2754	2756	2763	rVB3	1101	1110	0.00%	0.001%
67	9.944	2767	2769	2771	rBV2	511	344	0.00%	0.000%
68	9.998	2784	2786	2791	rBV2	661	390	0.00%	0.000%
69	10.034	2791	2797	2799	rBV3	726	851	0.00%	0.001%
70	10.130	2821	2827	2835	rBV6	3594	5326	0.02%	0.007%
71	10.220	2844	2855	2878	rVB	800436	1241090	4.21%	1.551%
72	10.455	2925	2928	2930	rBV3	1122	600	0.00%	0.001%
73	10.468	2930	2932	2936	rVB4	888	417	0.00%	0.001%
74	10.513	2942	2946	2947	rBV2	954	654	0.00%	0.001%
75	10.580	2965	2967	2968	rBV2	738	287	0.00%	0.000%
76	10.690	2999	3001	3004	rVB2	821	410	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021124.D
 Acq On : 23 Apr 2021 17:02
 Operator : SY/MD
 Sample : M2144-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	10.799	3033	3035	3039	rVB2	829	430	0.00%	0.001%
78	10.825	3039	3043	3045	rBV	767	591	0.00%	0.001%
79	10.921	3065	3073	3087	rBV9	4060	6909	0.02%	0.009%
80	10.979	3089	3091	3094	rBV	487	288	0.00%	0.000%
81	11.001	3094	3098	3103	rBV4	913	961	0.00%	0.001%
82	11.037	3106	3109	3115	rBB4	881	911	0.00%	0.001%
83	11.075	3119	3121	3122	rBV	570	275	0.00%	0.000%
84	11.188	3139	3156	3167	rBV	760770	1187333	4.03%	1.483%
85	11.278	3167	3184	3211	rVB2	7827798	13730499	46.62%	17.155%
86	11.651	3282	3300	3331	rBV	18372364	29449448	100.00%	36.793%
87	12.027	3414	3417	3420	rBV4	1528	988	0.00%	0.001%
88	12.146	3452	3454	3460	rVB5	1430	1057	0.00%	0.001%
89	12.172	3460	3462	3464	rBV2	885	580	0.00%	0.001%
90	12.217	3474	3476	3477	rBV	573	286	0.00%	0.000%
91	12.407	3526	3535	3547	rBV4	26717	43195	0.15%	0.054%
92	12.477	3555	3557	3559	rBV2	599	268	0.00%	0.000%
93	12.648	3600	3610	3623	rBV2	115462	187495	0.64%	0.234%
94	12.757	3636	3644	3657	rVB2	29494	49986	0.17%	0.062%
95	12.998	3715	3719	3723	rBV5	1491	1388	0.00%	0.002%
96	13.268	3790	3803	3824	rBV	4839327	7190626	24.42%	8.984%
97	13.751	3940	3953	3972	rVV	1995725	3042792	10.33%	3.802%
98	14.159	4072	4080	4096	rVB3	29841	48927	0.17%	0.061%
99	14.943	4320	4324	4328	rBV4	1736	1982	0.01%	0.002%
100	15.406	4458	4468	4481	rBV2	223441	343029	1.16%	0.429%




Sum of corrected areas: 80040207

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021124.D
Acq On : 23 Apr 2021 17:02
Operator : SY/MD
Sample : M2144-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

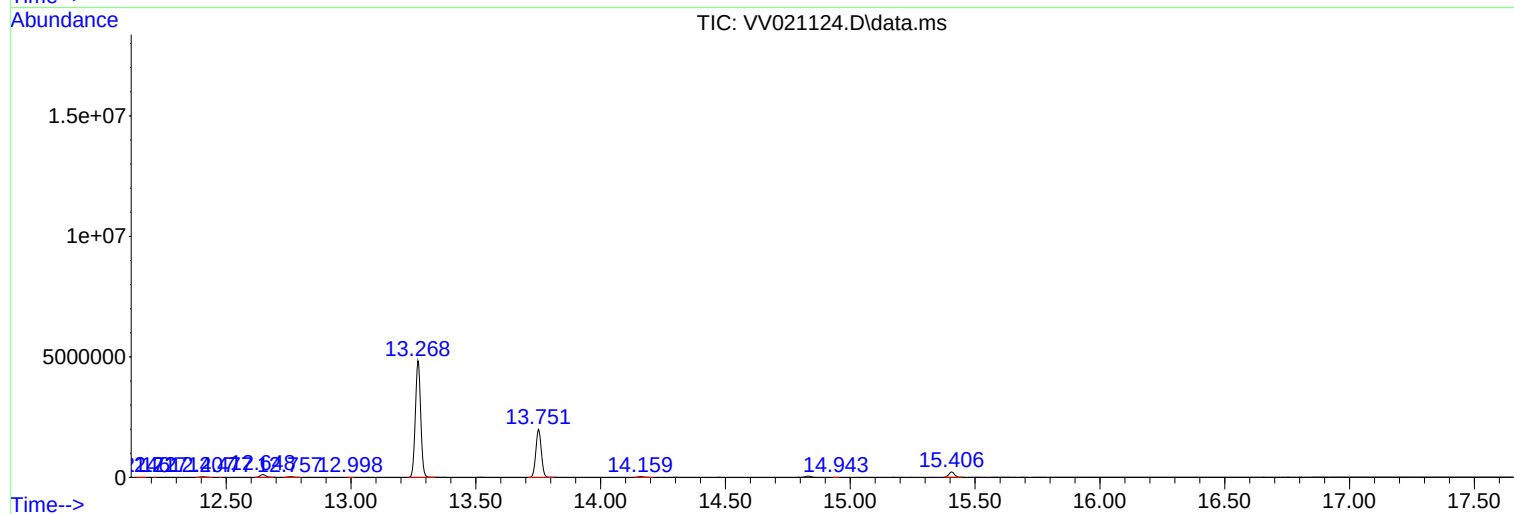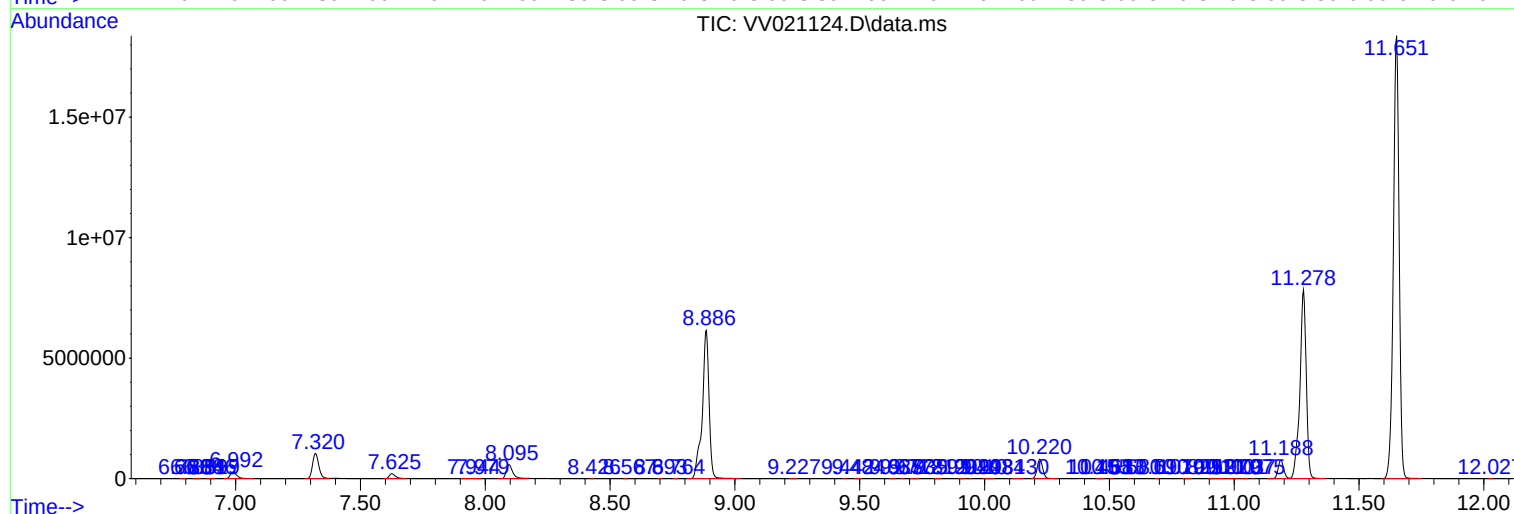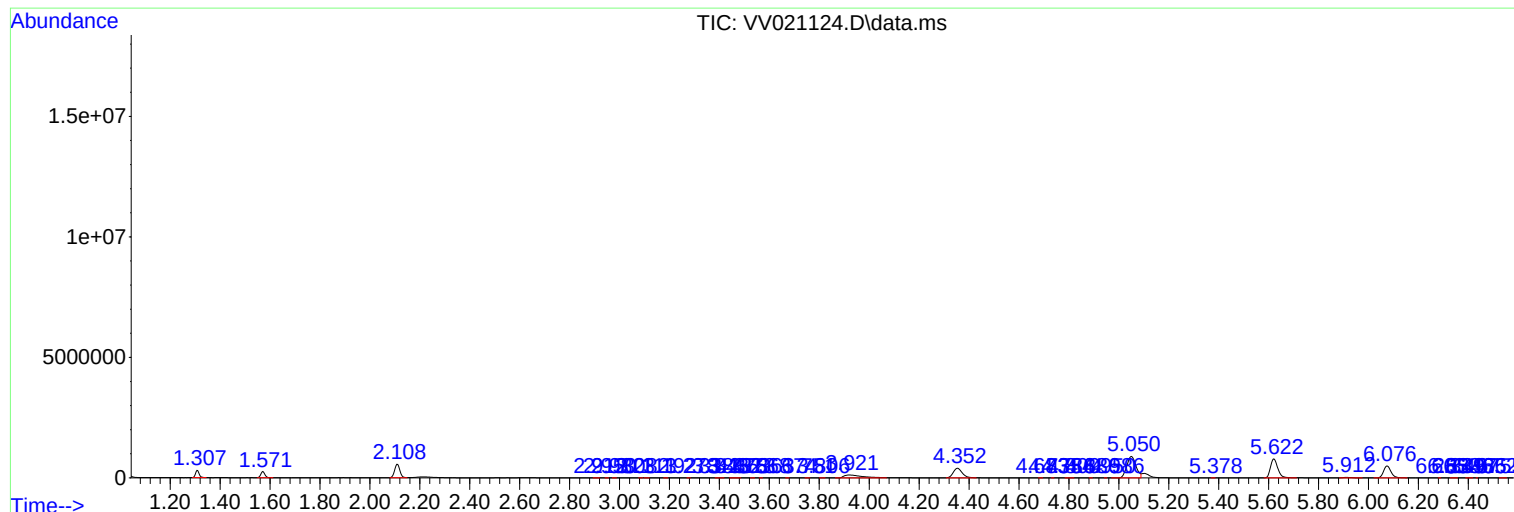

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021124.D
Acq On : 23 Apr 2021 17:02
Operator : SY/MD
Sample : M2144-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021124.D
Acq On : 23 Apr 2021 17:02
Operator : SY/MD
Sample : M2144-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
