

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021125.D
 Acq On : 23 Apr 2021 17:26
 Operator : SY/MD
 Sample : M2144-05 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021125.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	312042	316347	1.68%	0.532%
2	1.571	158	165	178	rVB	265928	301808	1.61%	0.507%
3	2.108	323	332	346	rBV	577794	824370	4.39%	1.385%
4	2.423	428	430	434	rVB2	1031	541	0.00%	0.001%
5	2.510	451	457	472	rVB3	15241	26259	0.14%	0.044%
6	2.619	489	491	492	rBV3	744	353	0.00%	0.001%
7	2.667	503	506	508	rBV	1155	698	0.00%	0.001%
8	2.732	524	526	530	rVB2	628	354	0.00%	0.001%
9	2.757	530	534	537	rBV4	1239	1035	0.01%	0.002%
10	2.818	550	553	554	rBV	467	296	0.00%	0.000%
11	2.870	566	569	571	rBV	569	368	0.00%	0.001%
12	2.902	575	579	583	rVB4	599	682	0.00%	0.001%
13	3.027	616	618	620	rBV	782	360	0.00%	0.001%
14	3.047	621	624	626	rBV2	684	442	0.00%	0.001%
15	3.095	636	639	642	rVB	1015	626	0.00%	0.001%
16	3.121	645	647	649	rVV	569	378	0.00%	0.001%
17	3.146	652	655	660	rVB4	697	632	0.00%	0.001%
18	3.195	667	670	672	rVB	498	286	0.00%	0.000%
19	3.317	706	708	711	rVB2	672	334	0.00%	0.001%
20	3.365	721	723	727	rVV3	912	539	0.00%	0.001%
21	3.429	741	743	746	rVV2	485	317	0.00%	0.001%
22	3.452	746	750	753	rVV3	982	776	0.00%	0.001%
23	3.471	753	756	759	rVB	750	476	0.00%	0.001%
24	3.535	772	776	779	rBV2	495	418	0.00%	0.001%
25	3.677	817	820	821	rBV	516	297	0.00%	0.000%
26	3.686	821	823	825	rVV	802	369	0.00%	0.001%
27	3.712	829	831	834	rVV2	621	342	0.00%	0.001%
28	3.764	837	847	860	rBV8	3249	8034	0.04%	0.014%
29	3.857	872	876	881	rVB5	755	682	0.00%	0.001%
30	3.918	882	895	931	rBV	105798	470915	2.51%	0.791%
31	4.352	1015	1030	1058	rBV	406244	1034096	5.50%	1.738%
32	4.664	1124	1127	1130	rBV4	882	773	0.00%	0.001%
33	4.744	1150	1152	1155	rBV3	859	588	0.00%	0.001%
34	4.760	1155	1157	1159	rVV2	698	345	0.00%	0.001%
35	4.828	1167	1178	1193	rBV4	8241	19834	0.11%	0.033%
36	4.931	1208	1210	1213	rVB2	628	290	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021125.D
 Acq On : 23 Apr 2021 17:26
 Operator : SY/MD
 Sample : M2144-05 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	4.957	1214	1218	1219	rBV3	621	367	0.00%	0.001%
38	5.050	1231	1247	1256	rBV2	927680	2347696	12.50%	3.945%
39	5.619	1412	1424	1446	rBV	780177	1589942	8.46%	2.672%
40	5.876	1501	1504	1505	rBV2	1208	620	0.00%	0.001%
41	6.075	1551	1566	1592	rBV	514751	1060372	5.64%	1.782%
42	6.391	1661	1664	1667	rBV3	1592	1153	0.01%	0.002%
43	6.419	1670	1673	1677	rVB4	782	593	0.00%	0.001%
44	6.439	1677	1679	1681	rBV3	545	287	0.00%	0.000%
45	6.548	1711	1713	1714	rVB2	791	304	0.00%	0.001%
46	6.645	1739	1743	1745	rBV2	871	498	0.00%	0.001%
47	6.722	1761	1767	1769	rBV4	956	727	0.00%	0.001%
48	6.844	1803	1805	1807	rBV2	583	322	0.00%	0.001%
49	6.882	1815	1817	1821	rBV2	509	319	0.00%	0.001%
50	6.905	1821	1824	1829	rBV3	1115	1078	0.01%	0.002%
51	6.989	1840	1850	1880	rBV	293656	546783	2.91%	0.919%
52	7.233	1924	1926	1930	rVB3	1205	737	0.00%	0.001%
53	7.320	1940	1953	1972	rBV	1075065	1860025	9.90%	3.126%
54	7.574	2026	2032	2037	rVB7	1064	1190	0.01%	0.002%
55	7.625	2037	2048	2080	rBV	206555	379390	2.02%	0.638%
56	7.972	2154	2156	2157	rBV2	832	327	0.00%	0.001%
57	8.095	2181	2194	2217	rBV	605554	1098968	5.85%	1.847%
58	8.603	2349	2352	2356	rBV3	684	573	0.00%	0.001%
59	8.709	2383	2385	2388	rVB4	704	275	0.00%	0.000%
60	8.773	2402	2405	2407	rBV4	722	527	0.00%	0.001%
61	8.886	2419	2440	2469	rBV2	10641632	18786206	100.00%	31.568%
62	9.403	2599	2601	2605	rBV3	639	567	0.00%	0.001%
63	9.673	2682	2685	2689	rBV4	947	914	0.00%	0.002%
64	9.712	2695	2697	2702	rBV3	692	373	0.00%	0.001%
65	9.741	2702	2706	2709	rVB4	804	574	0.00%	0.001%
66	9.779	2713	2718	2720	rBV3	685	575	0.00%	0.001%
67	9.889	2750	2752	2756	rBV3	705	547	0.00%	0.001%
68	9.911	2756	2759	2760	rBV	909	473	0.00%	0.001%
69	9.976	2777	2779	2782	rBV	685	397	0.00%	0.001%
70	10.053	2800	2803	2806	rBV3	397	341	0.00%	0.001%
71	10.136	2817	2829	2832	rBV6	3834	5723	0.03%	0.010%
72	10.172	2838	2840	2842	rBV	951	482	0.00%	0.001%
73	10.220	2843	2855	2876	rVV	835276	1311851	6.98%	2.204%
74	10.342	2891	2893	2895	rBV2	765	297	0.00%	0.000%
75	10.779	3025	3029	3032	rBV2	770	580	0.00%	0.001%
76	10.802	3032	3036	3038	rVV5	810	673	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021125.D
 Acq On : 23 Apr 2021 17:26
 Operator : SY/MD
 Sample : M2144-05 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GH5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

77	10.815	3038	3040	3042	rVB	1010	381	0.00%	0.001%
78	10.847	3048	3050	3055	rBV5	1250	928	0.00%	0.002%
79	10.924	3065	3074	3080	rBV9	4192	5935	0.03%	0.010%
80	11.040	3107	3110	3112	rBV2	975	560	0.00%	0.001%
81	11.114	3130	3133	3136	rVB2	858	543	0.00%	0.001%
82	11.188	3146	3156	3167	rBV	680407	1031742	5.49%	1.734%
83	11.278	3167	3184	3210	rVB2	5750876	10728205	57.11%	18.027%
84	11.648	3282	3299	3321	rBV2	7450054	13071173	69.58%	21.964%
85	12.024	3414	3416	3420	rBV3	1316	725	0.00%	0.001%
86	12.185	3463	3466	3468	rBV2	794	491	0.00%	0.001%
87	12.197	3468	3470	3474	rVB3	1179	755	0.00%	0.001%
88	12.307	3502	3504	3506	rVB2	1373	513	0.00%	0.001%
89	12.329	3509	3511	3513	rBV	923	508	0.00%	0.001%
90	12.377	3524	3526	3528	rBV2	772	422	0.00%	0.001%
91	12.410	3528	3536	3543	rVV4	8251	12809	0.07%	0.022%
92	12.660	3607	3614	3622	rBV10	4233	5659	0.03%	0.010%
93	12.763	3638	3646	3653	rBV10	4031	7446	0.04%	0.013%
94	12.982	3712	3714	3715	rBV	645	297	0.00%	0.000%
95	13.191	3777	3779	3781	rVB2	819	298	0.00%	0.001%
96	13.204	3781	3783	3785	rBV2	626	378	0.00%	0.001%
97	13.268	3791	3803	3827	rBV	1374037	2095949	11.16%	3.522%
98	13.493	3870	3873	3876	rBV4	1066	1073	0.01%	0.002%
99	13.754	3942	3954	3966	rBV	336675	524320	2.79%	0.881%
100	13.940	4010	4012	4016	rBV2	1066	649	0.00%	0.001%




Sum of corrected areas: 59510665

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021125.D
Acq On : 23 Apr 2021 17:26
Operator : SY/MD
Sample : M2144-05 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

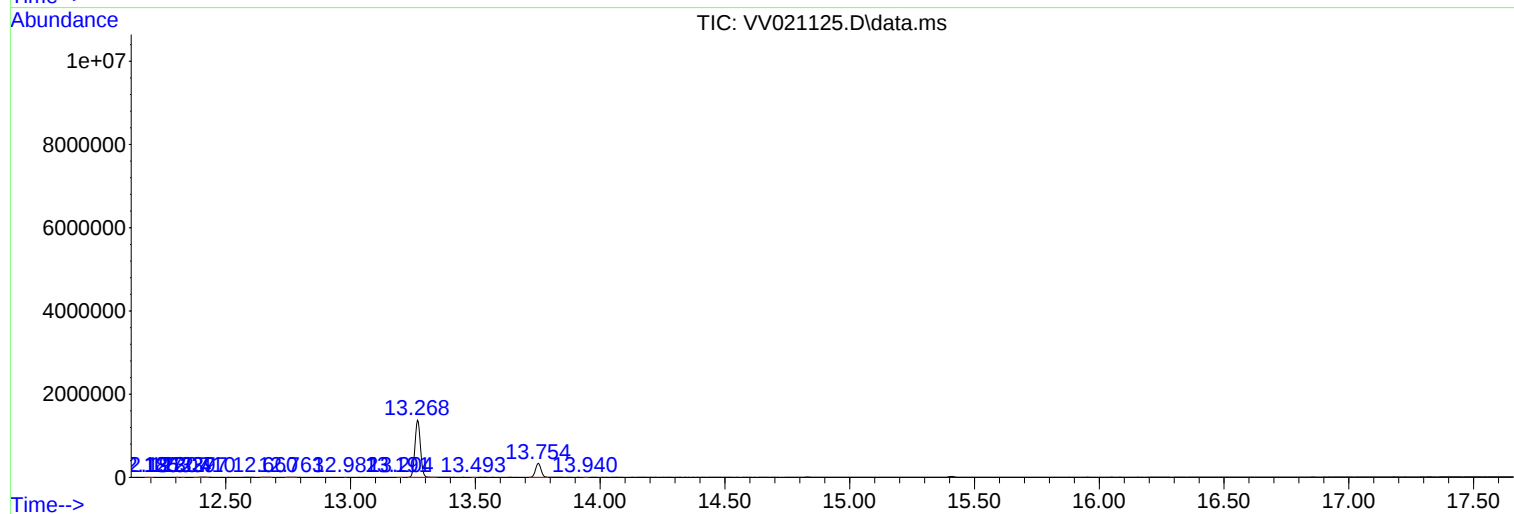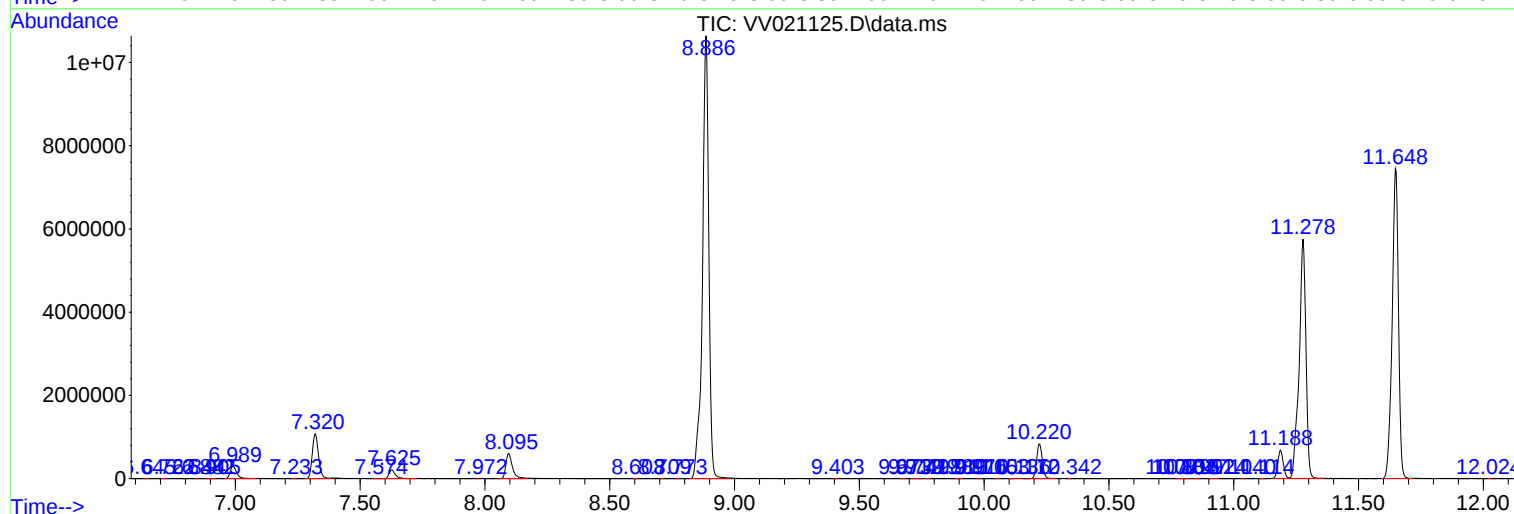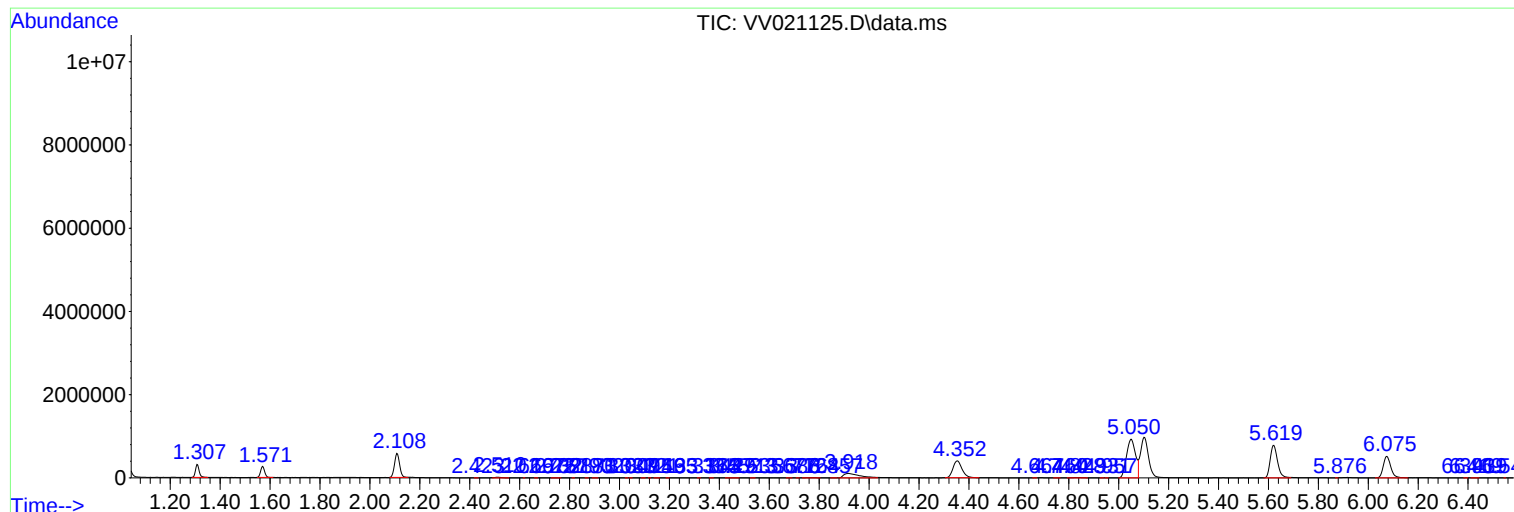

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021125.D
Acq On : 23 Apr 2021 17:26
Operator : SY/MD
Sample : M2144-05 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021125.D
Acq On : 23 Apr 2021 17:26
Operator : SY/MD
Sample : M2144-05 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GH5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
