

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021129.D
 Acq On : 23 Apr 2021 19:23
 Operator : SY/MD
 Sample : M2123-01 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021129.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	278269	289047	13.08%	1.612%
2	1.571	158	165	183	rVB	245175	281906	12.75%	1.573%
3	2.108	322	332	344	rBV	524084	746381	33.77%	4.164%
4	2.510	449	457	468	rVB4	5654	8473	0.38%	0.047%
5	2.574	474	477	479	rBV2	374	238	0.01%	0.001%
6	2.629	490	494	498	rBV3	792	642	0.03%	0.004%
7	2.648	498	500	503	rBV2	484	316	0.01%	0.002%
8	2.728	520	525	527	rBV4	615	617	0.03%	0.003%
9	2.760	532	535	539	rBV5	815	649	0.03%	0.004%
10	2.854	561	564	566	rBV	738	404	0.02%	0.002%
11	3.005	608	611	616	rVB3	706	498	0.02%	0.003%
12	3.040	620	622	624	rBV	494	225	0.01%	0.001%
13	3.085	631	636	638	rVB2	564	443	0.02%	0.002%
14	3.114	640	645	649	rVB2	712	682	0.03%	0.004%
15	3.140	649	653	654	rBV2	664	550	0.02%	0.003%
16	3.162	658	660	662	rBV	755	460	0.02%	0.003%
17	3.246	684	686	692	rVB3	786	564	0.03%	0.003%
18	3.281	692	697	698	rBV2	881	703	0.03%	0.004%
19	3.333	709	713	716	rBV3	549	445	0.02%	0.002%
20	3.349	716	718	721	rVB	431	228	0.01%	0.001%
21	3.368	721	724	730	rBV3	826	905	0.04%	0.005%
22	3.416	735	739	740	rBV	449	251	0.01%	0.001%
23	3.477	755	758	759	rBV2	480	282	0.01%	0.002%
24	3.497	763	764	767	rVB3	875	345	0.02%	0.002%
25	3.558	780	783	787	rVB2	393	322	0.01%	0.002%
26	3.590	791	793	795	rBV2	571	261	0.01%	0.001%
27	3.651	809	812	815	rBV	335	281	0.01%	0.002%
28	3.751	840	843	846	rVB2	598	362	0.02%	0.002%
29	3.841	869	871	874	rVB3	568	334	0.02%	0.002%
30	3.912	881	893	936	rBV	111029	449676	20.35%	2.509%
31	4.352	1015	1030	1054	rBV2	384217	953769	43.15%	5.321%
32	4.735	1146	1149	1150	rBV2	610	321	0.01%	0.002%
33	4.796	1164	1168	1171	rBV2	699	580	0.03%	0.003%
34	4.902	1199	1201	1205	rBV3	665	473	0.02%	0.003%
35	4.956	1216	1218	1220	rBV2	456	278	0.01%	0.002%
36	5.050	1230	1247	1274	rBV2	866406	2210249	100.00%	12.330%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021129.D
 Acq On : 23 Apr 2021 19:23
 Operator : SY/MD
 Sample : M2123-01 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	5.458	1372	1374	1379	rBV4	900	795	0.04%	0.004%
38	5.497	1383	1386	1388	rBV	719	536	0.02%	0.003%
39	5.622	1412	1425	1454	rBV	802674	1616321	73.13%	9.017%
40	5.911	1506	1515	1531	rVB6	11238	24743	1.12%	0.138%
41	6.024	1548	1550	1552	rBV2	438	267	0.01%	0.001%
42	6.075	1552	1566	1593	rVV	489483	1011346	45.76%	5.642%
43	6.355	1650	1653	1655	rBV3	749	575	0.03%	0.003%
44	6.506	1697	1700	1703	rBV3	820	533	0.02%	0.003%
45	6.538	1709	1710	1713	rVB2	949	328	0.01%	0.002%
46	6.564	1713	1718	1720	rBV2	821	865	0.04%	0.005%
47	6.686	1752	1756	1757	rBV	537	368	0.02%	0.002%
48	6.744	1772	1774	1777	rVB2	817	438	0.02%	0.002%
49	6.815	1794	1796	1798	rBV	432	218	0.01%	0.001%
50	6.924	1827	1830	1836	rBV4	722	797	0.04%	0.004%
51	6.992	1839	1851	1880	rBV	270098	509483	23.05%	2.842%
52	7.268	1935	1937	1940	rVB3	739	332	0.02%	0.002%
53	7.320	1940	1953	1971	rBV	991354	1710230	77.38%	9.541%
54	7.587	2033	2036	2037	rBV	661	387	0.02%	0.002%
55	7.625	2037	2048	2069	rVV2	189130	342608	15.50%	1.911%
56	7.837	2112	2114	2115	rBV2	722	295	0.01%	0.002%
57	8.095	2184	2194	2231	rBV	555312	1048121	47.42%	5.847%
58	8.345	2269	2272	2275	rBV3	1707	925	0.04%	0.005%
59	8.480	2312	2314	2317	rVB4	1415	742	0.03%	0.004%
60	8.564	2337	2340	2342	rBV3	685	411	0.02%	0.002%
61	8.628	2358	2360	2363	rBV	698	328	0.01%	0.002%
62	8.712	2384	2386	2390	rVB2	747	431	0.02%	0.002%
63	8.857	2418	2431	2449	rBV	1204175	1946198	88.05%	10.857%
64	9.146	2517	2521	2522	rBV3	1708	1146	0.05%	0.006%
65	9.214	2540	2542	2545	rBV2	621	301	0.01%	0.002%
66	9.291	2564	2566	2568	rBV2	519	277	0.01%	0.002%
67	9.426	2603	2608	2611	rBV4	887	854	0.04%	0.005%
68	9.474	2621	2623	2625	rBV3	479	255	0.01%	0.001%
69	9.487	2625	2627	2629	rVV	658	254	0.01%	0.001%
70	9.519	2636	2637	2642	rVB2	570	293	0.01%	0.002%
71	9.558	2644	2649	2651	rBV2	1063	984	0.04%	0.005%
72	9.628	2669	2671	2674	rBV	648	301	0.01%	0.002%
73	9.718	2698	2699	2702	rBV	432	265	0.01%	0.001%
74	9.844	2736	2738	2740	rBV2	551	245	0.01%	0.001%
75	9.972	2775	2778	2780	rBV	489	322	0.01%	0.002%
76	10.017	2787	2792	2797	rVB4	855	845	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021129.D
 Acq On : 23 Apr 2021 19:23
 Operator : SY/MD
 Sample : M2123-01 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	10.095	2814	2816	2818	rBV	777	436	0.02%	0.002%
78	10.136	2822	2829	2838	rVB6	4378	4991	0.23%	0.028%
79	10.223	2842	2856	2876	rBV	788106	1231194	55.70%	6.868%
80	10.458	2925	2929	2931	rBV3	1524	1039	0.05%	0.006%
81	10.493	2938	2940	2942	rBV3	788	346	0.02%	0.002%
82	10.670	2993	2995	2998	rBV2	544	257	0.01%	0.001%
83	10.702	3002	3005	3006	rBV2	398	229	0.01%	0.001%
84	10.882	3059	3061	3063	rVB3	529	227	0.01%	0.001%
85	10.924	3070	3074	3082	rVB7	3429	4537	0.21%	0.025%
86	10.985	3091	3093	3095	rBV2	587	307	0.01%	0.002%
87	11.156	3138	3146	3149	rBV5	2406	2719	0.12%	0.015%
88	11.194	3155	3158	3160	rBV3	820	554	0.03%	0.003%
89	11.255	3166	3177	3202	rBV	1172716	1804699	81.65%	10.068%
90	11.538	3263	3265	3268	rVB3	680	339	0.02%	0.002%
91	11.586	3276	3280	3281	rBV3	696	495	0.02%	0.003%
92	11.631	3281	3294	3311	rBV	1053814	1685362	76.25%	9.402%
93	11.802	3344	3347	3349	rBV3	1422	945	0.04%	0.005%
94	11.850	3359	3362	3363	rBV2	978	656	0.03%	0.004%
95	12.307	3496	3504	3505	rBV4	1335	1345	0.06%	0.008%
96	12.596	3591	3594	3595	rBV3	777	520	0.02%	0.003%
97	12.660	3610	3614	3616	rBV3	1137	946	0.04%	0.005%
98	12.834	3663	3668	3671	rBV4	1287	1171	0.05%	0.007%
99	12.963	3706	3708	3709	rBV4	679	290	0.01%	0.002%
100	14.040	4040	4043	4046	rBV	7273	4765	0.22%	0.027%




Sum of corrected areas: 17925492

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021129.D
Acq On : 23 Apr 2021 19:23
Operator : SY/MD
Sample : M2123-01 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

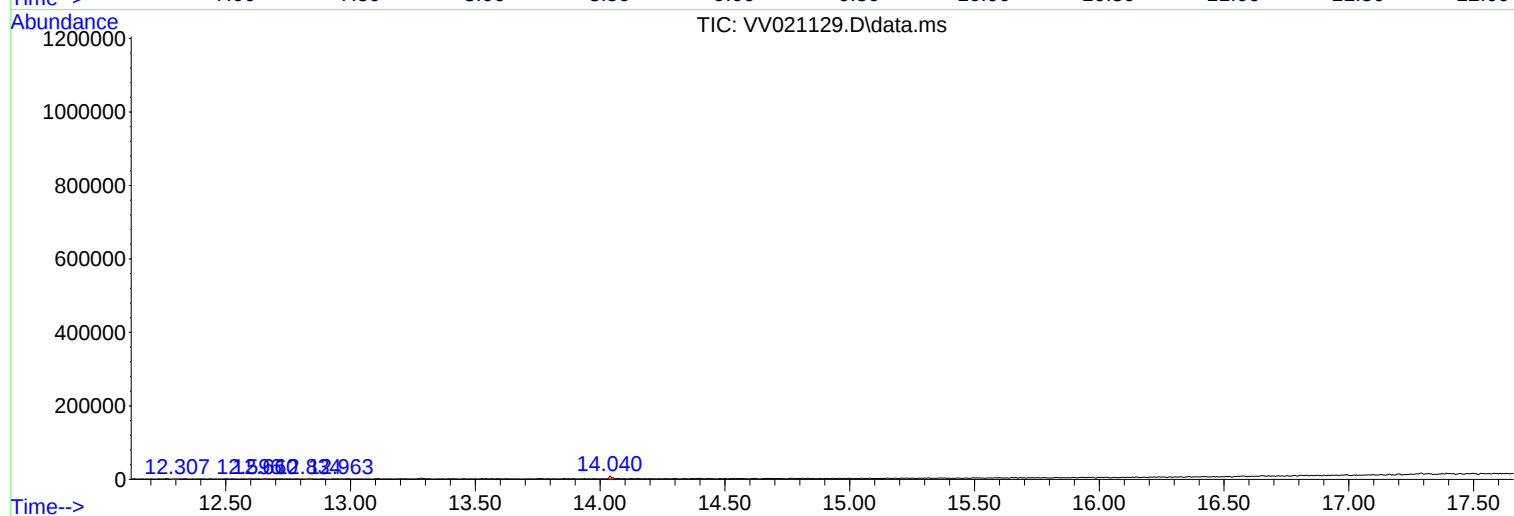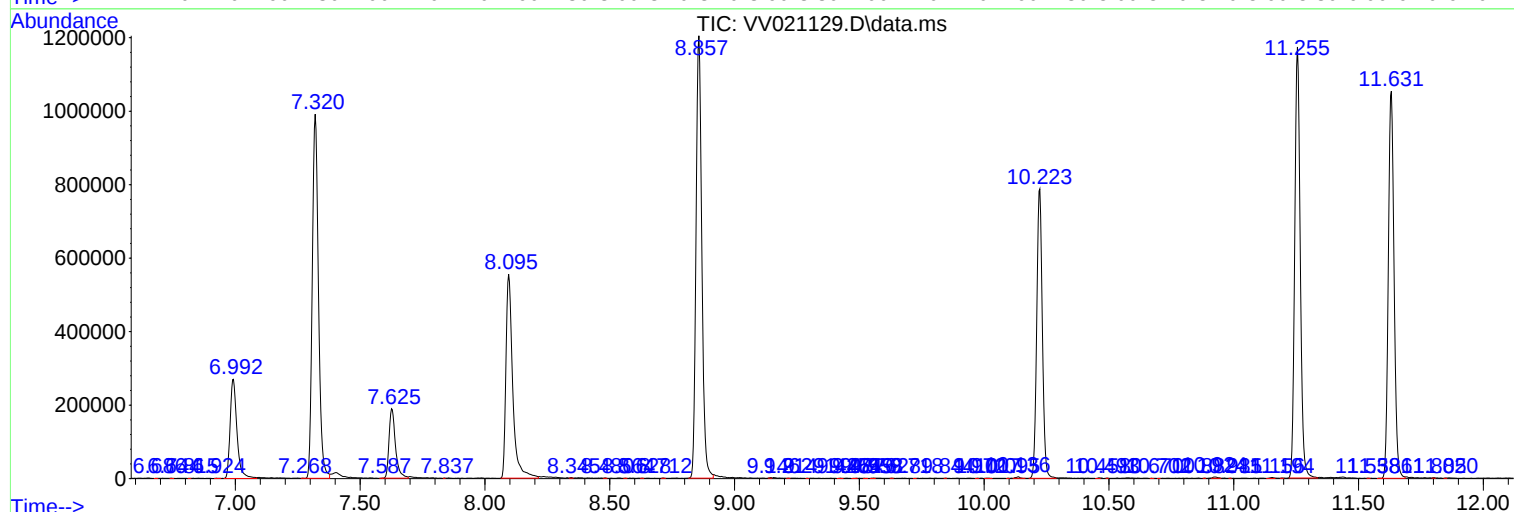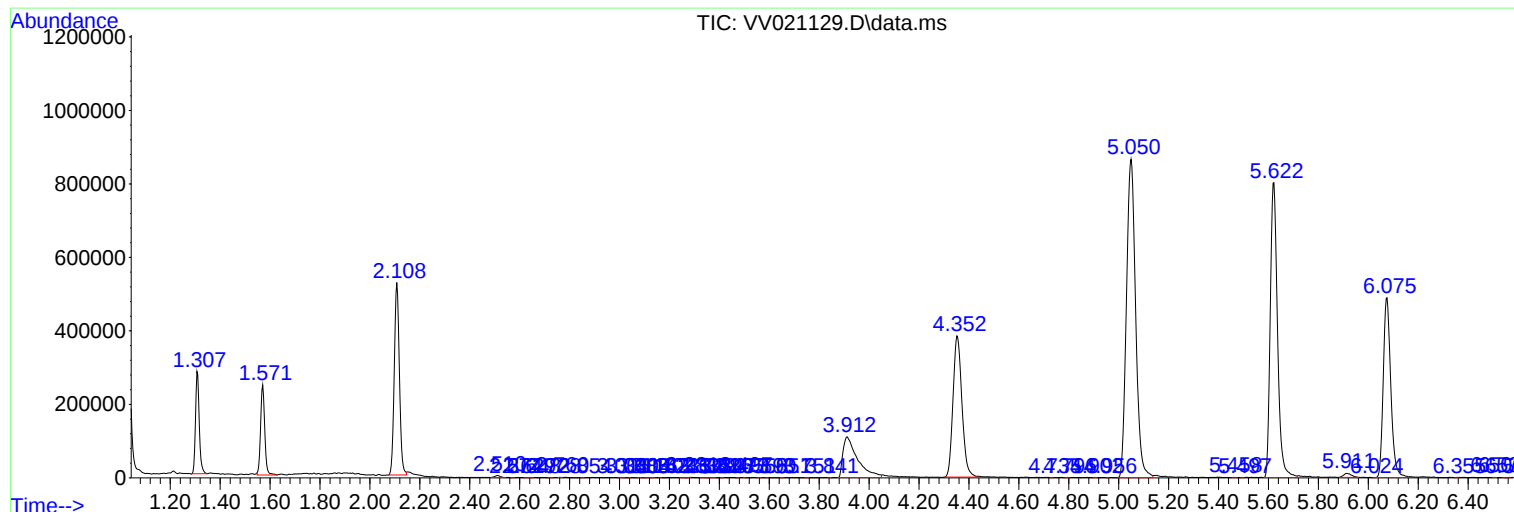

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021129.D
Acq On : 23 Apr 2021 19:23
Operator : SY/MD
Sample : M2123-01 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021129.D
Acq On : 23 Apr 2021 19:23
Operator : SY/MD
Sample : M2123-01 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------