

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021130.D
 Acq On : 23 Apr 2021 19:47
 Operator : SY/MD
 Sample : M2123-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021130.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	99	rVB	283752	286704	13.13%	1.647%
2	1.571	158	165	174	rVB	232325	264383	12.11%	1.519%
3	2.108	323	332	353	rVB	515849	740235	33.89%	4.253%
4	2.439	433	435	441	rBV5	1050	1090	0.05%	0.006%
5	2.510	450	457	471	rVV6	6861	11276	0.52%	0.065%
6	2.567	471	475	477	rVB	884	587	0.03%	0.003%
7	2.603	484	486	489	rBV2	584	375	0.02%	0.002%
8	2.654	499	502	504	rVV3	1004	561	0.03%	0.003%
9	2.667	504	506	510	rVB	617	394	0.02%	0.002%
10	2.847	560	562	564	rBV	574	322	0.01%	0.002%
11	2.940	588	591	595	rBV4	566	408	0.02%	0.002%
12	3.008	609	612	616	rBV2	540	346	0.02%	0.002%
13	3.063	627	629	633	rVB3	701	312	0.01%	0.002%
14	3.092	636	638	643	rVB3	549	476	0.02%	0.003%
15	3.121	643	647	650	rBV3	637	562	0.03%	0.003%
16	3.214	672	676	677	rBV	622	324	0.01%	0.002%
17	3.223	677	679	682	rVB3	714	319	0.01%	0.002%
18	3.294	696	701	704	rBV4	732	599	0.03%	0.003%
19	3.333	711	713	716	rBV	553	371	0.02%	0.002%
20	3.365	721	723	729	rVB3	1164	1118	0.05%	0.006%
21	3.394	729	732	734	rBV2	553	316	0.01%	0.002%
22	3.426	739	742	745	rBV2	708	511	0.02%	0.003%
23	3.503	762	766	767	rBV3	614	383	0.02%	0.002%
24	3.545	777	779	783	rVB2	798	527	0.02%	0.003%
25	3.577	784	789	791	rBV	437	350	0.02%	0.002%
26	3.667	815	817	821	rBV3	427	273	0.01%	0.002%
27	3.690	821	824	829	rVB4	632	416	0.02%	0.002%
28	3.731	833	837	838	rBV2	469	290	0.01%	0.002%
29	3.915	882	894	896	rBV2	89093	134033	6.14%	0.770%
30	4.352	1014	1030	1060	rBV	375484	948096	43.41%	5.448%
31	4.667	1125	1128	1132	rVB2	784	498	0.02%	0.003%
32	4.686	1132	1134	1136	rBV2	651	287	0.01%	0.002%
33	4.699	1136	1138	1140	rBV2	594	281	0.01%	0.002%
34	4.764	1156	1158	1162	rBV	621	482	0.02%	0.003%
35	4.844	1181	1183	1187	rVB3	1232	693	0.03%	0.004%
36	4.873	1187	1192	1196	rBV3	998	1082	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021130.D
 Acq On : 23 Apr 2021 19:47
 Operator : SY/MD
 Sample : M2123-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	4.992	1226	1229	1230	rBV2	811	436	0.02%	0.003%
38	5.050	1231	1247	1285	rVV2	848549	2183937	100.00%	12.549%
39	5.307	1324	1327	1329	rBV2	1863	1093	0.05%	0.006%
40	5.622	1408	1425	1452	rBV	790765	1596744	73.11%	9.175%
41	5.918	1506	1517	1537	rVB6	10523	25288	1.16%	0.145%
42	6.001	1541	1543	1546	rBV4	1252	608	0.03%	0.003%
43	6.075	1552	1566	1587	rBV	476540	988114	45.24%	5.678%
44	6.352	1650	1652	1655	rBV2	704	366	0.02%	0.002%
45	6.387	1661	1663	1666	rVB4	829	472	0.02%	0.003%
46	6.423	1672	1674	1678	rVB3	879	462	0.02%	0.003%
47	6.673	1750	1752	1754	rVB2	709	297	0.01%	0.002%
48	6.735	1769	1771	1773	rVB4	937	361	0.02%	0.002%
49	6.751	1773	1776	1778	rVV2	487	273	0.01%	0.002%
50	6.808	1792	1794	1796	rBV	537	323	0.01%	0.002%
51	6.886	1816	1818	1822	rVB3	831	548	0.03%	0.003%
52	6.908	1822	1825	1829	rVB3	907	585	0.03%	0.003%
53	6.937	1829	1834	1837	rBV3	687	499	0.02%	0.003%
54	6.992	1837	1851	1871	rBV	263630	487396	22.32%	2.801%
55	7.201	1912	1916	1917	rBV3	1113	681	0.03%	0.004%
56	7.278	1938	1940	1941	rBV3	728	389	0.02%	0.002%
57	7.320	1941	1953	1972	rBV	968168	1687238	77.26%	9.695%
58	7.625	2038	2048	2066	rBV	185716	327864	15.01%	1.884%
59	7.802	2100	2103	2104	rBV2	751	437	0.02%	0.003%
60	7.844	2113	2116	2121	rVB4	1250	953	0.04%	0.005%
61	7.876	2121	2126	2128	rBV4	1166	852	0.04%	0.005%
62	7.982	2156	2159	2169	rVB7	1396	1662	0.08%	0.010%
63	8.046	2176	2179	2183	rBV2	564	404	0.02%	0.002%
64	8.095	2183	2194	2220	rBV	526661	977048	44.74%	5.614%
65	8.680	2373	2376	2380	rBV3	1259	841	0.04%	0.005%
66	8.770	2402	2404	2407	rBV	650	293	0.01%	0.002%
67	8.799	2411	2413	2416	rBV2	450	310	0.01%	0.002%
68	8.857	2420	2431	2459	rBV	1170295	1937634	88.72%	11.134%
69	9.149	2519	2522	2523	rBV2	1405	817	0.04%	0.005%
70	9.259	2553	2556	2558	rBV2	784	457	0.02%	0.003%
71	9.455	2615	2617	2621	rVB2	712	442	0.02%	0.003%
72	9.474	2621	2623	2628	rBV3	484	335	0.02%	0.002%
73	9.599	2659	2662	2663	rBV2	427	272	0.01%	0.002%
74	9.648	2673	2677	2681	rBV2	863	713	0.03%	0.004%
75	9.686	2687	2689	2691	rBV3	918	429	0.02%	0.002%
76	9.860	2740	2743	2747	rBV5	658	520	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
 Data File : VV021130.D
 Acq On : 23 Apr 2021 19:47
 Operator : SY/MD
 Sample : M2123-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7A5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	9.892	2751	2753	2755	rBV2	448	279	0.01%	0.002%
78	10.075	2808	2810	2814	rVB3	553	302	0.01%	0.002%
79	10.136	2822	2829	2834	rVB7	3104	3579	0.16%	0.021%
80	10.223	2843	2856	2880	rVB	766463	1207096	55.27%	6.936%
81	10.310	2881	2883	2885	rBV3	702	367	0.02%	0.002%
82	10.432	2919	2921	2924	rBV3	826	596	0.03%	0.003%
83	10.471	2930	2933	2935	rVB	606	339	0.02%	0.002%
84	10.509	2942	2945	2947	rBV3	688	446	0.02%	0.003%
85	10.541	2952	2955	2957	rBV2	489	312	0.01%	0.002%
86	10.699	3001	3004	3010	rVB3	691	739	0.03%	0.004%
87	10.853	3049	3052	3057	rBV5	1494	1289	0.06%	0.007%
88	11.037	3106	3109	3116	rBV5	958	1177	0.05%	0.007%
89	11.088	3122	3125	3126	rBV	753	374	0.02%	0.002%
90	11.149	3140	3144	3148	rBV4	1738	1582	0.07%	0.009%
91	11.181	3153	3154	3156	rBV2	783	324	0.01%	0.002%
92	11.255	3165	3177	3206	rBV	1183985	1848771	84.65%	10.623%
93	11.631	3282	3294	3316	rBV	1083114	1704771	78.06%	9.796%
94	11.885	3370	3373	3377	rBV5	713	618	0.03%	0.004%
95	12.287	3495	3498	3501	rBV2	990	672	0.03%	0.004%
96	12.802	3656	3658	3660	rBV	567	276	0.01%	0.002%
97	13.226	3788	3790	3792	rBV3	752	371	0.02%	0.002%
98	13.358	3829	3831	3835	rBV2	828	457	0.02%	0.003%
99	13.522	3880	3882	3884	rBV3	652	297	0.01%	0.002%
100	14.098	4059	4061	4065	rBV3	940	660	0.03%	0.004%


Sum of corrected areas: 17403367

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021130.D
Acq On : 23 Apr 2021 19:47
Operator : SY/MD
Sample : M2123-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BG7A5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

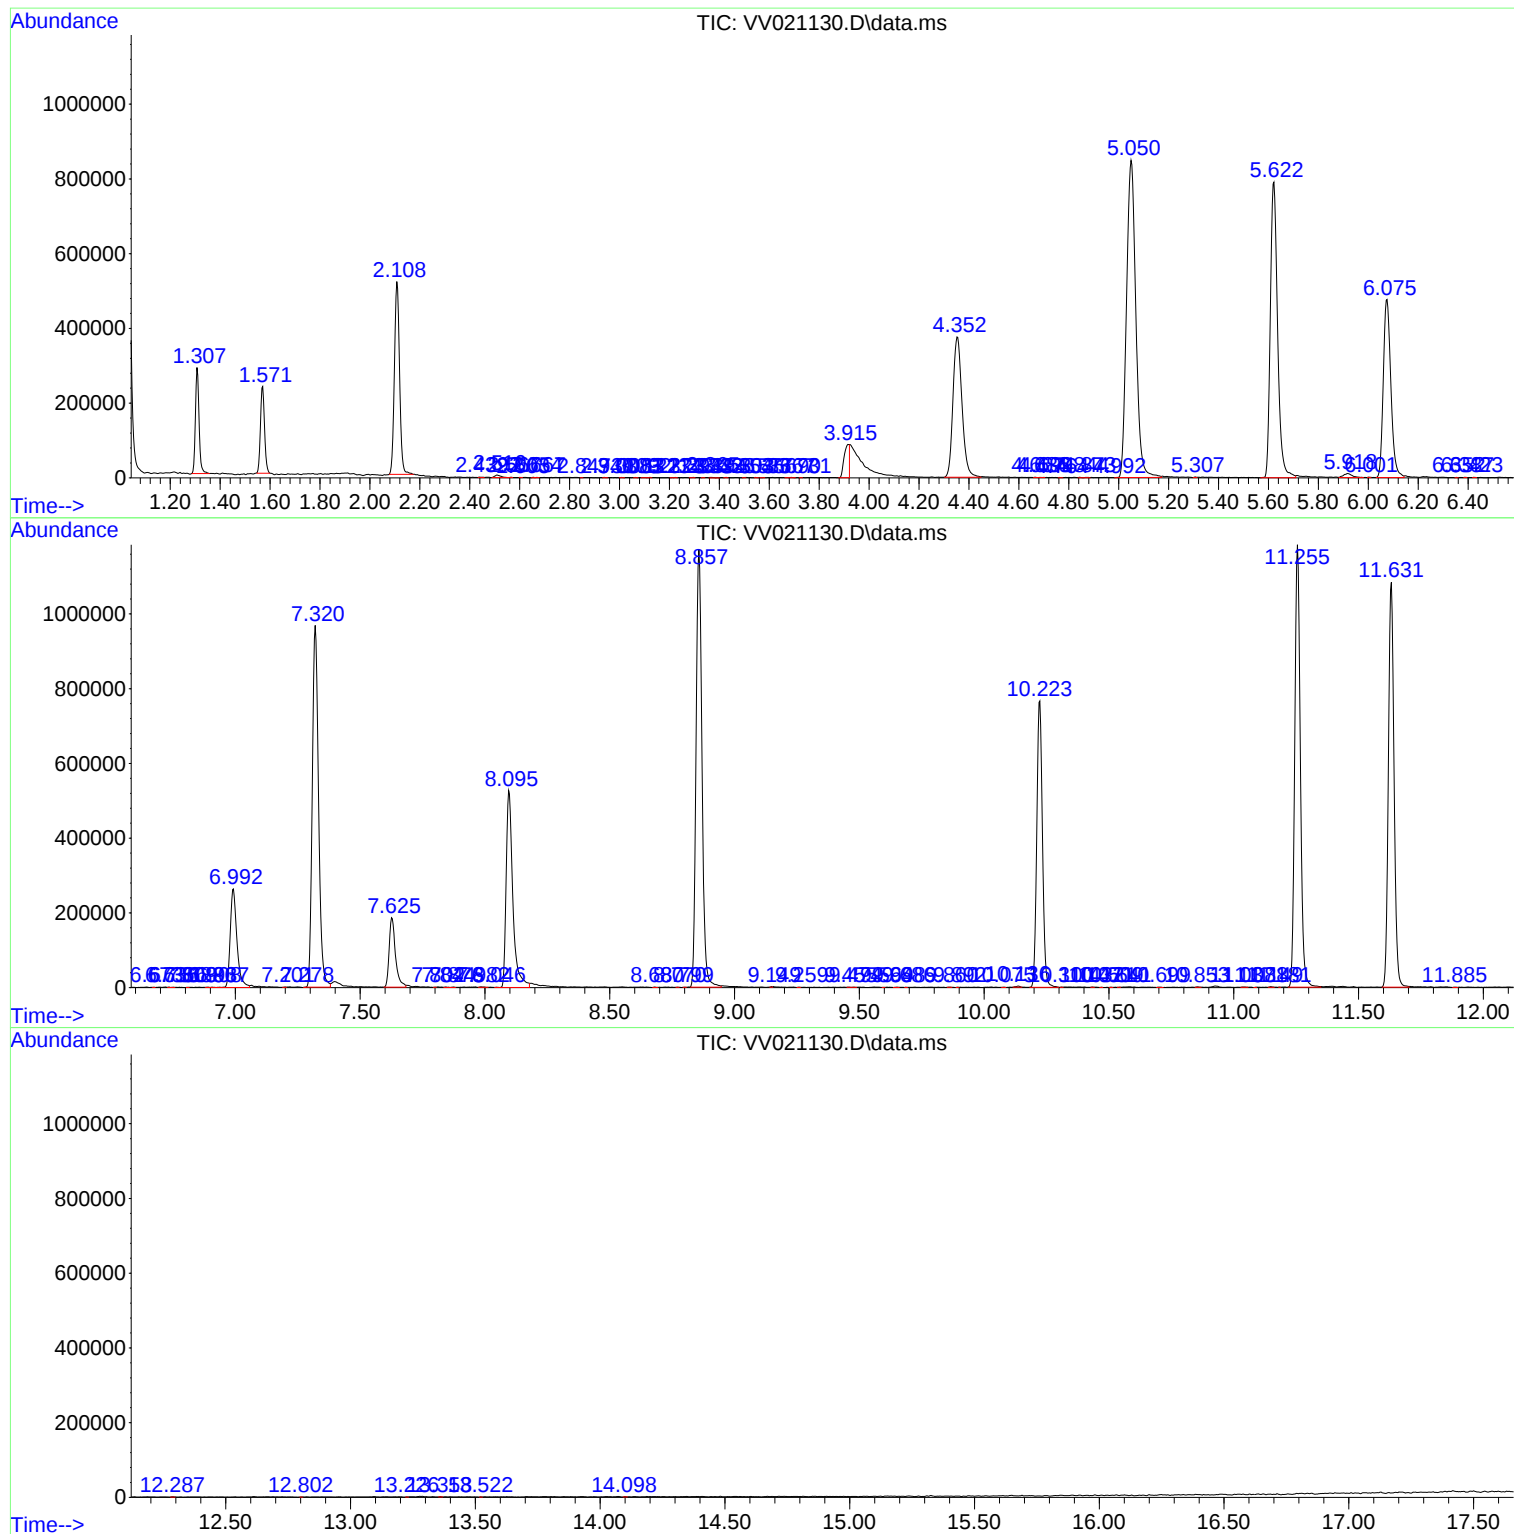

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021130.D
Acq On : 23 Apr 2021 19:47
Operator : SY/MD
Sample : M2123-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042321\
Data File : VV021130.D
Acq On : 23 Apr 2021 19:47
Operator : SY/MD
Sample : M2123-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7A5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------