

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042324\
 Data File : VW035355.D
 Acq On : 23 Apr 2024 12:51
 Operator : SY/MD
 Sample : P2157-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCOR81

Quant Time: Apr 24 00:39:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 23 23:26:51 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	385873	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	396856	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	182299	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	180941	48.554	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	97.100%		
7) Chloroethane-d5	1.532	69	146761	45.342	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	90.680%		
11) 1,1-Dichloroethene-d2	2.060	65	74043	45.326	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.660%		
21) 2-Butanone-d5	3.786	46	194940	88.202	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	88.200%		
24) Chloroform-d	4.246	84	310314	49.527	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.060%		
26) 1,2-Dichloroethane-d4	4.940	65	194256	48.833	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.660%		
32) Benzene-d6	4.957	84	625232	46.902	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.800%		
36) 1,2-Dichloropropane-d6	5.985	67	202675	47.878	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.760%		
41) Toluene-d8	7.243	98	540687	45.037	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.080%		
43) trans-1,3-Dichloroprop...	7.551	79	83235	40.446	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.900%		
47) 2-Hexanone-d5	8.024	63	108838	68.004	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	68.000%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	273906	46.988	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.980%		
66) 1,2-Dichlorobenzene-d4	11.558	152	216618	52.924	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	105.840%		
Target Compounds					Qvalue	
13) Acetone	2.114	43	9151	4.510	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035355.D
Acq On : 23 Apr 2024 12:51
Operator : SY/MD
Sample : P2157-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R81

Quant Time: Apr 24 00:39:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 23 23:26:51 2024
Response via : Initial Calibration

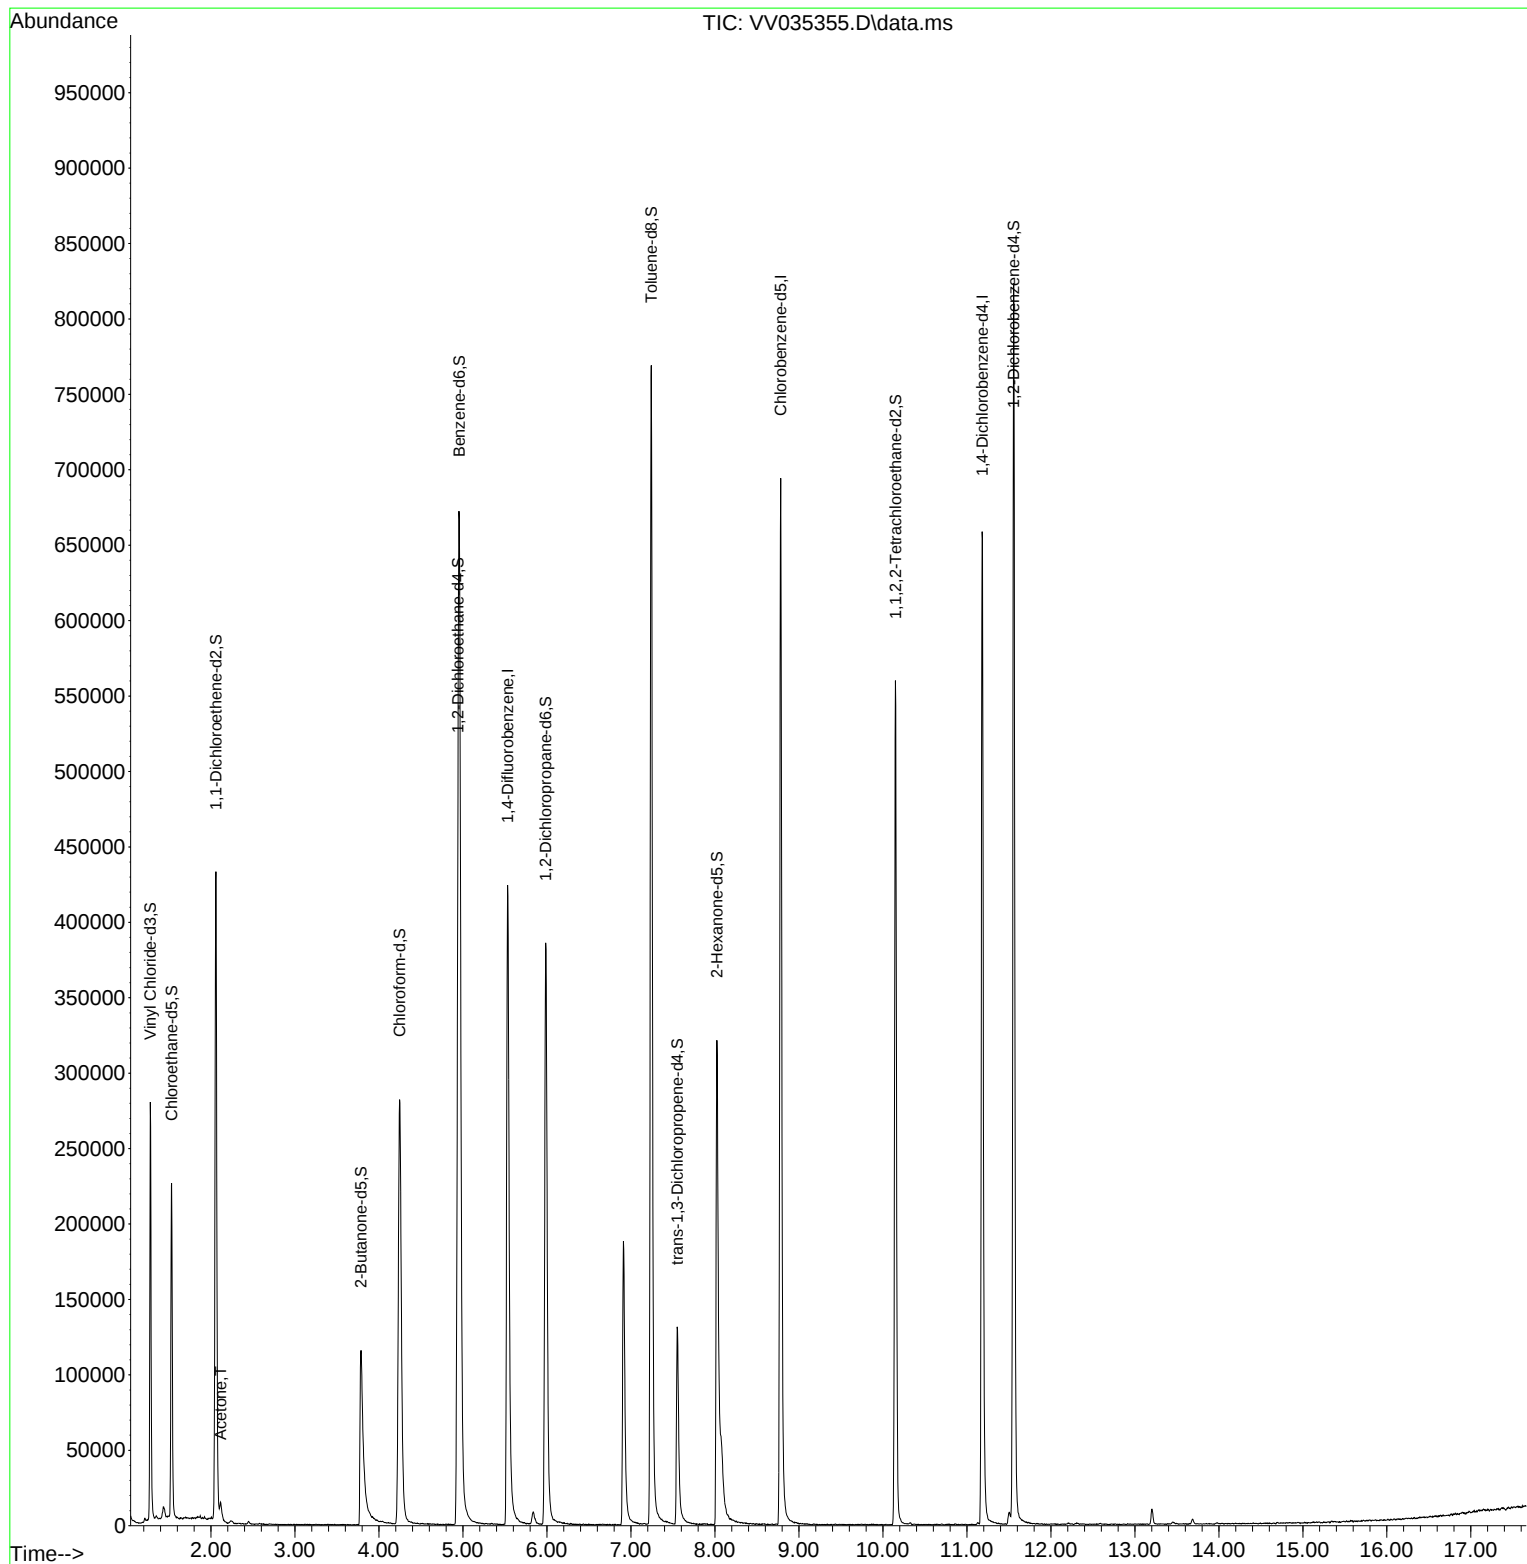

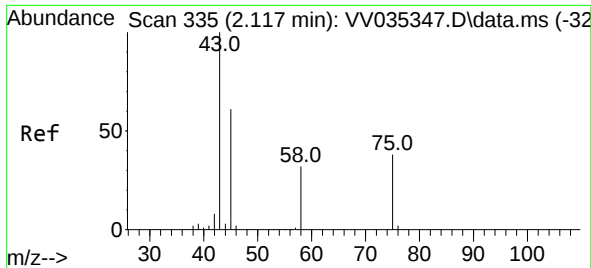

#13

Acetone

Concen: 4.510 ug/L

RT: 2.114 min Scan# 31

Delta R.T. -0.003 min

Lab File: VV035355.D


Acq: 23 Apr 2024 12:51

Instrument :

MSVOA_V

ClientSampleId :

MC0R81

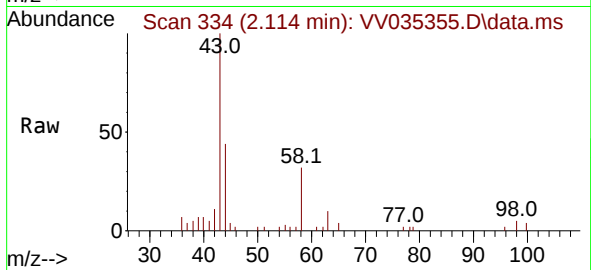

Tgt Ion: 43 Resp: 9151

Ion Ratio Lower Upper

43 100

58 33.7 0.0 66.0

