

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035349.D
 Acq On : 23 Apr 2024 10:32
 Operator : SY/MD
 Sample : P2170-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035349.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	60	rBV4	2589	3611	0.19%	0.027%
2	1.281	67	75	89	rBV	288832	308312	16.43%	2.269%
3	1.532	146	153	172	rVB	240205	283514	15.11%	2.086%
4	2.059	306	317	331	rBV	457587	665085	35.45%	4.894%
5	2.243	368	374	378	rBV3	1222	1572	0.08%	0.012%
6	2.320	395	398	403	rVB5	847	694	0.04%	0.005%
7	2.342	403	405	408	rBV	569	331	0.02%	0.002%
8	2.449	430	438	445	rBV7	1570	2328	0.12%	0.017%
9	2.506	453	456	459	rVB	391	248	0.01%	0.002%
10	2.545	465	468	471	rBV	356	237	0.01%	0.002%
11	2.564	471	474	476	rBV2	396	262	0.01%	0.002%
12	2.587	476	481	486	rVV3	654	679	0.04%	0.005%
13	2.613	486	489	496	rVB6	564	574	0.03%	0.004%
14	2.664	503	505	509	rVB2	413	276	0.01%	0.002%
15	2.706	509	518	522	rBV5	891	1319	0.07%	0.010%
16	2.834	556	558	563	rBV	434	377	0.02%	0.003%
17	3.095	636	639	643	rBV	277	233	0.01%	0.002%
18	3.175	662	664	670	rVV2	239	233	0.01%	0.002%
19	3.217	674	677	680	rVV2	337	231	0.01%	0.002%
20	3.252	684	688	690	rVV	377	353	0.02%	0.003%
21	3.503	761	766	770	rBV2	328	272	0.01%	0.002%
22	3.577	785	789	797	rVB3	255	287	0.02%	0.002%
23	3.622	797	803	809	rVB2	288	328	0.02%	0.002%
24	3.654	809	813	817	rVB2	309	237	0.01%	0.002%
25	3.686	821	823	826	rBV2	433	266	0.01%	0.002%
26	3.789	846	855	898	rBV	110566	338578	18.05%	2.491%
27	4.246	980	997	1029	rBV	296541	760627	40.54%	5.597%
28	4.513	1078	1080	1084	rBV3	279	238	0.01%	0.002%
29	4.532	1084	1086	1090	rVB3	490	241	0.01%	0.002%
30	4.622	1112	1114	1119	rBV3	310	256	0.01%	0.002%
31	4.674	1127	1130	1133	rBV3	334	235	0.01%	0.002%
32	4.693	1133	1136	1140	rVB2	289	247	0.01%	0.002%
33	4.728	1140	1147	1151	rBV3	678	751	0.04%	0.006%
34	4.953	1200	1217	1256	rBV2	703331	1876110	100.00%	13.804%
35	5.336	1332	1336	1339	rBV2	628	565	0.03%	0.004%
36	5.468	1374	1377	1380	rVB	422	228	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042324\
 Data File : VW035349.D
 Acq On : 23 Apr 2024 10:32
 Operator : SY/MD
 Sample : P2170-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.532	1386	1397	1438	rBV	456870	964238	51.40%	7.095%
38	5.744	1461	1463	1466	rVB4	601	337	0.02%	0.002%
39	5.780	1470	1474	1477	rBV3	370	337	0.02%	0.002%
40	5.834	1481	1491	1515	rVB5	9256	23720	1.26%	0.175%
41	5.985	1524	1538	1573	rBV	408853	854631	45.55%	6.288%
42	6.284	1627	1631	1635	rVB3	511	389	0.02%	0.003%
43	6.320	1639	1642	1646	rVV2	586	470	0.03%	0.003%
44	6.339	1646	1648	1653	rVB2	420	286	0.02%	0.002%
45	6.394	1663	1665	1671	rVB3	535	461	0.02%	0.003%
46	6.567	1714	1719	1724	rBV3	233	325	0.02%	0.002%
47	6.735	1769	1771	1776	rVB	358	273	0.01%	0.002%
48	6.911	1815	1826	1854	rBV	198682	383112	20.42%	2.819%
49	7.239	1917	1928	1959	rBV	815870	1444323	76.98%	10.627%
50	7.551	2016	2025	2056	rBV	140162	261343	13.93%	1.923%
51	7.796	2098	2101	2103	rVB2	710	445	0.02%	0.003%
52	7.870	2121	2124	2125	rBV2	843	460	0.02%	0.003%
53	7.908	2134	2136	2139	rBV2	479	316	0.02%	0.002%
54	8.024	2163	2172	2220	rBV2	312514	756613	40.33%	5.567%
55	8.378	2280	2282	2285	rBV3	434	304	0.02%	0.002%
56	8.448	2301	2304	2308	rVB4	474	327	0.02%	0.002%
57	8.468	2308	2310	2320	rVB3	505	433	0.02%	0.003%
58	8.525	2324	2328	2330	rBV2	652	390	0.02%	0.003%
59	8.577	2343	2344	2348	rVB2	548	285	0.02%	0.002%
60	8.718	2382	2388	2393	rVB3	442	556	0.03%	0.004%
61	8.783	2397	2408	2436	rBV	734984	1215017	64.76%	8.940%
62	9.487	2622	2627	2628	rBV3	541	380	0.02%	0.003%
63	9.837	2732	2736	2742	rVB2	339	367	0.02%	0.003%
64	9.876	2742	2748	2750	rBV2	515	492	0.03%	0.004%
65	10.149	2820	2833	2858	rBV	575264	904340	48.20%	6.654%
66	10.281	2871	2874	2877	rVB3	353	229	0.01%	0.002%
67	10.304	2880	2881	2884	rBV3	325	230	0.01%	0.002%
68	10.320	2884	2886	2887	rBV	777	345	0.02%	0.003%
69	10.406	2909	2913	2916	rBV2	303	277	0.01%	0.002%
70	10.734	3012	3015	3019	rBV2	373	305	0.02%	0.002%
71	10.786	3029	3031	3036	rBV	405	273	0.01%	0.002%
72	10.857	3050	3053	3059	rBV3	648	743	0.04%	0.005%
73	10.976	3085	3090	3096	rBV2	459	462	0.02%	0.003%
74	11.027	3103	3106	3109	rVB2	389	238	0.01%	0.002%
75	11.133	3128	3139	3144	rBV3	2235	3566	0.19%	0.026%
76	11.181	3144	3154	3183	rVV	700485	1120228	59.71%	8.242%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035349.D
 Acq On : 23 Apr 2024 10:32
 Operator : SY/MD
 Sample : P2170-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	11.503	3251	3254	3258	rVB4	458	303	0.02%	0.002%
78	11.558	3258	3271	3304	rBV	842312	1336658	71.25%	9.835%
79	11.802	3344	3347	3354	rVB5	498	488	0.03%	0.004%
80	11.902	3375	3378	3384	rVB3	562	507	0.03%	0.004%
81	11.959	3393	3396	3401	rVB4	359	361	0.02%	0.003%
82	12.236	3479	3482	3486	rVB	481	325	0.02%	0.002%
83	12.265	3486	3491	3493	rBV	403	383	0.02%	0.003%
84	12.590	3586	3592	3600	rVV5	2417	3566	0.19%	0.026%
85	12.693	3620	3624	3627	rVB3	332	233	0.01%	0.002%
86	12.741	3635	3639	3642	rBV2	392	315	0.02%	0.002%
87	12.828	3663	3666	3670	rVB2	344	273	0.01%	0.002%
88	13.033	3728	3730	3736	rVB2	290	296	0.02%	0.002%
89	13.136	3760	3762	3767	rBV3	337	320	0.02%	0.002%
90	13.168	3770	3772	3775	rVV2	388	241	0.01%	0.002%
91	13.204	3775	3783	3800	rVB3	6940	11766	0.63%	0.087%
92	13.307	3811	3815	3819	rBV2	402	312	0.02%	0.002%
93	13.445	3848	3858	3871	rBV	17284	30575	1.63%	0.225%
94	13.686	3923	3933	3945	rBV2	5883	9879	0.53%	0.073%
95	13.754	3951	3954	3958	rVB3	349	247	0.01%	0.002%
96	13.879	3989	3993	3998	rVB4	694	740	0.04%	0.005%
97	13.905	3998	4001	4004	rBV2	449	314	0.02%	0.002%
98	13.982	4023	4025	4028	rVB3	539	245	0.01%	0.002%
99	14.159	4077	4080	4084	rBV4	471	425	0.02%	0.003%
100	14.979	4333	4335	4338	rBV2	471	330	0.02%	0.002%




Sum of corrected areas: 13590903

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035349.D
Acq On : 23 Apr 2024 10:32
Operator : SY/MD
Sample : P2170-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

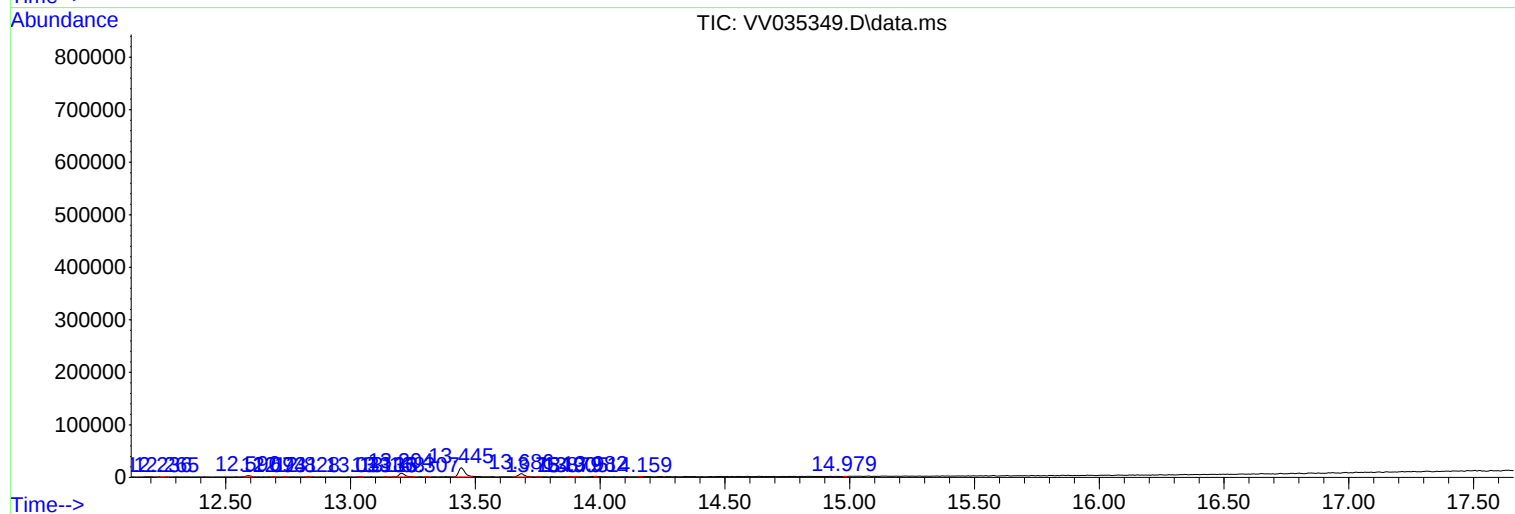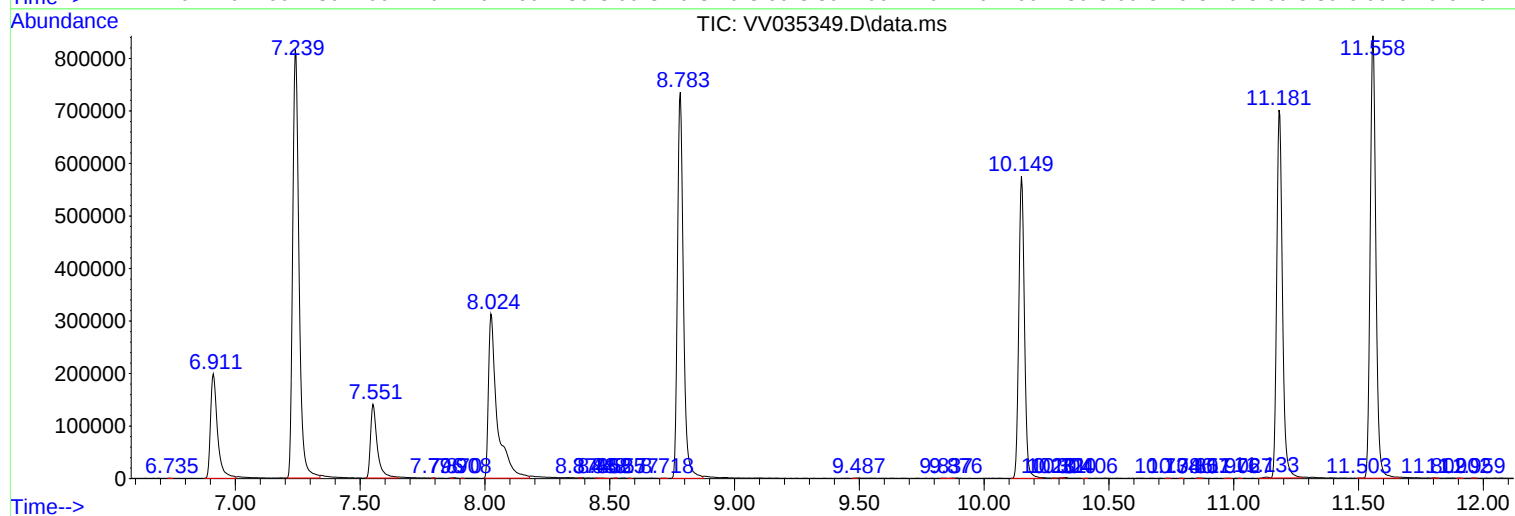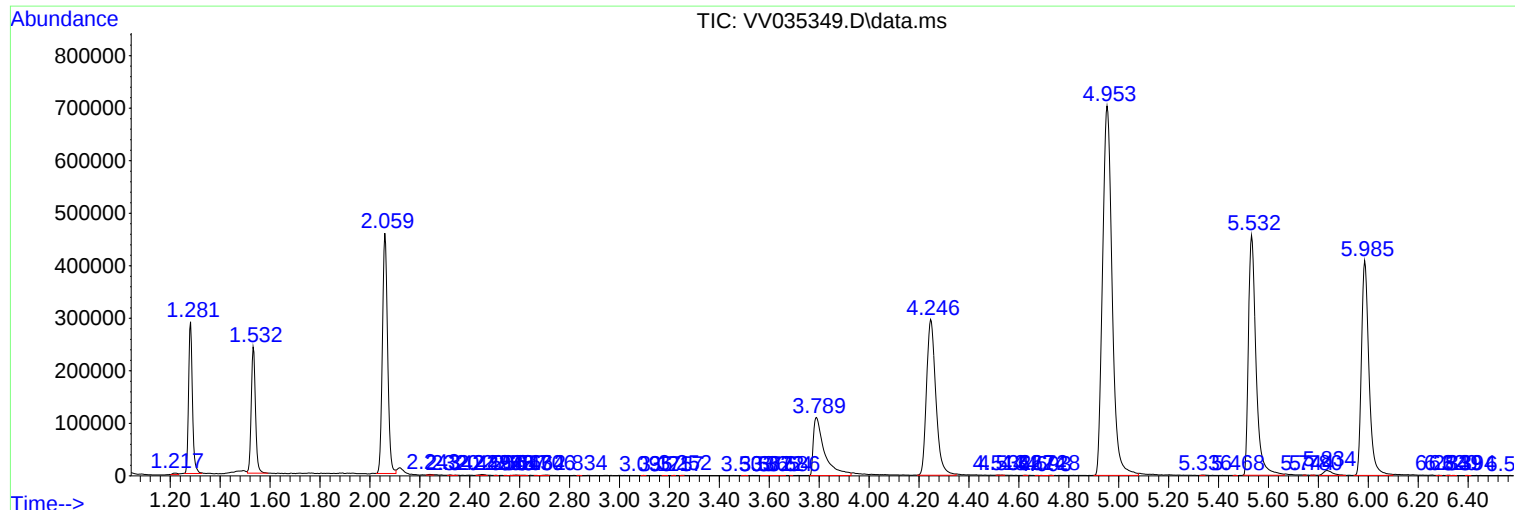

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035349.D
Acq On : 23 Apr 2024 10:32
Operator : SY/MD
Sample : P2170-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035349.D
Acq On : 23 Apr 2024 10:32
Operator : SY/MD
Sample : P2170-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------