

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035350.D
 Acq On : 23 Apr 2024 10:55
 Operator : SY/MD
 Sample : P2170-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035350.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	49	55	57	rBV4	2083	2152	0.12%	0.016%
2	1.281	68	75	95	rBV	281228	294275	16.02%	2.192%
3	1.535	146	154	170	rVB	227123	270673	14.73%	2.016%
4	2.063	307	318	336	rBV	431365	635127	34.57%	4.731%
5	2.240	369	373	380	rVB4	1167	1484	0.08%	0.011%
6	2.314	393	396	400	rBV6	407	286	0.02%	0.002%
7	2.336	400	403	404	rBV2	553	241	0.01%	0.002%
8	2.423	427	430	432	rBV	450	330	0.02%	0.002%
9	2.449	432	438	452	rVB6	1893	3568	0.19%	0.027%
10	2.561	468	473	475	rBV2	611	545	0.03%	0.004%
11	2.648	496	500	504	rVB	262	294	0.02%	0.002%
12	2.709	511	519	523	rVB6	670	984	0.05%	0.007%
13	2.741	523	529	530	rBV2	368	339	0.02%	0.003%
14	2.883	569	573	577	rVV2	316	222	0.01%	0.002%
15	2.937	586	590	592	rBV2	340	224	0.01%	0.002%
16	2.950	592	594	598	rVB2	322	222	0.01%	0.002%
17	2.998	602	609	611	rBV2	203	226	0.01%	0.002%
18	3.124	643	648	651	rBV3	351	343	0.02%	0.003%
19	3.195	666	670	672	rBV3	314	235	0.01%	0.002%
20	3.317	704	708	711	rVB2	530	333	0.02%	0.002%
21	3.580	784	790	797	rBV2	209	222	0.01%	0.002%
22	3.744	837	841	847	rVB2	310	317	0.02%	0.002%
23	3.789	847	855	891	rBV	119598	355219	19.33%	2.646%
24	4.140	962	964	967	rVB2	458	249	0.01%	0.002%
25	4.249	982	998	1028	rBV2	289186	746049	40.61%	5.557%
26	4.561	1093	1095	1098	rBV2	367	254	0.01%	0.002%
27	4.957	1201	1218	1250	rBV2	692043	1837313	100.00%	13.686%
28	5.333	1333	1335	1339	rBV3	492	359	0.02%	0.003%
29	5.394	1350	1354	1359	rVB2	316	334	0.02%	0.002%
30	5.535	1386	1398	1440	rBV	452802	968786	52.73%	7.216%
31	5.841	1482	1493	1515	rVB4	7848	20283	1.10%	0.151%
32	5.989	1526	1539	1571	rBV	402477	839570	45.70%	6.254%
33	6.252	1618	1621	1625	rVB2	337	210	0.01%	0.002%
34	6.397	1663	1666	1669	rVB	513	344	0.02%	0.003%
35	6.416	1669	1672	1677	rBV	441	355	0.02%	0.003%
36	6.628	1734	1738	1744	rVV2	264	267	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035350.D
 Acq On : 23 Apr 2024 10:55
 Operator : SY/MD
 Sample : P2170-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.657	1744	1747	1750	rVV2	404	296	0.02%	0.002%
38	6.674	1750	1752	1756	rVV	362	285	0.02%	0.002%
39	6.751	1775	1776	1779	rVV2	411	212	0.01%	0.002%
40	6.773	1779	1783	1791	rVV3	297	352	0.02%	0.003%
41	6.911	1816	1826	1856	rBV	191061	375715	20.45%	2.799%
42	7.153	1897	1901	1904	rBV3	411	371	0.02%	0.003%
43	7.243	1917	1929	1972	rBV	782425	1403786	76.40%	10.456%
44	7.551	2016	2025	2051	rBV	137822	255814	13.92%	1.905%
45	7.879	2125	2127	2133	rVB3	589	548	0.03%	0.004%
46	7.956	2144	2151	2155	rBV3	220	275	0.01%	0.002%
47	8.024	2163	2172	2215	rBV2	329499	777503	42.32%	5.791%
48	8.442	2298	2302	2304	rBV3	323	238	0.01%	0.002%
49	8.548	2332	2335	2338	rVB2	415	229	0.01%	0.002%
50	8.596	2348	2350	2353	rVB2	811	402	0.02%	0.003%
51	8.619	2353	2357	2359	rBV2	593	389	0.02%	0.003%
52	8.722	2386	2389	2392	rBV2	375	324	0.02%	0.002%
53	8.783	2397	2408	2455	rVV	741310	1225729	66.71%	9.130%
54	9.046	2488	2490	2492	rBV3	446	245	0.01%	0.002%
55	9.091	2500	2504	2505	rBV2	467	301	0.02%	0.002%
56	9.140	2516	2519	2521	rBV3	685	328	0.02%	0.002%
57	9.223	2539	2545	2546	rBV2	355	325	0.02%	0.002%
58	9.342	2578	2582	2590	rVB2	317	322	0.02%	0.002%
59	9.545	2643	2645	2650	rVV4	355	288	0.02%	0.002%
60	9.802	2720	2725	2729	rVV2	356	425	0.02%	0.003%
61	9.870	2743	2746	2749	rBV2	381	288	0.02%	0.002%
62	10.149	2821	2833	2855	rBV	589262	918480	49.99%	6.841%
63	10.320	2882	2886	2898	rVB7	1514	2388	0.13%	0.018%
64	10.374	2900	2903	2907	rVB2	353	259	0.01%	0.002%
65	10.480	2933	2936	2939	rBV3	316	229	0.01%	0.002%
66	10.554	2953	2959	2962	rBV2	245	216	0.01%	0.002%
67	10.786	3028	3031	3034	rBV2	413	334	0.02%	0.002%
68	11.181	3144	3154	3180	rBV	698371	1122773	61.11%	8.363%
69	11.435	3230	3233	3237	rVB4	775	541	0.03%	0.004%
70	11.558	3258	3271	3298	rBV	829116	1315598	71.60%	9.799%
71	11.728	3322	3324	3331	rVB4	494	380	0.02%	0.003%
72	11.831	3352	3356	3360	rVB4	504	373	0.02%	0.003%
73	11.921	3380	3384	3387	rBV2	357	243	0.01%	0.002%
74	11.940	3387	3390	3395	rVB2	480	349	0.02%	0.003%
75	12.037	3417	3420	3424	rBV2	314	266	0.01%	0.002%
76	12.188	3460	3467	3471	rBV3	854	994	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035350.D
 Acq On : 23 Apr 2024 10:55
 Operator : SY/MD
 Sample : P2170-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	12.342	3509	3515	3517	rVB3	510	361	0.02%	0.003%
78	12.384	3524	3528	3530	rBV2	335	234	0.01%	0.002%
79	12.451	3547	3549	3553	rVB3	412	289	0.02%	0.002%
80	12.541	3574	3577	3580	rVV2	436	314	0.02%	0.002%
81	12.593	3586	3593	3594	rBV5	1492	1455	0.08%	0.011%
82	12.699	3621	3626	3629	rBV2	286	292	0.02%	0.002%
83	12.808	3657	3660	3663	rBV3	328	295	0.02%	0.002%
84	12.927	3695	3697	3702	rVB2	366	238	0.01%	0.002%
85	12.956	3702	3706	3709	rBV2	381	304	0.02%	0.002%
86	13.024	3722	3727	3734	rBV	384	523	0.03%	0.004%
87	13.204	3776	3783	3793	rBV4	4226	7161	0.39%	0.053%
88	13.291	3808	3810	3816	rVB4	539	417	0.02%	0.003%
89	13.381	3835	3838	3842	rVB3	406	305	0.02%	0.002%
90	13.448	3851	3859	3872	rVV2	8042	13183	0.72%	0.098%
91	13.500	3872	3875	3879	rVB2	756	626	0.03%	0.005%
92	13.567	3891	3896	3901	rBV4	498	614	0.03%	0.005%
93	13.635	3913	3917	3919	rBV2	359	300	0.02%	0.002%
94	13.686	3925	3933	3944	rVB5	3375	5546	0.30%	0.041%
95	13.728	3944	3946	3950	rBV	341	275	0.01%	0.002%
96	13.760	3953	3956	3959	rBV	508	312	0.02%	0.002%
97	13.882	3991	3994	3997	rBV3	443	291	0.02%	0.002%
98	14.365	4141	4144	4147	rBV3	594	420	0.02%	0.003%
99	14.503	4183	4187	4191	rBV3	490	397	0.02%	0.003%
100	14.628	4222	4226	4227	rBV	630	442	0.02%	0.003%


Sum of corrected areas: 13425241

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035350.D
Acq On : 23 Apr 2024 10:55
Operator : SY/MD
Sample : P2170-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

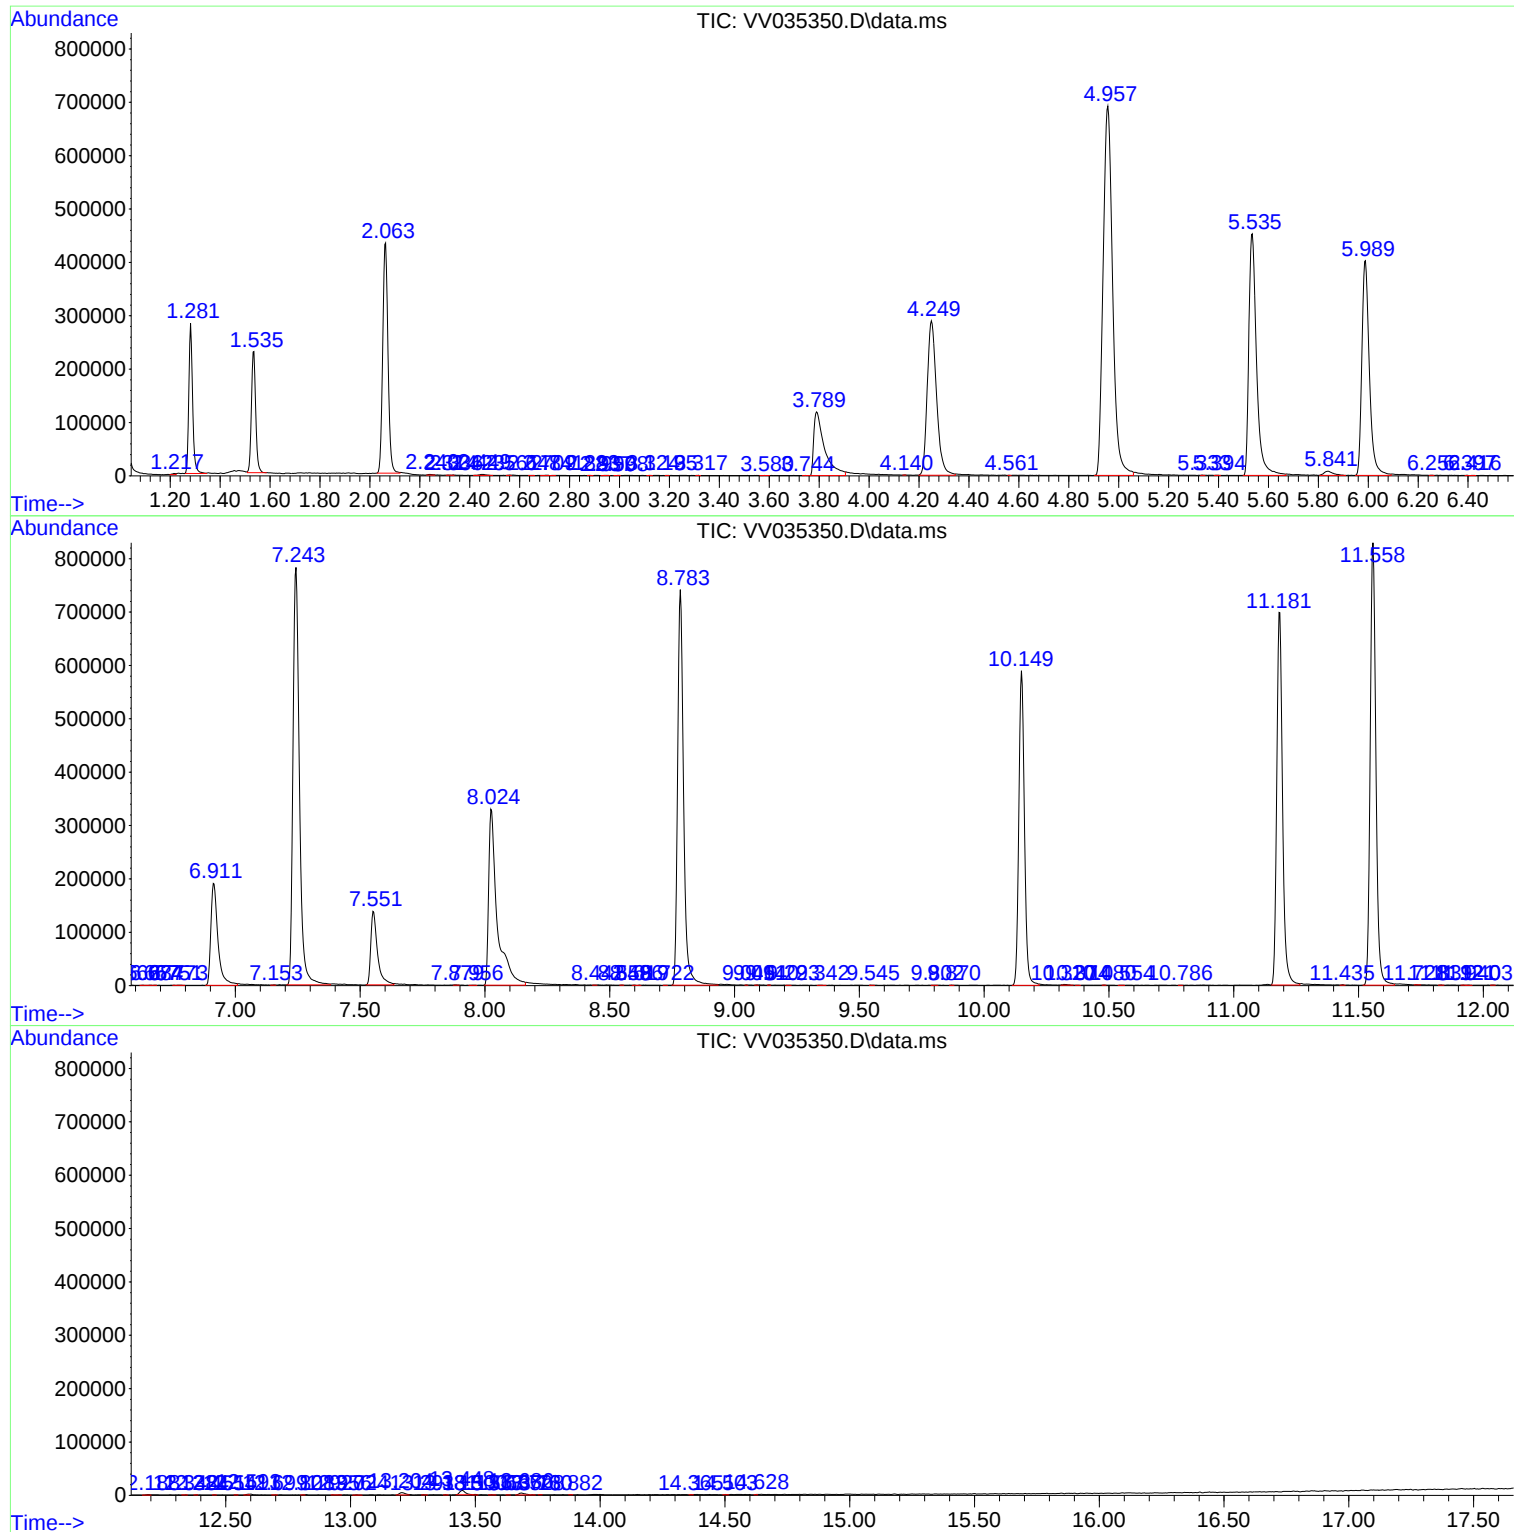

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035350.D
Acq On : 23 Apr 2024 10:55
Operator : SY/MD
Sample : P2170-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035350.D
Acq On : 23 Apr 2024 10:55
Operator : SY/MD
Sample : P2170-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------