

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035351.D
 Acq On : 23 Apr 2024 11:18
 Operator : SY/MD
 Sample : P2157-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035351.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rBV	283251	298671	16.25%	2.367%
2	1.532	146	153	167	rVB	231131	270305	14.71%	2.142%
3	2.060	307	317	330	rBV	444677	643842	35.04%	5.103%
4	2.394	419	421	425	rBV3	578	543	0.03%	0.004%
5	2.503	451	455	456	rBV	433	270	0.01%	0.002%
6	2.748	529	531	534	rBV	208	138	0.01%	0.001%
7	2.796	541	546	549	rBV2	283	277	0.02%	0.002%
8	2.957	594	596	598	rBV	235	135	0.01%	0.001%
9	2.995	606	608	612	rVB2	375	190	0.01%	0.002%
10	3.073	629	632	636	rVB2	256	161	0.01%	0.001%
11	3.105	639	642	646	rBV2	165	151	0.01%	0.001%
12	3.159	656	659	665	rVB2	281	200	0.01%	0.002%
13	3.192	666	669	672	rBV	169	131	0.01%	0.001%
14	3.339	712	715	717	rBV2	203	154	0.01%	0.001%
15	3.397	726	733	737	rBV3	264	297	0.02%	0.002%
16	3.436	741	745	755	rVB3	359	408	0.02%	0.003%
17	3.497	755	764	767	rBV2	365	355	0.02%	0.003%
18	3.516	767	770	776	rVB3	238	251	0.01%	0.002%
19	3.555	778	782	784	rBV2	389	284	0.02%	0.002%
20	3.584	788	791	792	rBV	172	99	0.01%	0.001%
21	3.719	830	833	836	rBV2	200	151	0.01%	0.001%
22	3.757	840	845	846	rBV	177	126	0.01%	0.001%
23	3.786	846	854	893	rBV	116526	342751	18.65%	2.717%
24	4.246	983	997	1033	rBV	288129	735180	40.01%	5.827%
25	4.690	1133	1135	1139	rVB3	255	161	0.01%	0.001%
26	4.728	1144	1147	1148	rBV2	291	152	0.01%	0.001%
27	4.889	1195	1197	1199	rBV2	328	198	0.01%	0.002%
28	4.954	1201	1217	1261	rVV2	697626	1837588	100.00%	14.564%
29	5.407	1356	1358	1359	rBV	269	114	0.01%	0.001%
30	5.532	1385	1397	1436	rBV	347192	749210	40.77%	5.938%
31	5.831	1481	1490	1511	rBV2	8119	19990	1.09%	0.158%
32	5.986	1525	1538	1567	rBV	396106	829305	45.13%	6.573%
33	6.272	1625	1627	1629	rBV2	530	270	0.01%	0.002%
34	6.317	1639	1641	1645	rBV3	843	559	0.03%	0.004%
35	6.333	1645	1646	1651	rVB2	661	348	0.02%	0.003%
36	6.362	1651	1655	1660	rBV2	424	546	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042324\
 Data File : VW035351.D
 Acq On : 23 Apr 2024 11:18
 Operator : SY/MD
 Sample : P2157-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.439	1676	1679	1680	rBV	202	104	0.01%	0.001%
38	6.449	1680	1682	1685	rVB	492	236	0.01%	0.002%
39	6.471	1686	1689	1690	rBV	260	99	0.01%	0.001%
40	6.481	1690	1692	1694	rBV2	401	219	0.01%	0.002%
41	6.539	1706	1710	1714	rVB3	506	419	0.02%	0.003%
42	6.571	1714	1720	1721	rBV2	140	130	0.01%	0.001%
43	6.616	1732	1734	1737	rVB2	201	100	0.01%	0.001%
44	6.632	1737	1739	1741	rVB2	390	169	0.01%	0.001%
45	6.648	1741	1744	1748	rBV2	349	347	0.02%	0.003%
46	6.725	1764	1768	1770	rBV2	205	170	0.01%	0.001%
47	6.767	1778	1781	1782	rBV2	427	229	0.01%	0.002%
48	6.876	1811	1815	1816	rBV2	329	224	0.01%	0.002%
49	6.912	1816	1826	1855	rBV	192087	372528	20.27%	2.953%
50	7.159	1899	1903	1905	rBV2	370	217	0.01%	0.002%
51	7.195	1912	1914	1915	rBV	344	119	0.01%	0.001%
52	7.240	1918	1928	1966	rVV	798338	1415430	77.03%	11.218%
53	7.551	2016	2025	2058	rBV	136444	256113	13.94%	2.030%
54	7.857	2118	2120	2122	rBV3	464	233	0.01%	0.002%
55	7.941	2142	2146	2148	rVB2	459	287	0.02%	0.002%
56	7.957	2148	2151	2152	rBV2	241	164	0.01%	0.001%
57	8.024	2163	2172	2223	rBV2	318283	769910	41.90%	6.102%
58	8.535	2329	2331	2333	rBV2	258	146	0.01%	0.001%
59	8.638	2360	2363	2365	rBV2	316	243	0.01%	0.002%
60	8.690	2375	2379	2383	rBV2	480	388	0.02%	0.003%
61	8.712	2383	2386	2388	rBV2	378	203	0.01%	0.002%
62	8.728	2388	2391	2395	rVB2	239	169	0.01%	0.001%
63	8.783	2396	2408	2442	rBV	564059	950009	51.70%	7.529%
64	9.156	2522	2524	2526	rBV	368	157	0.01%	0.001%
65	9.172	2526	2529	2533	rVV3	474	474	0.03%	0.004%
66	9.201	2536	2538	2540	rVV	381	134	0.01%	0.001%
67	9.230	2545	2547	2553	rVB2	326	212	0.01%	0.002%
68	9.259	2553	2556	2559	rBV3	266	178	0.01%	0.001%
69	9.381	2592	2594	2597	rVB2	209	101	0.01%	0.001%
70	9.452	2612	2616	2618	rBV	234	135	0.01%	0.001%
71	9.487	2624	2627	2629	rBV2	249	165	0.01%	0.001%
72	9.506	2630	2633	2637	rVV3	322	231	0.01%	0.002%
73	9.542	2641	2644	2648	rVB2	353	292	0.02%	0.002%
74	9.629	2667	2671	2674	rBV3	253	231	0.01%	0.002%
75	9.645	2674	2676	2681	rVB2	337	270	0.01%	0.002%
76	9.670	2681	2684	2686	rBV2	160	120	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035351.D
 Acq On : 23 Apr 2024 11:18
 Operator : SY/MD
 Sample : P2157-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.805	2721	2726	2730	rBV3	358	437	0.02%	0.003%
78	9.854	2737	2741	2742	rBV2	290	171	0.01%	0.001%
79	9.931	2760	2765	2767	rBV2	177	165	0.01%	0.001%
80	9.966	2773	2776	2777	rBV	161	99	0.01%	0.001%
81	9.976	2777	2779	2782	rVV	291	146	0.01%	0.001%
82	10.002	2785	2787	2790	rVB2	334	227	0.01%	0.002%
83	10.095	2814	2816	2821	rVB2	243	140	0.01%	0.001%
84	10.149	2821	2833	2868	rBV	569124	901796	49.07%	7.147%
85	10.403	2910	2912	2914	rBV2	221	107	0.01%	0.001%
86	10.484	2936	2937	2942	rBV2	171	113	0.01%	0.001%
87	10.532	2950	2952	2957	rVB2	245	168	0.01%	0.001%
88	10.664	2991	2993	2994	rBV2	207	102	0.01%	0.001%
89	10.767	3023	3025	3028	rVB2	333	175	0.01%	0.001%
90	10.789	3029	3032	3037	rVB2	683	479	0.03%	0.004%
91	10.812	3037	3039	3041	rBV	228	106	0.01%	0.001%
92	10.863	3051	3055	3057	rBV3	479	347	0.02%	0.003%
93	11.130	3127	3138	3144	rBV3	1386	2519	0.14%	0.020%
94	11.182	3144	3154	3182	rBV	534106	871276	47.41%	6.905%
95	11.503	3247	3254	3258	rBV5	5616	8296	0.45%	0.066%
96	11.558	3261	3271	3299	rVB	826848	1310741	71.33%	10.389%
97	13.059	3736	3738	3742	rVB	292	177	0.01%	0.001%
98	13.204	3777	3783	3797	rBV4	4079	6183	0.34%	0.049%
99	13.452	3850	3860	3869	rBV3	4644	8001	0.44%	0.063%
100	13.587	3898	3902	3905	rBV	391	376	0.02%	0.003%




Sum of corrected areas: 12617163

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035351.D
Acq On : 23 Apr 2024 11:18
Operator : SY/MD
Sample : P2157-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

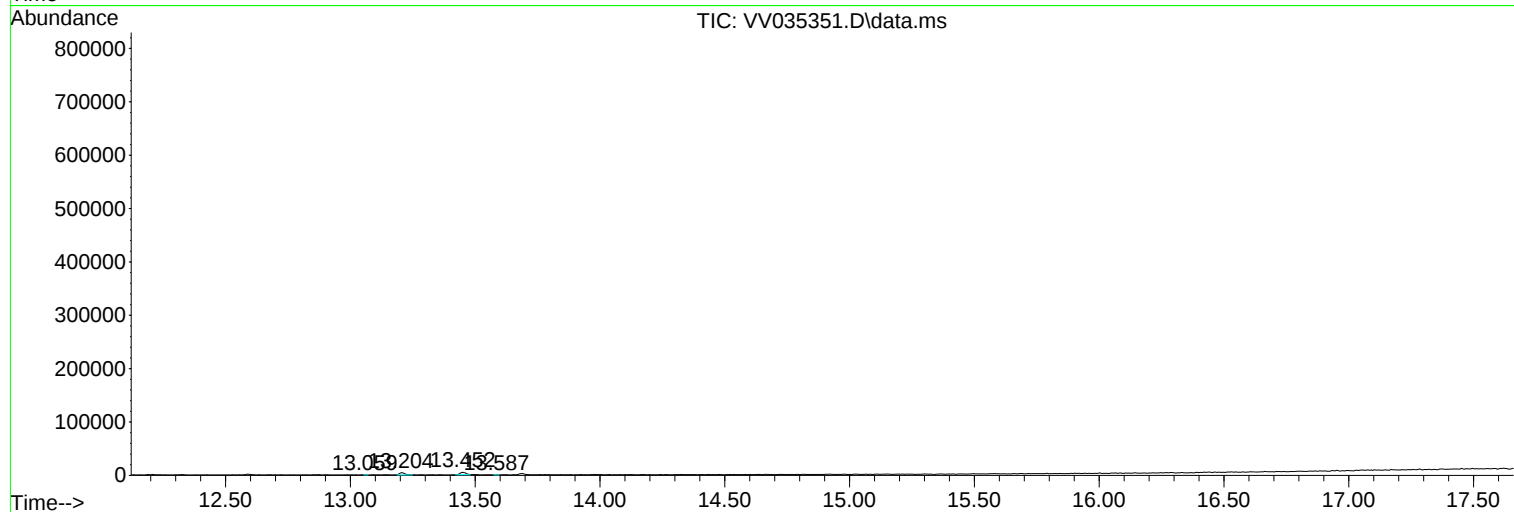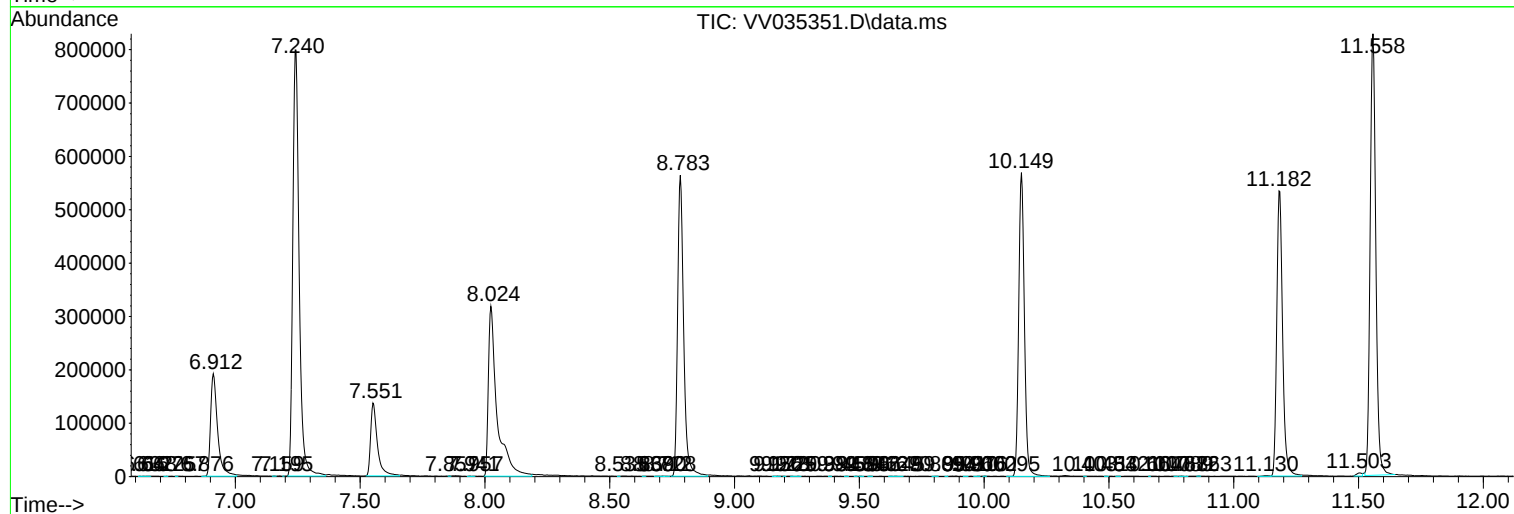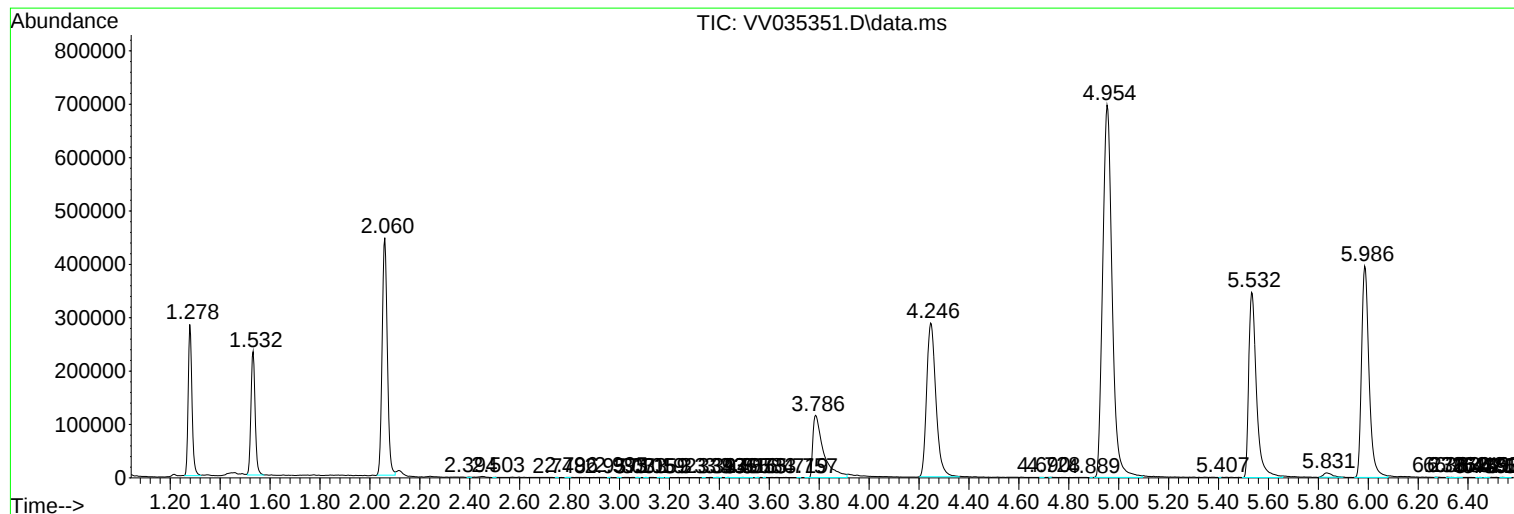

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035351.D
Acq On : 23 Apr 2024 11:18
Operator : SY/MD
Sample : P2157-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035351.D
Acq On : 23 Apr 2024 11:18
Operator : SY/MD
Sample : P2157-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------