

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035352.D
 Acq On : 23 Apr 2024 11:41
 Operator : SY/MD
 Sample : P2157-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035352.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	280822	295604	16.35%	2.226%
2	1.532	145	153	172	rVB	226884	271464	15.01%	2.044%
3	2.059	307	317	334	rBV	439862	640000	35.39%	4.820%
4	2.233	367	371	379	rBV6	1073	1407	0.08%	0.011%
5	2.609	485	488	492	rBV2	459	398	0.02%	0.003%
6	2.654	500	502	503	rBV2	242	84	0.00%	0.001%
7	2.706	515	518	526	rVB4	398	490	0.03%	0.004%
8	2.741	527	529	535	rVB3	380	239	0.01%	0.002%
9	2.883	570	573	575	rBV2	243	132	0.01%	0.001%
10	2.924	583	586	589	rVB	340	216	0.01%	0.002%
11	2.976	598	602	603	rBV	249	168	0.01%	0.001%
12	3.040	618	622	625	rBV2	199	150	0.01%	0.001%
13	3.082	632	635	636	rBV2	363	215	0.01%	0.002%
14	3.159	656	659	667	rBV3	287	359	0.02%	0.003%
15	3.214	672	676	677	rBV2	199	141	0.01%	0.001%
16	3.246	683	686	689	rVB2	279	164	0.01%	0.001%
17	3.301	698	703	704	rBV2	120	106	0.01%	0.001%
18	3.465	751	754	758	rBV2	150	110	0.01%	0.001%
19	3.497	758	764	766	rBV	247	272	0.02%	0.002%
20	3.519	769	771	775	rBV2	175	104	0.01%	0.001%
21	3.561	782	784	787	rBV	187	150	0.01%	0.001%
22	3.606	794	798	806	rVB2	148	183	0.01%	0.001%
23	3.651	810	812	815	rBV2	206	114	0.01%	0.001%
24	3.699	824	827	830	rBV2	222	123	0.01%	0.001%
25	3.735	836	838	841	rBV2	210	101	0.01%	0.001%
26	3.786	846	854	897	rBV	113702	336773	18.62%	2.536%
27	4.246	982	997	1032	rBV	283165	732524	40.51%	5.516%
28	4.654	1121	1124	1128	rVB2	507	365	0.02%	0.003%
29	4.744	1147	1152	1156	rBV2	565	562	0.03%	0.004%
30	4.796	1166	1168	1169	rBV	245	85	0.00%	0.001%
31	4.892	1195	1198	1201	rBV3	389	268	0.01%	0.002%
32	4.953	1201	1217	1247	rBV2	687381	1808296	100.00%	13.618%
33	5.297	1321	1324	1327	rBV3	481	432	0.02%	0.003%
34	5.365	1341	1345	1350	rVB4	407	468	0.03%	0.004%
35	5.391	1350	1353	1357	rBV2	399	344	0.02%	0.003%
36	5.532	1386	1397	1446	rBV	463298	984934	54.47%	7.417%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042324\
 Data File : VW035352.D
 Acq On : 23 Apr 2024 11:41
 Operator : SY/MD
 Sample : P2157-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.834	1481	1491	1503	rBV5	6940	16514	0.91%	0.124%
38	5.985	1525	1538	1574	rBV	392749	828006	45.79%	6.235%
39	6.243	1616	1618	1619	rBV2	348	123	0.01%	0.001%
40	6.284	1627	1631	1633	rBV2	656	459	0.03%	0.003%
41	6.336	1644	1647	1651	rBV	487	359	0.02%	0.003%
42	6.352	1651	1652	1653	rBV	406	126	0.01%	0.001%
43	6.416	1667	1672	1673	rBV3	332	281	0.02%	0.002%
44	6.493	1693	1696	1697	rBV	251	130	0.01%	0.001%
45	6.551	1711	1714	1717	rVV	229	119	0.01%	0.001%
46	6.599	1727	1729	1733	rVB2	222	153	0.01%	0.001%
47	6.625	1733	1737	1740	rBV2	149	134	0.01%	0.001%
48	6.645	1741	1743	1745	rVB2	414	146	0.01%	0.001%
49	6.680	1751	1754	1756	rBV2	347	233	0.01%	0.002%
50	6.722	1764	1767	1769	rBV3	277	214	0.01%	0.002%
51	6.773	1781	1783	1786	rVB2	558	258	0.01%	0.002%
52	6.799	1786	1791	1792	rBV2	195	115	0.01%	0.001%
53	6.828	1796	1800	1803	rBV3	247	184	0.01%	0.001%
54	6.911	1815	1826	1855	rBV	192180	372834	20.62%	2.808%
55	7.243	1917	1929	1968	rBV	785446	1405532	77.73%	10.585%
56	7.551	2016	2025	2049	rBV	134656	250943	13.88%	1.890%
57	7.844	2114	2116	2118	rBV	288	139	0.01%	0.001%
58	7.915	2136	2138	2143	rVB2	515	290	0.02%	0.002%
59	8.024	2163	2172	2216	rBV2	316484	758018	41.92%	5.708%
60	8.525	2326	2328	2329	rBV2	332	97	0.01%	0.001%
61	8.551	2333	2336	2338	rBV4	571	373	0.02%	0.003%
62	8.622	2356	2358	2361	rBV2	396	234	0.01%	0.002%
63	8.783	2397	2408	2434	rBV	735558	1223789	67.68%	9.216%
64	9.181	2530	2532	2535	rVB3	479	231	0.01%	0.002%
65	9.230	2545	2547	2551	rBV2	208	136	0.01%	0.001%
66	9.284	2561	2564	2568	rBV2	384	272	0.02%	0.002%
67	9.310	2569	2572	2577	rVB2	245	162	0.01%	0.001%
68	9.493	2627	2629	2631	rBV	264	151	0.01%	0.001%
69	9.574	2651	2654	2658	rVB2	364	255	0.01%	0.002%
70	9.635	2670	2673	2677	rVB2	320	187	0.01%	0.001%
71	9.657	2677	2680	2683	rBB2	316	142	0.01%	0.001%
72	9.683	2686	2688	2691	rBV	142	105	0.01%	0.001%
73	9.738	2703	2705	2706	rBV	288	93	0.01%	0.001%
74	9.841	2735	2737	2743	rBV2	290	222	0.01%	0.002%
75	9.869	2743	2746	2747	rBV	291	186	0.01%	0.001%
76	9.902	2754	2756	2761	rVB	245	136	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035352.D
 Acq On : 23 Apr 2024 11:41
 Operator : SY/MD
 Sample : P2157-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.972	2775	2778	2782	rBV2	174	105	0.01%	0.001%
78	10.095	2812	2816	2820	rBV2	326	326	0.02%	0.002%
79	10.149	2821	2833	2856	rBV	559635	892239	49.34%	6.719%
80	10.377	2900	2904	2907	rBV3	358	246	0.01%	0.002%
81	10.397	2907	2910	2913	rBV3	420	321	0.02%	0.002%
82	10.480	2934	2936	2937	rBV	373	177	0.01%	0.001%
83	10.564	2958	2962	2963	rBV2	315	200	0.01%	0.002%
84	10.619	2971	2979	2982	rBV4	437	566	0.03%	0.004%
85	10.651	2986	2989	2991	rBV2	188	108	0.01%	0.001%
86	10.815	3036	3040	3042	rBV	556	357	0.02%	0.003%
87	10.828	3042	3044	3048	rVB2	293	165	0.01%	0.001%
88	10.934	3074	3077	3081	rBV2	213	171	0.01%	0.001%
89	11.133	3130	3139	3144	rBV4	1426	2114	0.12%	0.016%
90	11.185	3144	3155	3185	rBV	711039	1129806	62.48%	8.508%
91	11.471	3240	3244	3248	rBV4	595	710	0.04%	0.005%
92	11.558	3254	3271	3293	rBV	809759	1299992	71.89%	9.790%
93	11.953	3391	3394	3396	rBV2	350	254	0.01%	0.002%
94	12.107	3439	3442	3445	rBV2	425	301	0.02%	0.002%
95	12.673	3616	3618	3626	rVB3	551	465	0.03%	0.004%
96	12.747	3638	3641	3644	rVB2	450	273	0.02%	0.002%
97	13.027	3724	3728	3733	rVB4	453	510	0.03%	0.004%
98	13.088	3745	3747	3749	rBV2	306	156	0.01%	0.001%
99	13.204	3777	3783	3794	rBV5	3434	6119	0.34%	0.046%
100	13.455	3855	3861	3866	rBV3	2954	3755	0.21%	0.028%




Sum of corrected areas: 13279062

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035352.D
Acq On : 23 Apr 2024 11:41
Operator : SY/MD
Sample : P2157-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

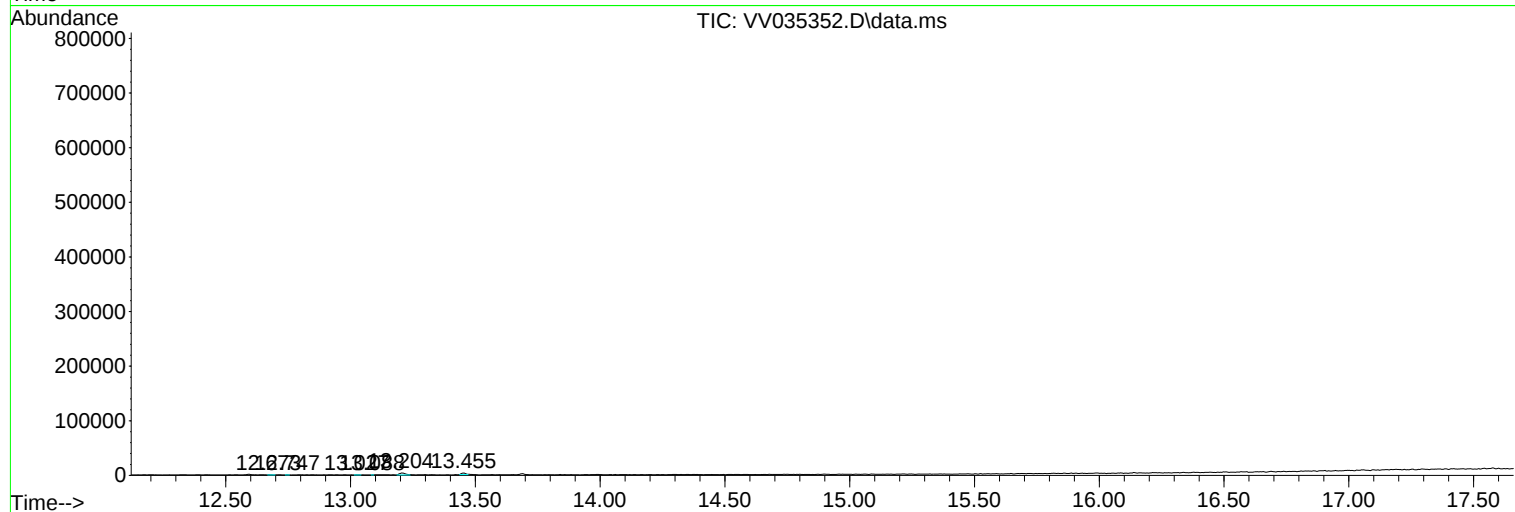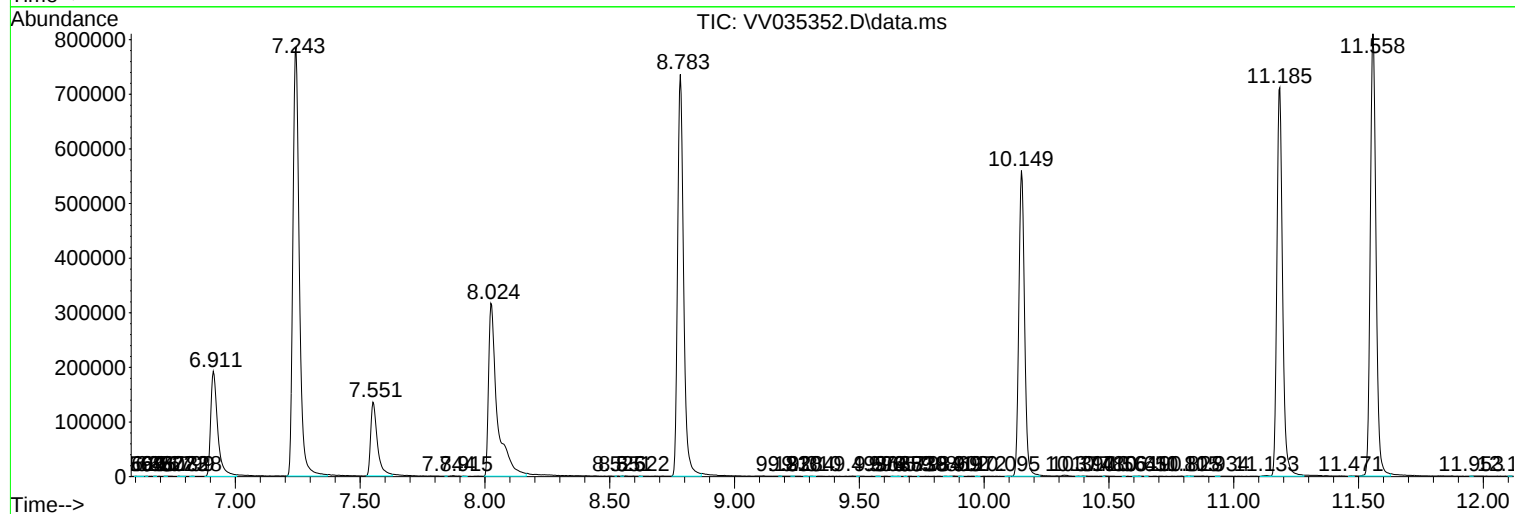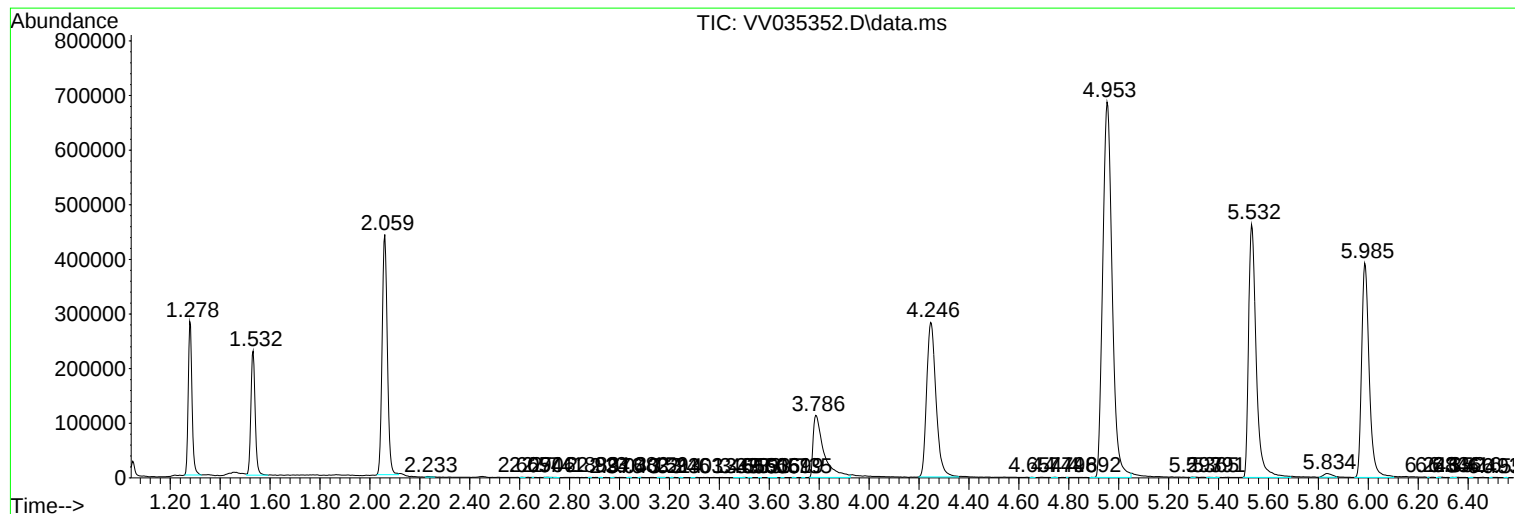

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035352.D
Acq On : 23 Apr 2024 11:41
Operator : SY/MD
Sample : P2157-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035352.D
Acq On : 23 Apr 2024 11:41
Operator : SY/MD
Sample : P2157-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------