

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035353.D
 Acq On : 23 Apr 2024 12:05
 Operator : SY/MD
 Sample : P2157-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035353.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	284395	298782	16.19%	2.246%
2	1.532	146	153	168	rVB	230352	271564	14.71%	2.041%
3	2.060	307	317	330	rBV	443117	640821	34.71%	4.816%
4	2.452	431	439	454	rVB5	1700	2735	0.15%	0.021%
5	2.619	488	491	492	rBV2	308	191	0.01%	0.001%
6	2.693	509	514	515	rBV	501	375	0.02%	0.003%
7	2.864	564	567	568	rBV2	236	132	0.01%	0.001%
8	2.960	595	597	599	rBV	309	149	0.01%	0.001%
9	3.005	607	611	614	rBV	460	307	0.02%	0.002%
10	3.021	614	616	619	rVB	291	154	0.01%	0.001%
11	3.076	630	633	636	rBV3	244	238	0.01%	0.002%
12	3.111	642	644	648	rBV2	373	224	0.01%	0.002%
13	3.233	679	682	685	rBV	275	211	0.01%	0.002%
14	3.262	690	691	694	rBV	119	57	0.00%	0.000%
15	3.336	712	714	715	rBV	139	43	0.00%	0.000%
16	3.388	728	730	732	rBV2	162	72	0.00%	0.001%
17	3.426	741	742	744	rBV	220	77	0.00%	0.001%
18	3.442	744	747	749	rVV2	113	56	0.00%	0.000%
19	3.462	749	753	754	rVB	313	191	0.01%	0.001%
20	3.481	754	759	761	rBV	233	191	0.01%	0.001%
21	3.513	765	769	773	rBV2	243	220	0.01%	0.002%
22	3.561	781	784	786	rBV2	208	139	0.01%	0.001%
23	3.613	796	800	801	rBV2	225	155	0.01%	0.001%
24	3.667	812	817	820	rBV2	320	242	0.01%	0.002%
25	3.693	822	825	829	rVV2	161	130	0.01%	0.001%
26	3.786	844	854	900	rBV	118476	360245	19.52%	2.708%
27	4.246	983	997	1034	rBV2	288593	742901	40.24%	5.584%
28	4.953	1201	1217	1256	rBV2	704934	1845976	100.00%	13.874%
29	5.381	1348	1350	1353	rVB3	522	276	0.01%	0.002%
30	5.423	1361	1363	1365	rBV3	369	139	0.01%	0.001%
31	5.532	1386	1397	1423	rBV	437948	910126	49.30%	6.840%
32	5.834	1484	1491	1509	rVB2	7673	16515	0.89%	0.124%
33	5.924	1515	1519	1524	rVB3	569	539	0.03%	0.004%
34	5.986	1525	1538	1568	rBV	398617	836927	45.34%	6.290%
35	6.243	1616	1618	1620	rBV2	554	263	0.01%	0.002%
36	6.281	1628	1630	1632	rBV2	231	128	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042324\
 Data File : VW035353.D
 Acq On : 23 Apr 2024 12:05
 Operator : SY/MD
 Sample : P2157-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.314	1637	1640	1641	rBV2	434	198	0.01%	0.001%
38	6.423	1670	1674	1676	rBV2	198	174	0.01%	0.001%
39	6.455	1682	1684	1685	rBV	241	77	0.00%	0.001%
40	6.481	1690	1692	1694	rBV	120	46	0.00%	0.000%
41	6.497	1694	1697	1699	rBV2	339	238	0.01%	0.002%
42	6.535	1705	1709	1711	rBV2	197	139	0.01%	0.001%
43	6.551	1712	1714	1717	rVB2	172	61	0.00%	0.000%
44	6.580	1721	1723	1725	rBV2	173	83	0.00%	0.001%
45	6.632	1735	1739	1743	rBV	370	340	0.02%	0.003%
46	6.677	1751	1753	1755	rBV2	253	141	0.01%	0.001%
47	6.728	1766	1769	1771	rBV2	406	228	0.01%	0.002%
48	6.764	1777	1780	1781	rBV2	181	67	0.00%	0.001%
49	6.783	1784	1786	1787	rBV2	410	157	0.01%	0.001%
50	6.828	1797	1800	1803	rBV2	226	141	0.01%	0.001%
51	6.912	1816	1826	1861	rBV	194487	381950	20.69%	2.871%
52	7.243	1917	1929	1963	rBV	798457	1426478	77.28%	10.721%
53	7.551	2016	2025	2044	rBV	135660	249225	13.50%	1.873%
54	7.834	2111	2113	2116	rVB2	474	248	0.01%	0.002%
55	7.947	2147	2148	2152	rVB2	256	134	0.01%	0.001%
56	7.969	2153	2155	2157	rBV	246	121	0.01%	0.001%
57	8.024	2163	2172	2223	rBV2	331462	793492	42.98%	5.964%
58	8.490	2315	2317	2321	rBV5	441	320	0.02%	0.002%
59	8.612	2352	2355	2358	rBV3	532	376	0.02%	0.003%
60	8.783	2397	2408	2439	rBV	710781	1171223	63.45%	8.803%
61	9.040	2486	2488	2493	rVB2	506	328	0.02%	0.002%
62	9.095	2501	2505	2509	rBV3	891	664	0.04%	0.005%
63	9.114	2509	2511	2515	rBV4	585	429	0.02%	0.003%
64	9.149	2519	2522	2525	rBV3	563	366	0.02%	0.003%
65	9.188	2530	2534	2535	rBV	380	238	0.01%	0.002%
66	9.223	2543	2545	2548	rBV2	279	194	0.01%	0.001%
67	9.362	2586	2588	2595	rVB2	245	190	0.01%	0.001%
68	9.397	2595	2599	2601	rBV2	268	167	0.01%	0.001%
69	9.413	2601	2604	2606	rVV3	366	171	0.01%	0.001%
70	9.471	2620	2622	2624	rVB	236	94	0.01%	0.001%
71	9.529	2637	2640	2642	rBV	176	97	0.01%	0.001%
72	9.548	2643	2646	2648	rBV	223	134	0.01%	0.001%
73	9.564	2648	2651	2652	rBV	176	77	0.00%	0.001%
74	9.600	2660	2662	2663	rBV	171	75	0.00%	0.001%
75	9.638	2671	2674	2678	rVB	293	213	0.01%	0.002%
76	9.664	2678	2682	2684	rBV	351	252	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035353.D
 Acq On : 23 Apr 2024 12:05
 Operator : SY/MD
 Sample : P2157-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.764	2711	2713	2714	rBV	132	56	0.00%	0.000%
78	9.776	2715	2717	2722	rVB	312	203	0.01%	0.002%
79	10.149	2821	2833	2860	rBV	583936	920948	49.89%	6.922%
80	10.368	2899	2901	2904	rVB	299	125	0.01%	0.001%
81	10.384	2904	2906	2909	rBV2	307	185	0.01%	0.001%
82	10.410	2911	2914	2915	rBV	255	127	0.01%	0.001%
83	10.452	2924	2927	2928	rBV	331	163	0.01%	0.001%
84	10.526	2944	2950	2951	rBV2	324	230	0.01%	0.002%
85	10.548	2955	2957	2959	rVV	210	114	0.01%	0.001%
86	10.561	2959	2961	2968	rVB2	290	288	0.02%	0.002%
87	10.593	2968	2971	2972	rBV2	226	134	0.01%	0.001%
88	10.696	3001	3003	3007	rBV	227	153	0.01%	0.001%
89	10.789	3028	3032	3035	rBV2	349	368	0.02%	0.003%
90	10.850	3050	3051	3052	rBV2	148	45	0.00%	0.000%
91	11.108	3129	3131	3132	rBV	326	123	0.01%	0.001%
92	11.127	3132	3137	3143	rVV5	1204	1572	0.09%	0.012%
93	11.182	3143	3154	3178	rBV	688453	1079360	58.47%	8.112%
94	11.487	3245	3249	3253	rBV3	519	584	0.03%	0.004%
95	11.558	3259	3271	3297	rBV	841623	1328779	71.98%	9.987%
96	11.905	3376	3379	3383	rVB	411	308	0.02%	0.002%
97	12.471	3552	3555	3559	rBV2	430	365	0.02%	0.003%
98	12.587	3585	3591	3598	rBV3	2488	3166	0.17%	0.024%
99	13.210	3776	3785	3792	rBV7	3917	6229	0.34%	0.047%
100	13.979	4021	4024	4029	rBV2	780	692	0.04%	0.005%




Sum of corrected areas: 13305154

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035353.D
Acq On : 23 Apr 2024 12:05
Operator : SY/MD
Sample : P2157-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RJ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

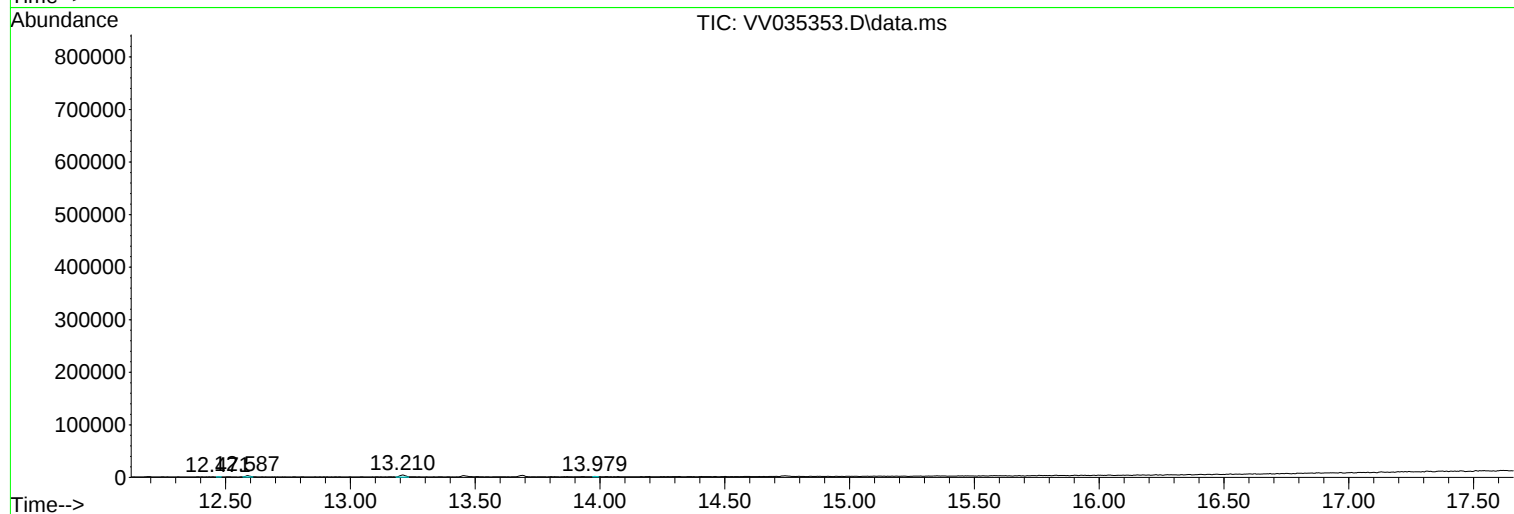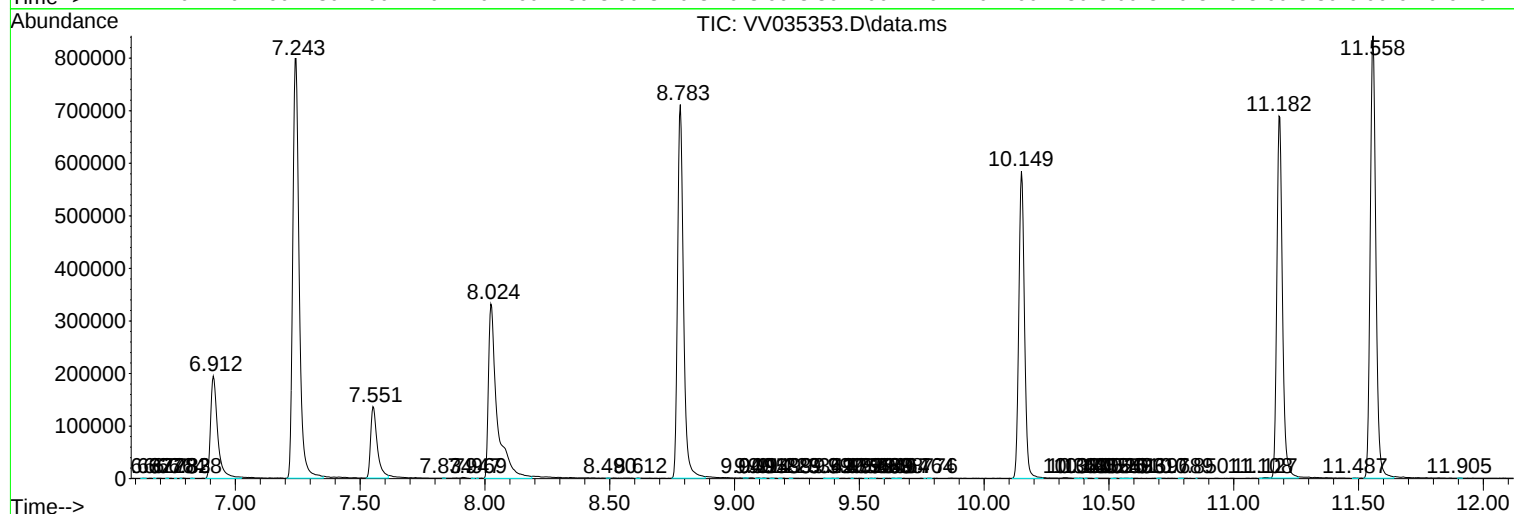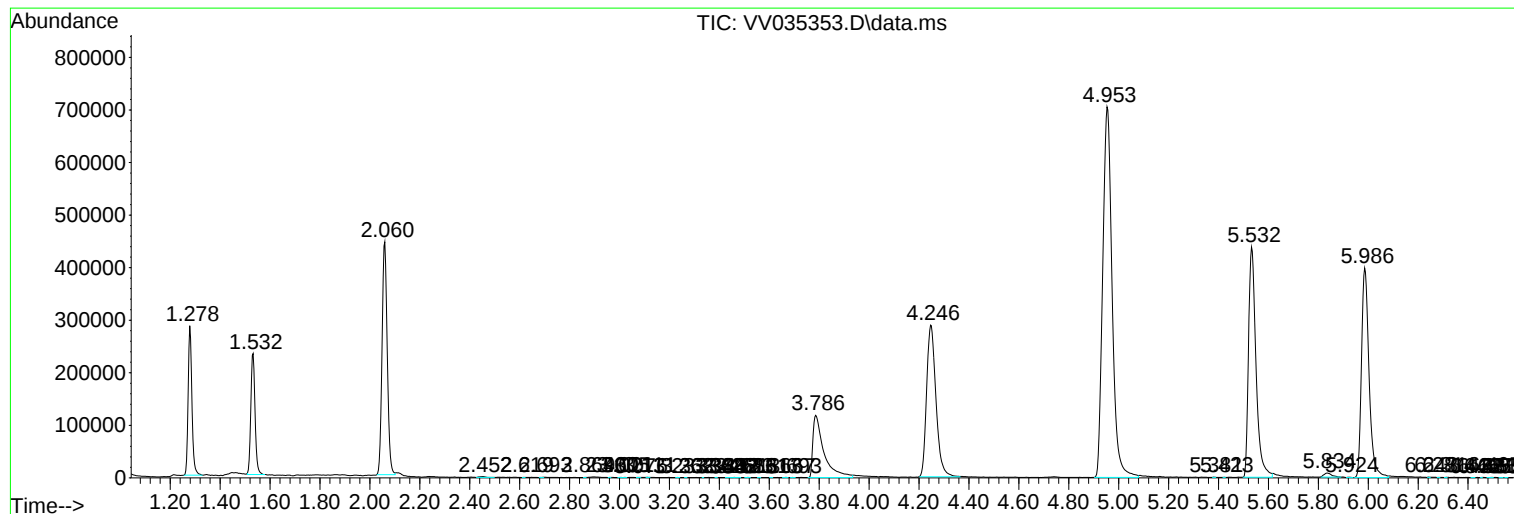

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035353.D
Acq On : 23 Apr 2024 12:05
Operator : SY/MD
Sample : P2157-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RJ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035353.D
Acq On : 23 Apr 2024 12:05
Operator : SY/MD
Sample : P2157-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RJ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------