

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035354.D
 Acq On : 23 Apr 2024 12:28
 Operator : SY/MD
 Sample : P2157-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RJ9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035354.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rBV	278987	295255	16.45%	2.077%
2	1.529	145	152	167	rVB	226186	266754	14.86%	1.876%
3	2.056	307	316	334	rBV	432420	630446	35.13%	4.434%
4	2.490	449	451	456	rVB2	354	220	0.01%	0.002%
5	2.555	464	471	472	rBV3	1364	1298	0.07%	0.009%
6	2.966	597	599	600	rBV3	159	67	0.00%	0.000%
7	3.027	616	618	621	rVB2	230	127	0.01%	0.001%
8	3.043	621	623	625	rVB2	180	89	0.00%	0.001%
9	3.076	630	633	635	rBV	172	127	0.01%	0.001%
10	3.246	684	686	689	rVB	260	143	0.01%	0.001%
11	3.265	689	692	693	rBV	240	141	0.01%	0.001%
12	3.310	703	706	708	rBV	202	122	0.01%	0.001%
13	3.387	725	730	735	rBV3	392	437	0.02%	0.003%
14	3.439	744	746	747	rBV	169	73	0.00%	0.001%
15	3.471	750	756	758	rBV2	192	230	0.01%	0.002%
16	3.564	782	785	787	rBV	128	65	0.00%	0.000%
17	3.609	797	799	801	rVV2	257	99	0.01%	0.001%
18	3.622	801	803	806	rVB	316	163	0.01%	0.001%
19	3.638	806	808	815	rVB2	235	203	0.01%	0.001%
20	3.670	815	818	819	rBV	194	109	0.01%	0.001%
21	3.680	819	821	826	rBV2	197	195	0.01%	0.001%
22	3.722	831	834	838	rVB2	154	116	0.01%	0.001%
23	3.786	844	854	899	rBV	125108	377283	21.02%	2.654%
24	4.246	983	997	1028	rBV	282856	730349	40.69%	5.137%
25	4.690	1132	1135	1136	rBV2	511	257	0.01%	0.002%
26	4.773	1159	1161	1166	rBV3	391	240	0.01%	0.002%
27	4.822	1173	1176	1179	rVB	328	190	0.01%	0.001%
28	4.841	1179	1182	1183	rBV3	188	130	0.01%	0.001%
29	4.889	1194	1197	1200	rBV3	294	256	0.01%	0.002%
30	4.953	1201	1217	1228	rBV2	696911	1793028	99.90%	12.611%
31	5.532	1386	1397	1435	rBV	433241	914059	50.93%	6.429%
32	5.838	1482	1492	1509	rBV5	6667	14986	0.83%	0.105%
33	5.985	1521	1538	1571	rBV	398031	832450	46.38%	5.855%
34	6.272	1625	1627	1630	rVB3	603	330	0.02%	0.002%
35	6.310	1636	1639	1644	rVB4	495	369	0.02%	0.003%
36	6.371	1654	1658	1660	rBV2	244	208	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035354.D
 Acq On : 23 Apr 2024 12:28
 Operator : SY/MD
 Sample : P2157-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RJ9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.432	1675	1677	1678	rBV2	212	75	0.00%	0.001%
38	6.468	1685	1688	1692	rBV3	356	273	0.02%	0.002%
39	6.510	1697	1701	1704	rBV	213	181	0.01%	0.001%
40	6.526	1704	1706	1708	rVB	226	96	0.01%	0.001%
41	6.545	1708	1712	1715	rVB	559	270	0.02%	0.002%
42	6.561	1715	1717	1719	rBV2	83	47	0.00%	0.000%
43	6.612	1730	1733	1737	rBV2	400	321	0.02%	0.002%
44	6.738	1768	1772	1775	rBV3	279	196	0.01%	0.001%
45	6.799	1787	1791	1794	rBV	400	205	0.01%	0.001%
46	6.818	1795	1797	1801	rBV2	333	219	0.01%	0.002%
47	6.844	1803	1805	1808	rVB2	290	163	0.01%	0.001%
48	6.911	1816	1826	1863	rBV	192846	380197	21.18%	2.674%
49	7.243	1917	1929	1959	rBV	783093	1402814	78.16%	9.867%
50	7.551	2016	2025	2057	rBV	135340	257129	14.33%	1.809%
51	7.799	2099	2102	2104	rBV2	511	330	0.02%	0.002%
52	7.854	2116	2119	2121	rBV3	699	390	0.02%	0.003%
53	7.915	2136	2138	2141	rVB2	525	245	0.01%	0.002%
54	7.960	2147	2152	2153	rBV2	247	206	0.01%	0.001%
55	7.985	2158	2160	2163	rBV2	557	261	0.01%	0.002%
56	8.024	2163	2172	2221	rBV2	330022	770076	42.91%	5.416%
57	8.458	2304	2307	2309	rBV	549	336	0.02%	0.002%
58	8.619	2354	2357	2360	rBV3	493	373	0.02%	0.003%
59	8.645	2363	2365	2367	rBV2	293	141	0.01%	0.001%
60	8.683	2374	2377	2378	rBV2	415	211	0.01%	0.001%
61	8.783	2397	2408	2412	rBV	750856	1113441	62.04%	7.831%
62	9.066	2493	2496	2499	rBV2	693	516	0.03%	0.004%
63	9.188	2531	2534	2540	rBV4	604	621	0.03%	0.004%
64	9.278	2561	2562	2565	rBV2	299	206	0.01%	0.001%
65	9.313	2571	2573	2574	rBV2	200	76	0.00%	0.001%
66	9.323	2574	2576	2577	rVB2	190	52	0.00%	0.000%
67	9.371	2589	2591	2595	rVB2	565	340	0.02%	0.002%
68	9.403	2597	2601	2604	rBV2	360	222	0.01%	0.002%
69	9.435	2604	2611	2613	rBV3	265	334	0.02%	0.002%
70	9.464	2618	2620	2622	rBV2	319	152	0.01%	0.001%
71	9.532	2638	2641	2644	rVB2	295	196	0.01%	0.001%
72	9.554	2645	2648	2650	rBV2	236	127	0.01%	0.001%
73	9.583	2655	2657	2659	rVB	186	66	0.00%	0.000%
74	9.599	2660	2662	2664	rBV2	237	116	0.01%	0.001%
75	9.673	2683	2685	2686	rBV2	187	86	0.00%	0.001%
76	9.718	2697	2699	2701	rBV	200	93	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035354.D
 Acq On : 23 Apr 2024 12:28
 Operator : SY/MD
 Sample : P2157-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RJ9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

77	9.847	2738	2739	2741	rVB	150	55	0.00%	0.000%
78	9.876	2744	2748	2752	rVV4	326	295	0.02%	0.002%
79	9.956	2771	2773	2775	rBV	217	94	0.01%	0.001%
80	10.037	2796	2798	2800	rBV	226	99	0.01%	0.001%
81	10.149	2821	2833	2865	rBV	584577	917417	51.12%	6.453%
82	10.432	2917	2921	2924	rBV4	341	253	0.01%	0.002%
83	10.542	2952	2955	2959	rBV2	221	144	0.01%	0.001%
84	10.561	2959	2961	2963	rVB	124	29	0.00%	0.000%
85	10.577	2963	2966	2967	rBV	189	82	0.00%	0.001%
86	10.587	2967	2969	2973	rBV3	275	183	0.01%	0.001%
87	10.632	2981	2983	2985	rBV	230	91	0.01%	0.001%
88	10.706	3002	3006	3009	rBV2	275	235	0.01%	0.002%
89	11.033	3104	3108	3111	rBV	236	180	0.01%	0.001%
90	11.053	3111	3114	3117	rBV	261	171	0.01%	0.001%
91	11.120	3126	3135	3144	rBV	32505	52198	2.91%	0.367%
92	11.185	3144	3155	3190	rVB2	716685	1458785	81.28%	10.260%
93	11.558	3259	3271	3300	rBV2	923116	1794737	100.00%	12.623%
94	11.869	3367	3368	3371	rBV2	344	154	0.01%	0.001%
95	12.107	3440	3442	3445	rBV2	281	139	0.01%	0.001%
96	12.355	3517	3519	3520	rBV	588	262	0.01%	0.002%
97	12.445	3545	3547	3553	rVB2	384	230	0.01%	0.002%
98	12.593	3586	3593	3601	rBV6	1377	2067	0.12%	0.015%
99	13.197	3771	3781	3805	rBV	92186	152547	8.50%	1.073%
100	13.683	3922	3932	3941	rBV2	28609	45126	2.51%	0.317%


Sum of corrected areas: 14217586

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035354.D
Acq On : 23 Apr 2024 12:28
Operator : SY/MD
Sample : P2157-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RJ9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

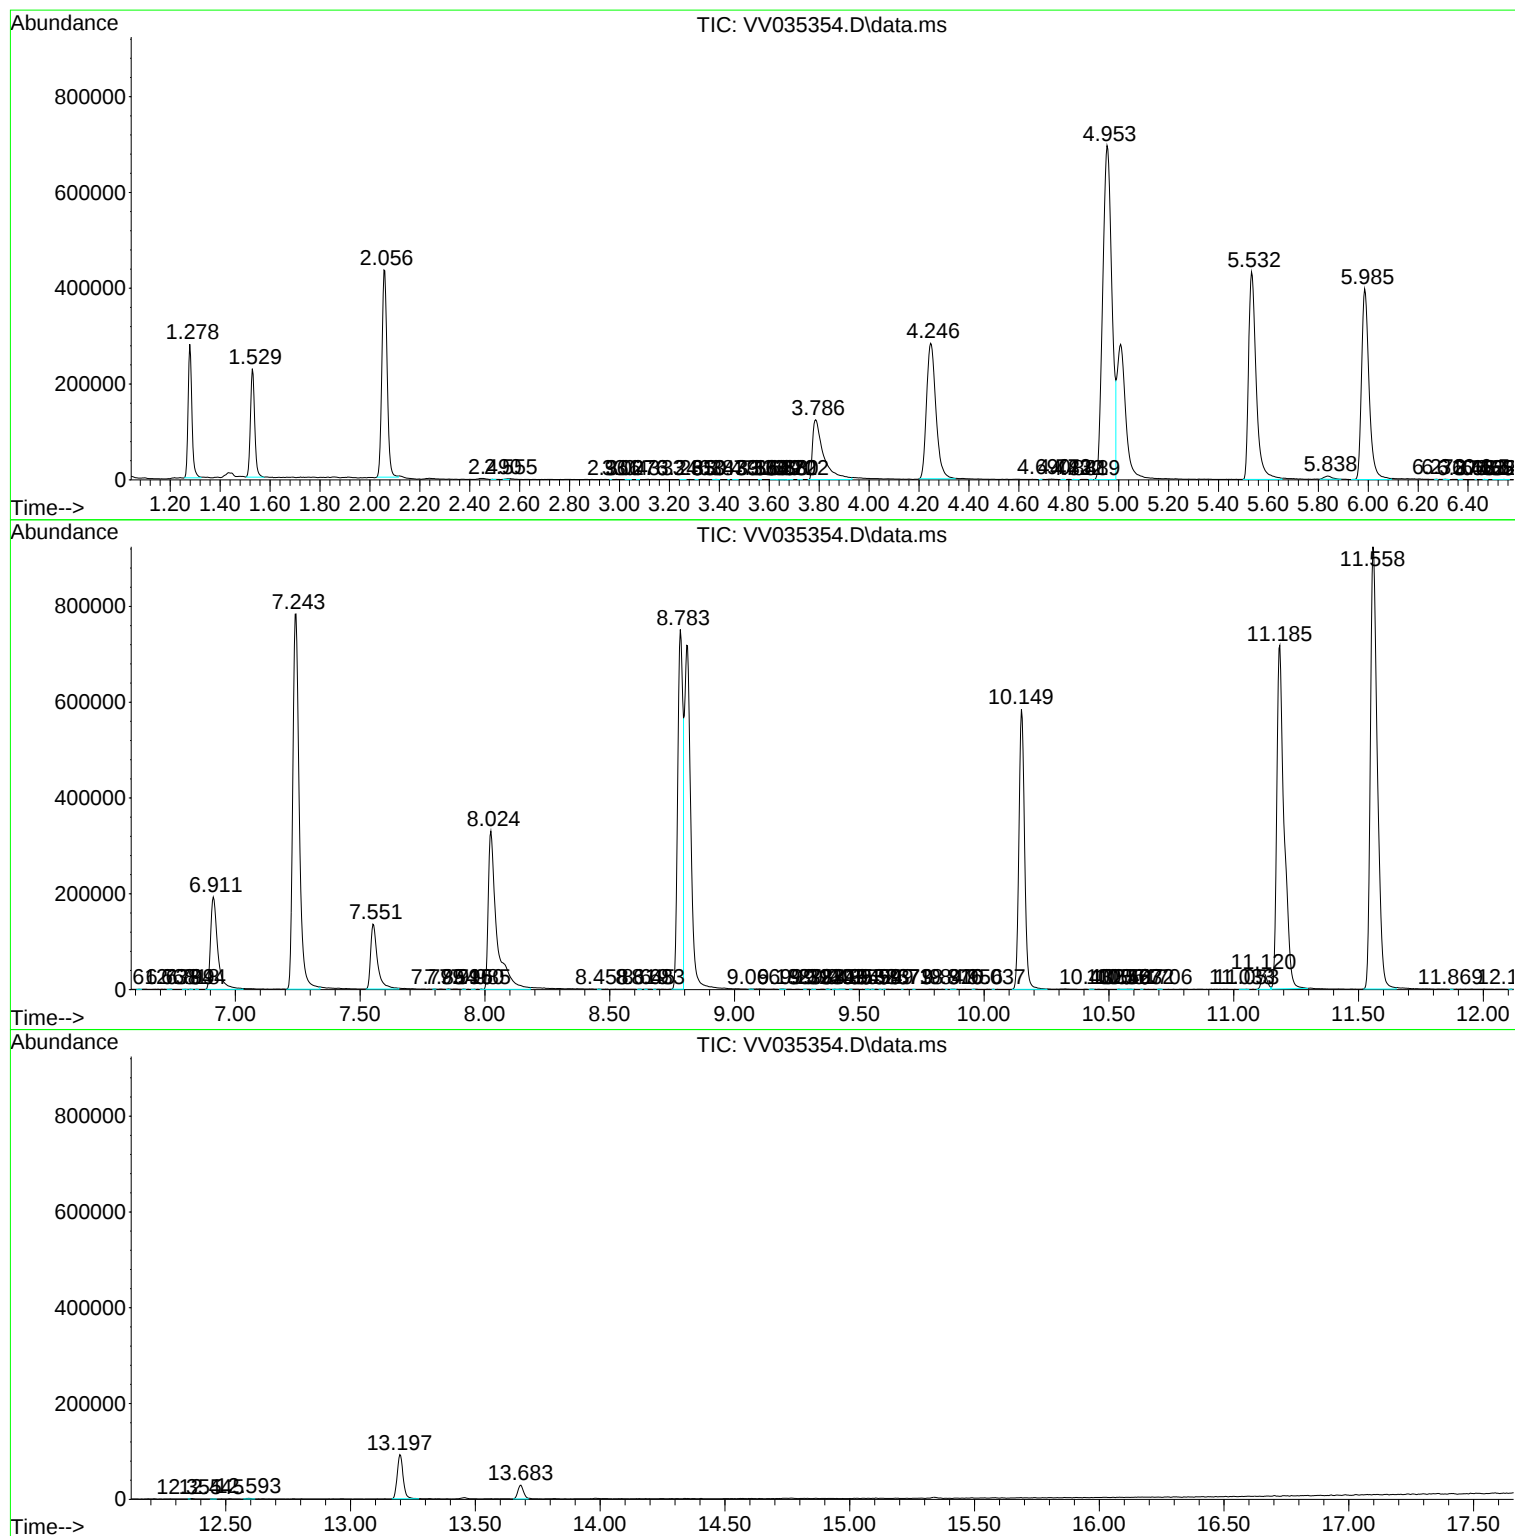

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035354.D
Acq On : 23 Apr 2024 12:28
Operator : SY/MD
Sample : P2157-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RJ9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035354.D
Acq On : 23 Apr 2024 12:28
Operator : SY/MD
Sample : P2157-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RJ9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------