

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035356.D
 Acq On : 23 Apr 2024 13:15
 Operator : SY/MD
 Sample : P2157-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035356.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rBV	277355	290850	16.36%	2.282%
2	1.529	145	152	166	rVB	216277	259316	14.58%	2.035%
3	2.060	307	317	331	rBV	424792	618855	34.80%	4.856%
4	2.722	520	523	526	rBV2	387	252	0.01%	0.002%
5	2.834	555	558	565	rVB4	523	498	0.03%	0.004%
6	2.870	565	569	570	rBV	206	133	0.01%	0.001%
7	2.908	577	581	582	rBV	336	198	0.01%	0.002%
8	2.934	587	589	595	rBV2	176	191	0.01%	0.001%
9	3.056	623	627	631	rBV2	240	147	0.01%	0.001%
10	3.072	631	632	633	rBV	119	46	0.00%	0.000%
11	3.137	650	652	655	rVB2	319	96	0.01%	0.001%
12	3.156	655	658	662	rVB	231	153	0.01%	0.001%
13	3.227	677	680	683	rBV2	350	271	0.02%	0.002%
14	3.320	705	709	711	rBV2	123	84	0.00%	0.001%
15	3.336	711	714	717	rBV	329	285	0.02%	0.002%
16	3.407	733	736	739	rVB3	200	123	0.01%	0.001%
17	3.474	754	757	760	rVB2	319	181	0.01%	0.001%
18	3.487	760	761	763	rVB	203	50	0.00%	0.000%
19	3.519	763	771	775	rBV2	285	300	0.02%	0.002%
20	3.542	775	778	780	rBV2	129	82	0.00%	0.001%
21	3.555	780	782	786	rBV	191	133	0.01%	0.001%
22	3.625	800	804	806	rBV2	131	91	0.01%	0.001%
23	3.638	806	808	811	rVB	211	113	0.01%	0.001%
24	3.654	811	813	816	rBV2	130	59	0.00%	0.000%
25	3.738	835	839	844	rVB	307	221	0.01%	0.002%
26	3.786	845	854	889	rBV	116253	333972	18.78%	2.621%
27	4.249	983	998	1037	rBV	275759	710698	39.96%	5.577%
28	4.751	1153	1154	1156	rBV	226	87	0.00%	0.001%
29	4.957	1201	1218	1263	rBV2	672682	1778353	100.00%	13.955%
30	5.532	1386	1397	1432	rBV	420890	882767	49.64%	6.927%
31	5.834	1482	1491	1508	rBV4	7632	17332	0.97%	0.136%
32	5.985	1526	1538	1575	rBV	384546	806769	45.37%	6.331%
33	6.230	1612	1614	1617	rBV2	353	153	0.01%	0.001%
34	6.336	1644	1647	1651	rBV2	298	233	0.01%	0.002%
35	6.384	1658	1662	1663	rBV2	229	166	0.01%	0.001%
36	6.391	1663	1664	1671	rVV2	386	305	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035356.D
 Acq On : 23 Apr 2024 13:15
 Operator : SY/MD
 Sample : P2157-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.420	1671	1673	1674	rVV	213	101	0.01%	0.001%
38	6.448	1678	1682	1686	rBV3	413	377	0.02%	0.003%
39	6.474	1688	1690	1691	rVB2	253	80	0.00%	0.001%
40	6.526	1704	1706	1708	rBV	173	55	0.00%	0.000%
41	6.538	1708	1710	1715	rVB2	351	213	0.01%	0.002%
42	6.564	1715	1718	1720	rBV2	358	170	0.01%	0.001%
43	6.577	1720	1722	1724	rVB	251	104	0.01%	0.001%
44	6.593	1724	1727	1730	rVB2	137	94	0.01%	0.001%
45	6.616	1730	1734	1737	rBV3	417	332	0.02%	0.003%
46	6.744	1768	1774	1775	rBV2	456	352	0.02%	0.003%
47	6.793	1786	1789	1791	rBV	175	136	0.01%	0.001%
48	6.834	1798	1802	1805	rBV2	196	160	0.01%	0.001%
49	6.911	1816	1826	1855	rBV	184323	359136	20.19%	2.818%
50	7.146	1897	1899	1903	rBV2	425	342	0.02%	0.003%
51	7.243	1917	1929	1965	rBV	767462	1357683	76.34%	10.654%
52	7.551	2016	2025	2055	rBV	131229	246691	13.87%	1.936%
53	7.870	2120	2124	2127	rBV3	471	399	0.02%	0.003%
54	7.947	2145	2148	2149	rBV2	381	152	0.01%	0.001%
55	7.992	2159	2162	2163	rBV2	323	148	0.01%	0.001%
56	8.024	2163	2172	2216	rBV2	320643	746142	41.96%	5.855%
57	8.545	2332	2334	2335	rBV2	382	148	0.01%	0.001%
58	8.638	2361	2363	2365	rBV2	209	118	0.01%	0.001%
59	8.680	2374	2376	2378	rBV	321	177	0.01%	0.001%
60	8.735	2389	2393	2397	rVB3	290	258	0.01%	0.002%
61	8.783	2397	2408	2440	rBV	678350	1131413	63.62%	8.878%
62	9.014	2476	2480	2483	rBV4	614	594	0.03%	0.005%
63	9.262	2554	2557	2559	rBV3	319	178	0.01%	0.001%
64	9.281	2562	2563	2569	rVB2	538	361	0.02%	0.003%
65	9.304	2569	2570	2572	rVB	131	49	0.00%	0.000%
66	9.320	2572	2575	2579	rBV2	384	278	0.02%	0.002%
67	9.387	2591	2596	2599	rBV2	249	233	0.01%	0.002%
68	9.452	2612	2616	2620	rBV2	496	393	0.02%	0.003%
69	9.635	2670	2673	2677	rBV	149	143	0.01%	0.001%
70	9.702	2691	2694	2699	rVB	268	195	0.01%	0.002%
71	9.728	2699	2702	2704	rBV2	138	94	0.01%	0.001%
72	9.770	2712	2715	2718	rVB2	288	188	0.01%	0.001%
73	9.850	2737	2740	2742	rBV	168	107	0.01%	0.001%
74	9.937	2765	2767	2772	rVB	218	124	0.01%	0.001%
75	10.017	2789	2792	2796	rVB2	171	92	0.01%	0.001%
76	10.043	2796	2800	2803	rBV2	178	164	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035356.D
 Acq On : 23 Apr 2024 13:15
 Operator : SY/MD
 Sample : P2157-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.062	2803	2806	2809	rBV2	203	126	0.01%	0.001%
78	10.149	2822	2833	2867	rBV	559460	884217	49.72%	6.939%
79	10.480	2931	2936	2939	rBV3	253	267	0.02%	0.002%
80	10.525	2947	2950	2952	rBV2	193	119	0.01%	0.001%
81	10.792	3030	3033	3037	rVB	451	238	0.01%	0.002%
82	10.895	3063	3065	3067	rBV2	234	108	0.01%	0.001%
83	10.969	3086	3088	3094	rVB2	270	163	0.01%	0.001%
84	11.050	3110	3113	3119	rVB	321	263	0.01%	0.002%
85	11.088	3123	3125	3127	rBV	252	153	0.01%	0.001%
86	11.133	3131	3139	3144	rBV5	1119	1623	0.09%	0.013%
87	11.185	3144	3155	3180	rBV	640165	1027637	57.79%	8.064%
88	11.558	3259	3271	3297	rBV	801946	1265071	71.14%	9.927%
89	11.943	3389	3391	3394	rVB2	535	214	0.01%	0.002%
90	12.008	3408	3411	3413	rBV2	252	167	0.01%	0.001%
91	12.072	3429	3431	3432	rBV2	287	107	0.01%	0.001%
92	12.185	3463	3466	3467	rBV	347	200	0.01%	0.002%
93	12.403	3530	3534	3538	rVB2	314	255	0.01%	0.002%
94	12.548	3577	3579	3581	rBV	336	143	0.01%	0.001%
95	12.583	3587	3590	3593	rBV2	533	451	0.03%	0.004%
96	12.857	3667	3675	3682	rBV3	658	1097	0.06%	0.009%
97	13.207	3777	3784	3793	rBV6	4175	6590	0.37%	0.052%
98	13.381	3835	3838	3841	rBV2	432	398	0.02%	0.003%
99	13.660	3923	3925	3928	rBV	426	278	0.02%	0.002%
100	13.686	3928	3933	3941	rVV3	1500	1957	0.11%	0.015%




Sum of corrected areas: 12743579

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035356.D
Acq On : 23 Apr 2024 13:15
Operator : SY/MD
Sample : P2157-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

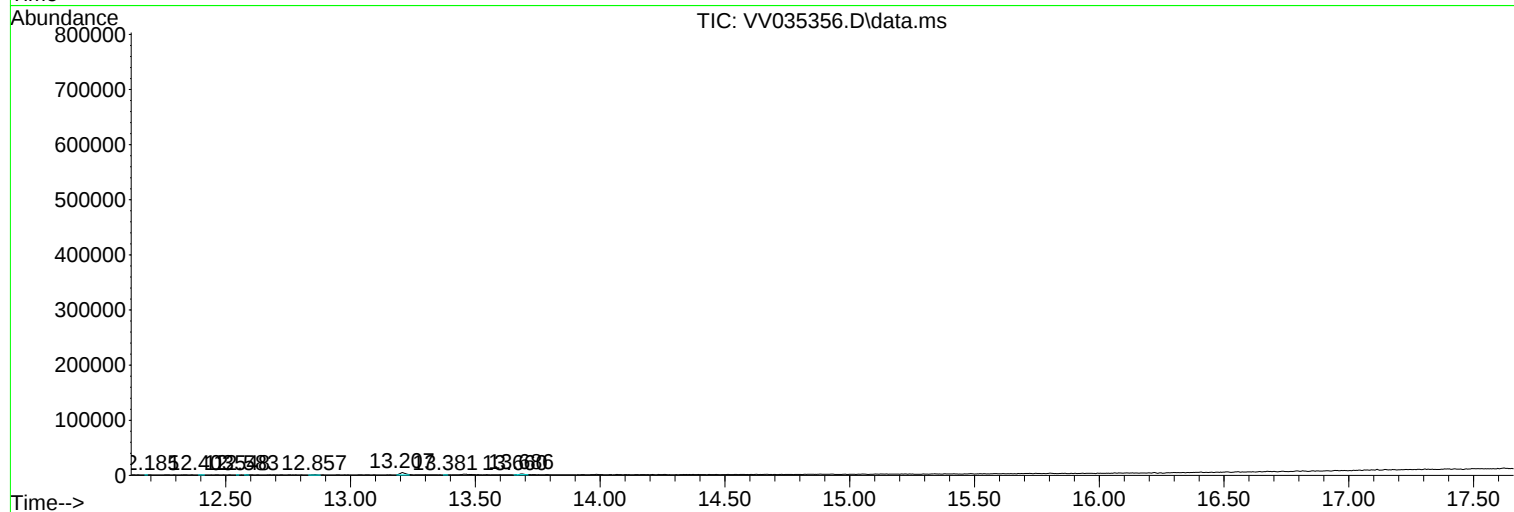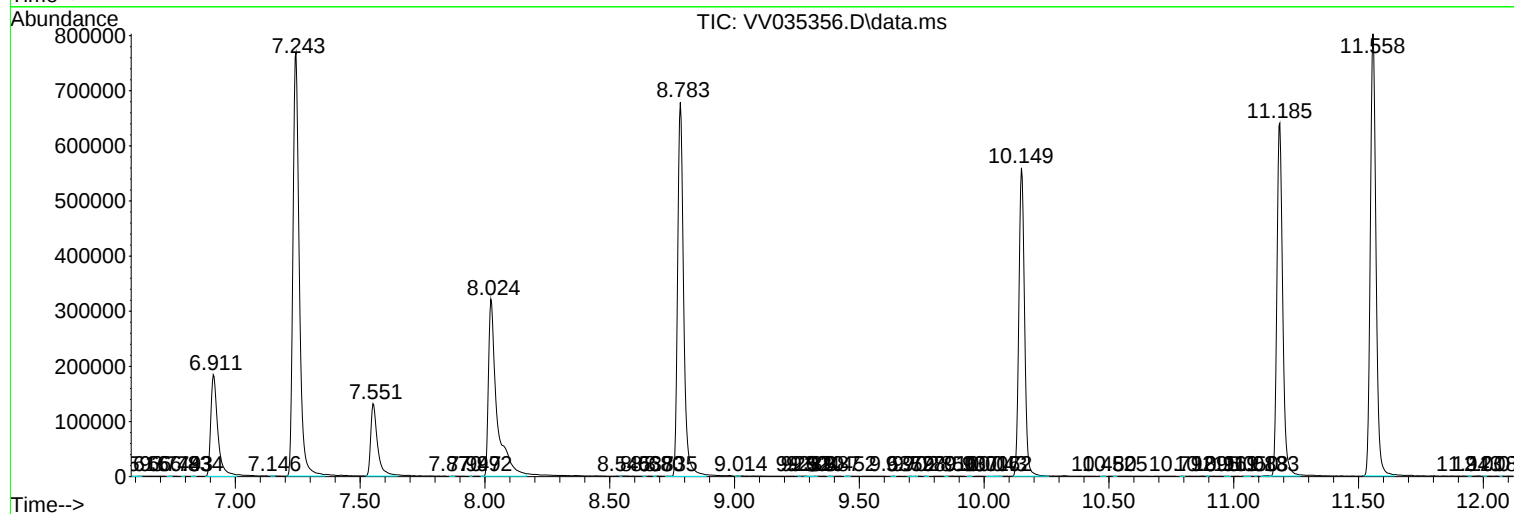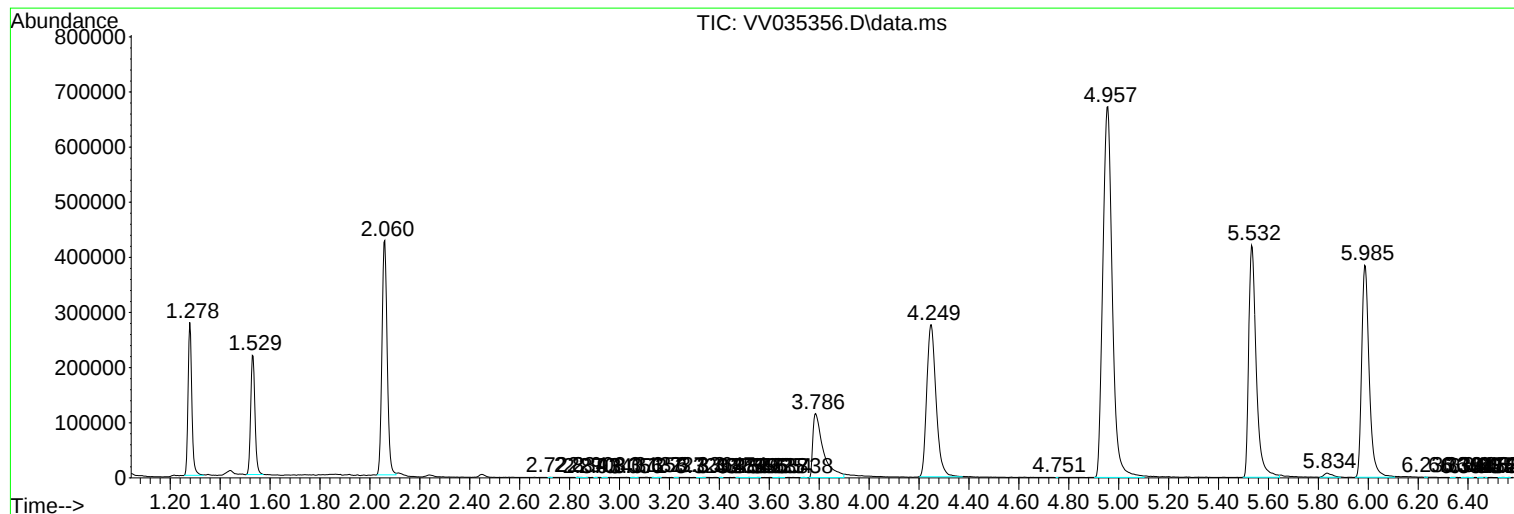

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035356.D
Acq On : 23 Apr 2024 13:15
Operator : SY/MD
Sample : P2157-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035356.D
Acq On : 23 Apr 2024 13:15
Operator : SY/MD
Sample : P2157-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc