

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035358.D
 Acq On : 23 Apr 2024 14:01
 Operator : SY/MD
 Sample : P2158-04DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035358.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rBV	280087	296812	2.40%	0.739%
2	1.532	145	153	167	rVB	245913	284464	2.30%	0.708%
3	2.060	306	317	338	rBV	445968	650867	5.25%	1.620%
4	2.275	382	384	389	rVB3	700	382	0.00%	0.001%
5	2.298	389	391	394	rBV2	459	330	0.00%	0.001%
6	2.391	417	420	425	rBV3	541	531	0.00%	0.001%
7	2.452	430	439	449	rVB4	2426	4371	0.04%	0.011%
8	2.561	464	473	483	rBV4	1917	3609	0.03%	0.009%
9	2.767	533	537	541	rVB2	315	276	0.00%	0.001%
10	2.806	547	549	553	rVB	580	363	0.00%	0.001%
11	2.973	597	601	606	rVB2	366	433	0.00%	0.001%
12	3.089	632	637	641	rVB3	342	342	0.00%	0.001%
13	3.507	763	767	770	rVV2	369	313	0.00%	0.001%
14	3.654	808	813	814	rBV	596	490	0.00%	0.001%
15	3.796	846	857	906	rBV	125987	426089	3.44%	1.061%
16	4.246	981	997	1034	rBV	297977	771761	6.23%	1.921%
17	4.548	1087	1091	1094	rBV3	489	403	0.00%	0.001%
18	4.580	1097	1101	1106	rVB4	689	599	0.00%	0.001%
19	4.738	1137	1150	1162	rBV4	4605	11668	0.09%	0.029%
20	4.957	1200	1218	1222	rBV2	757882	1596005	12.88%	3.973%
21	5.005	1224	1233	1277	rVB	4083502	9021323	72.81%	22.456%
22	5.532	1386	1397	1433	rBV	465073	972681	7.85%	2.421%
23	5.770	1469	1471	1476	rVB3	707	488	0.00%	0.001%
24	5.838	1481	1492	1506	rBV4	6156	13871	0.11%	0.035%
25	5.918	1515	1517	1520	rVB4	624	348	0.00%	0.001%
26	5.986	1522	1538	1577	rBV	412669	862084	6.96%	2.146%
27	6.185	1599	1600	1605	rVB2	655	385	0.00%	0.001%
28	6.317	1639	1641	1646	rVB3	638	429	0.00%	0.001%
29	6.365	1653	1656	1659	rBV4	473	278	0.00%	0.001%
30	6.458	1681	1685	1691	rVV3	434	484	0.00%	0.001%
31	6.596	1724	1728	1732	rBV4	517	505	0.00%	0.001%
32	6.635	1735	1740	1742	rBV2	455	305	0.00%	0.001%
33	6.651	1742	1745	1748	rBV3	333	313	0.00%	0.001%
34	6.725	1763	1768	1771	rBV2	363	318	0.00%	0.001%
35	6.764	1776	1780	1784	rVV4	317	269	0.00%	0.001%
36	6.841	1800	1804	1808	rBV2	323	259	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042324\
 Data File : VW035358.D
 Acq On : 23 Apr 2024 14:01
 Operator : SY/MD
 Sample : P2158-04DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.912	1815	1826	1860	rBV	201449	392392	3.17%	0.977%
38	7.162	1901	1904	1906	rBV3	417	332	0.00%	0.001%
39	7.243	1917	1929	1955	rBV	809973	1438427	11.61%	3.581%
40	7.516	2011	2014	2016	rBV2	569	381	0.00%	0.001%
41	7.551	2016	2025	2053	rVV	140246	261149	2.11%	0.650%
42	7.831	2110	2112	2117	rVB3	492	374	0.00%	0.001%
43	7.915	2132	2138	2143	rVB5	1077	1148	0.01%	0.003%
44	7.979	2154	2158	2162	rBV3	307	311	0.00%	0.001%
45	8.024	2163	2172	2223	rBV2	357225	833967	6.73%	2.076%
46	8.365	2275	2278	2282	rVB3	604	417	0.00%	0.001%
47	8.484	2313	2315	2319	rVB4	547	344	0.00%	0.001%
48	8.532	2327	2330	2332	rVB2	470	280	0.00%	0.001%
49	8.809	2397	2416	2471	rBV	7032254	12390307	100.00%	30.842%
50	9.355	2583	2586	2589	rBV4	358	338	0.00%	0.001%
51	9.419	2603	2606	2608	rBV2	370	243	0.00%	0.001%
52	9.497	2627	2630	2635	rVB2	510	518	0.00%	0.001%
53	9.622	2666	2669	2672	rBV2	364	258	0.00%	0.001%
54	9.661	2678	2681	2684	rBV2	421	283	0.00%	0.001%
55	9.680	2684	2687	2690	rVB2	471	289	0.00%	0.001%
56	9.744	2703	2707	2713	rVB3	426	443	0.00%	0.001%
57	9.776	2714	2717	2719	rBV3	421	244	0.00%	0.001%
58	9.834	2731	2735	2739	rVB3	410	364	0.00%	0.001%
59	9.947	2769	2770	2781	rVB2	454	447	0.00%	0.001%
60	10.014	2785	2791	2792	rBV	451	392	0.00%	0.001%
61	10.149	2821	2833	2861	rBV	600940	949241	7.66%	2.363%
62	10.317	2881	2885	2887	rBV2	683	482	0.00%	0.001%
63	10.493	2936	2940	2945	rVB2	395	416	0.00%	0.001%
64	10.583	2964	2968	2973	rBV4	419	337	0.00%	0.001%
65	10.799	3032	3035	3038	rVB2	451	264	0.00%	0.001%
66	10.989	3090	3094	3098	rVV2	259	299	0.00%	0.001%
67	11.120	3123	3135	3144	rBV	77384	122641	0.99%	0.305%
68	11.204	3144	3161	3193	rVB2	2345691	4639434	37.44%	11.548%
69	11.574	3258	3276	3300	rBV2	1846017	3931087	31.73%	9.785%
70	11.802	3345	3347	3350	rBV3	544	245	0.00%	0.001%
71	11.876	3366	3370	3379	rVB5	549	591	0.00%	0.001%
72	11.915	3379	3382	3385	rBV3	381	256	0.00%	0.001%
73	11.931	3385	3387	3390	rVV2	581	357	0.00%	0.001%
74	11.947	3390	3392	3397	rVB3	564	482	0.00%	0.001%
75	12.162	3455	3459	3462	rVB2	401	323	0.00%	0.001%
76	12.307	3500	3504	3507	rBV2	269	252	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035358.D
 Acq On : 23 Apr 2024 14:01
 Operator : SY/MD
 Sample : P2158-04DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	12.474	3553	3556	3562	rVB3	425	403	0.00%	0.001%
78	12.564	3581	3584	3585	rBV2	458	267	0.00%	0.001%
79	12.593	3588	3593	3609	rVV10	3033	6560	0.05%	0.016%
80	12.728	3632	3635	3637	rBV2	541	288	0.00%	0.001%
81	12.744	3638	3640	3644	rVV3	598	362	0.00%	0.001%
82	12.799	3653	3657	3659	rBV3	351	263	0.00%	0.001%
83	12.915	3690	3693	3695	rVB	452	282	0.00%	0.001%
84	13.030	3726	3729	3731	rBV2	360	244	0.00%	0.001%
85	13.197	3771	3781	3802	rVV	146949	232662	1.88%	0.579%
86	13.349	3826	3828	3834	rVB	433	290	0.00%	0.001%
87	13.458	3855	3862	3869	rBV5	1436	2407	0.02%	0.006%
88	13.683	3922	3932	3944	rBV3	17567	27153	0.22%	0.068%
89	13.841	3979	3981	3985	rVB2	419	262	0.00%	0.001%
90	13.863	3985	3988	3993	rBV3	571	512	0.00%	0.001%
91	13.969	4018	4021	4023	rBV2	532	388	0.00%	0.001%
92	14.040	4040	4043	4048	rVB4	563	387	0.00%	0.001%
93	14.075	4052	4054	4060	rVB3	515	333	0.00%	0.001%
94	14.185	4086	4088	4092	rBV2	377	292	0.00%	0.001%
95	14.439	4165	4167	4170	rBV	421	328	0.00%	0.001%
96	14.763	4262	4268	4274	rBV8	2257	3145	0.03%	0.008%
97	14.914	4311	4315	4317	rBV4	736	509	0.00%	0.001%
98	15.066	4359	4362	4367	rBV5	550	558	0.00%	0.001%
99	15.140	4382	4385	4387	rBV3	682	390	0.00%	0.001%
100	15.384	4457	4461	4463	rBV4	946	696	0.01%	0.002%




Sum of corrected areas: 40173784

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035358.D
Acq On : 23 Apr 2024 14:01
Operator : SY/MD
Sample : P2158-04DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

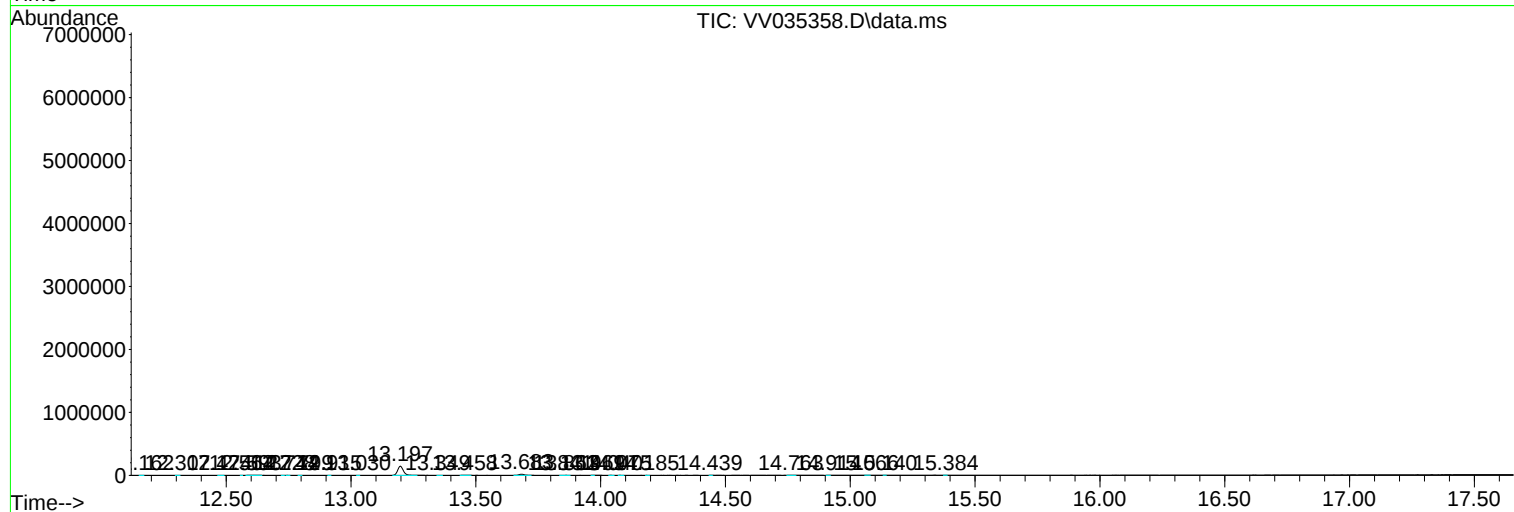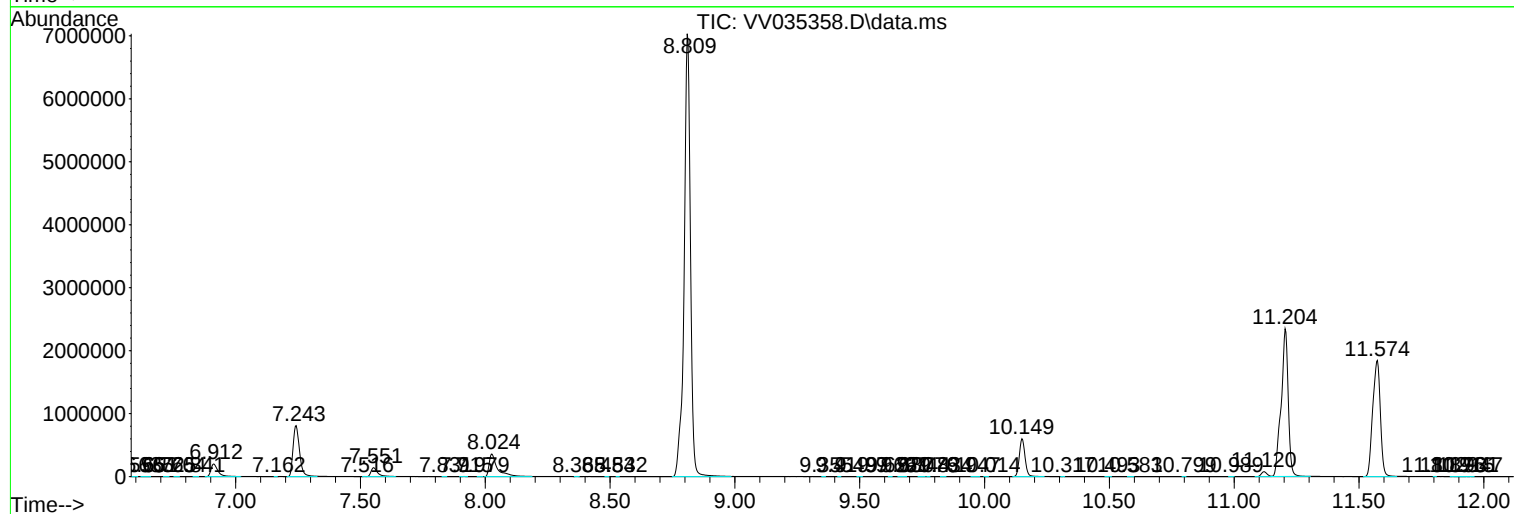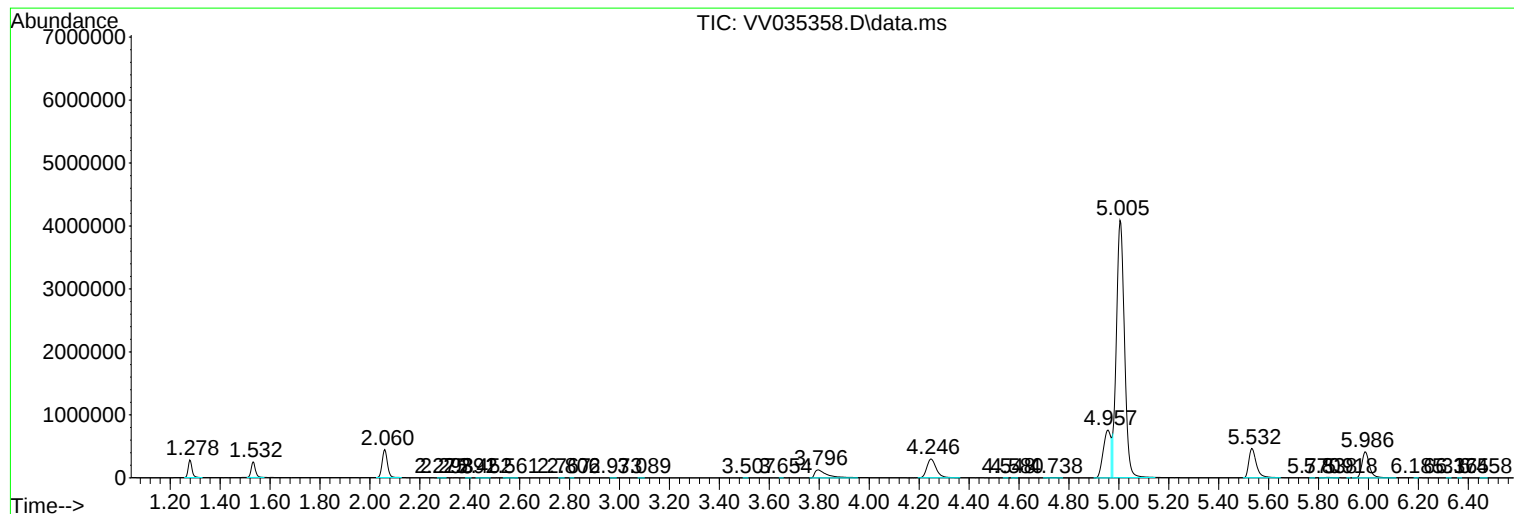

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035358.D
Acq On : 23 Apr 2024 14:01
Operator : SY/MD
Sample : P2158-04DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035358.D
Acq On : 23 Apr 2024 14:01
Operator : SY/MD
Sample : P2158-04DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------