

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035359.D
 Acq On : 23 Apr 2024 14:24
 Operator : SY/MD
 Sample : VIBLK281
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK281

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035359.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	94	rBV	253670	270084	15.52%	2.158%
2	1.532	146	153	168	rVB	218260	254824	14.64%	2.036%
3	2.060	307	317	331	rBV	402475	581596	33.42%	4.647%
4	2.687	510	512	514	rBV	304	154	0.01%	0.001%
5	2.834	554	558	561	rBV2	320	230	0.01%	0.002%
6	2.966	597	599	600	rBV	170	66	0.00%	0.001%
7	2.976	600	602	606	rVV2	382	199	0.01%	0.002%
8	3.105	640	642	646	rVB	297	157	0.01%	0.001%
9	3.127	646	649	651	rBV	186	112	0.01%	0.001%
10	3.137	651	652	658	rVB	279	175	0.01%	0.001%
11	3.172	658	663	666	rBV	371	261	0.01%	0.002%
12	3.195	667	670	676	rVB3	307	305	0.02%	0.002%
13	3.223	676	679	680	rBV	233	108	0.01%	0.001%
14	3.256	685	689	692	rVB2	307	237	0.01%	0.002%
15	3.278	692	696	699	rBV2	368	270	0.02%	0.002%
16	3.362	719	722	725	rBV	182	159	0.01%	0.001%
17	3.387	729	730	733	rVB	243	87	0.00%	0.001%
18	3.407	733	736	738	rBV2	304	214	0.01%	0.002%
19	3.429	741	743	746	rVB2	234	131	0.01%	0.001%
20	3.449	746	749	751	rBV	220	138	0.01%	0.001%
21	3.523	770	772	774	rBV2	178	97	0.01%	0.001%
22	3.555	780	782	787	rBV2	222	141	0.01%	0.001%
23	3.616	795	801	802	rBV	250	200	0.01%	0.002%
24	3.654	810	813	814	rBV	224	131	0.01%	0.001%
25	3.693	821	825	831	rVB3	465	459	0.03%	0.004%
26	3.725	831	835	839	rVB2	169	121	0.01%	0.001%
27	3.751	839	843	846	rBV2	143	123	0.01%	0.001%
28	3.793	846	856	895	rBV	109623	343352	19.73%	2.744%
29	4.246	983	997	1028	rBV	267094	689309	39.61%	5.508%
30	4.667	1124	1128	1130	rBV3	257	232	0.01%	0.002%
31	4.786	1161	1165	1167	rBV3	219	191	0.01%	0.002%
32	4.953	1202	1217	1263	rBV3	648228	1740410	100.00%	13.907%
33	5.313	1326	1329	1331	rVB3	474	202	0.01%	0.002%
34	5.330	1331	1334	1336	rBV	487	286	0.02%	0.002%
35	5.342	1336	1338	1340	rBV2	308	165	0.01%	0.001%
36	5.439	1364	1368	1369	rBV3	379	260	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035359.D
 Acq On : 23 Apr 2024 14:24
 Operator : SY/MD
 Sample : VIBLK281
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK281

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.532	1386	1397	1441	rBV	400939	852174	48.96%	6.810%
38	5.985	1525	1538	1572	rBV	374153	784787	45.09%	6.271%
39	6.342	1645	1649	1650	rBV	209	148	0.01%	0.001%
40	6.365	1654	1656	1657	rBV	263	107	0.01%	0.001%
41	6.452	1681	1683	1685	rBV	218	106	0.01%	0.001%
42	6.477	1689	1691	1698	rVB2	182	126	0.01%	0.001%
43	6.516	1698	1703	1708	rBV2	204	227	0.01%	0.002%
44	6.548	1711	1713	1714	rBV	204	70	0.00%	0.001%
45	6.612	1730	1733	1736	rBV	438	292	0.02%	0.002%
46	6.628	1736	1738	1741	rBV2	326	178	0.01%	0.001%
47	6.641	1741	1742	1743	rBV2	183	69	0.00%	0.001%
48	6.674	1748	1752	1757	rVB3	306	341	0.02%	0.003%
49	6.702	1757	1761	1764	rBV2	251	128	0.01%	0.001%
50	6.731	1768	1770	1771	rBV	265	104	0.01%	0.001%
51	6.786	1785	1787	1791	rVB3	295	163	0.01%	0.001%
52	6.809	1791	1794	1795	rBV	120	73	0.00%	0.001%
53	6.837	1800	1803	1806	rVB	220	112	0.01%	0.001%
54	6.911	1815	1826	1851	rBV	182663	353905	20.33%	2.828%
55	7.243	1917	1929	1968	rBV	716755	1294598	74.38%	10.345%
56	7.551	2016	2025	2055	rBV	128023	241443	13.87%	1.929%
57	7.812	2104	2106	2112	rVB2	358	289	0.02%	0.002%
58	7.837	2112	2114	2118	rVB3	436	289	0.02%	0.002%
59	7.857	2118	2120	2123	rBV2	505	308	0.02%	0.002%
60	7.876	2123	2126	2129	rBV3	353	205	0.01%	0.002%
61	7.911	2135	2137	2141	rBV2	469	291	0.02%	0.002%
62	7.969	2150	2155	2156	rBV	354	254	0.01%	0.002%
63	8.027	2163	2173	2225	rBV2	312152	772049	44.36%	6.169%
64	8.487	2314	2316	2319	rBV2	292	128	0.01%	0.001%
65	8.548	2333	2335	2336	rBV	400	157	0.01%	0.001%
66	8.603	2350	2352	2355	rBV2	315	243	0.01%	0.002%
67	8.728	2389	2391	2394	rBV	237	101	0.01%	0.001%
68	8.783	2397	2408	2449	rBV	651492	1139691	65.48%	9.107%
69	9.159	2524	2525	2526	rBV	318	89	0.01%	0.001%
70	9.304	2566	2570	2571	rBV	400	203	0.01%	0.002%
71	9.329	2576	2578	2581	rVV3	282	132	0.01%	0.001%
72	9.490	2625	2628	2633	rBV	475	423	0.02%	0.003%
73	9.525	2638	2639	2642	rBV2	283	178	0.01%	0.001%
74	9.686	2685	2689	2690	rBV2	181	115	0.01%	0.001%
75	9.712	2692	2697	2699	rBV2	348	260	0.01%	0.002%
76	9.770	2713	2715	2718	rVB	427	207	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035359.D
 Acq On : 23 Apr 2024 14:24
 Operator : SY/MD
 Sample : VIBLK281
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK281

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.792	2718	2722	2727	rVB2	300	249	0.01%	0.002%
78	9.882	2746	2750	2754	rBV3	300	299	0.02%	0.002%
79	9.934	2764	2766	2769	rVB	354	141	0.01%	0.001%
80	10.062	2804	2806	2808	rBV2	169	109	0.01%	0.001%
81	10.149	2822	2833	2858	rBV	550687	875761	50.32%	6.998%
82	10.361	2897	2899	2904	rBV2	367	353	0.02%	0.003%
83	10.429	2918	2920	2923	rVB2	310	160	0.01%	0.001%
84	10.464	2929	2931	2935	rBV	271	145	0.01%	0.001%
85	10.506	2939	2944	2947	rBV2	384	394	0.02%	0.003%
86	10.612	2974	2977	2980	rBV2	175	126	0.01%	0.001%
87	10.763	3022	3024	3025	rBV2	137	64	0.00%	0.001%
88	10.786	3025	3031	3034	rVV4	385	404	0.02%	0.003%
89	10.866	3053	3056	3059	rBV2	512	362	0.02%	0.003%
90	11.127	3131	3137	3144	rBV6	2112	3342	0.19%	0.027%
91	11.185	3144	3155	3187	rVV	615972	1037470	59.61%	8.290%
92	11.558	3260	3271	3300	rBV	771471	1236501	71.05%	9.881%
93	11.898	3374	3377	3381	rBV	534	407	0.02%	0.003%
94	12.111	3441	3443	3447	rBV2	307	192	0.01%	0.002%
95	12.734	3635	3637	3640	rBV3	361	253	0.01%	0.002%
96	13.008	3718	3722	3726	rBV2	386	335	0.02%	0.003%
97	13.107	3750	3753	3755	rBV	414	325	0.02%	0.003%
98	13.149	3760	3766	3772	rBV2	490	719	0.04%	0.006%
99	13.204	3773	3783	3803	rVV3	12178	22463	1.29%	0.179%
100	13.683	3929	3932	3946	rVB8	2781	3800	0.22%	0.030%




Sum of corrected areas: 12514323

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035359.D
Acq On : 23 Apr 2024 14:24
Operator : SY/MD
Sample : VIBLK281
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK281

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

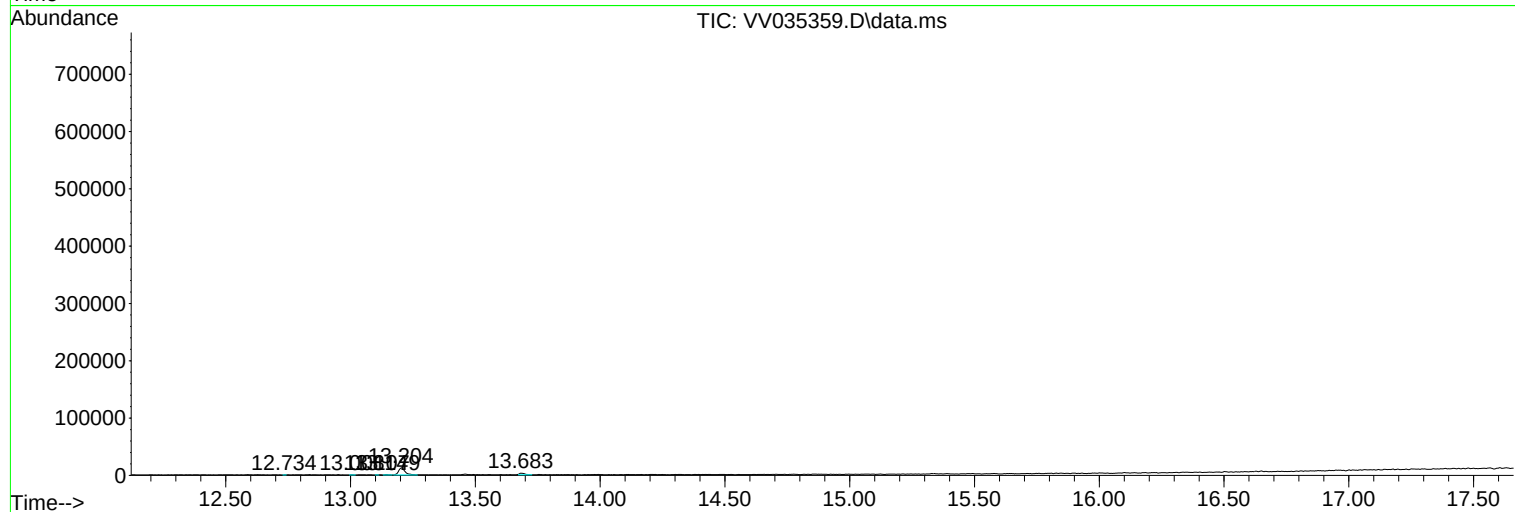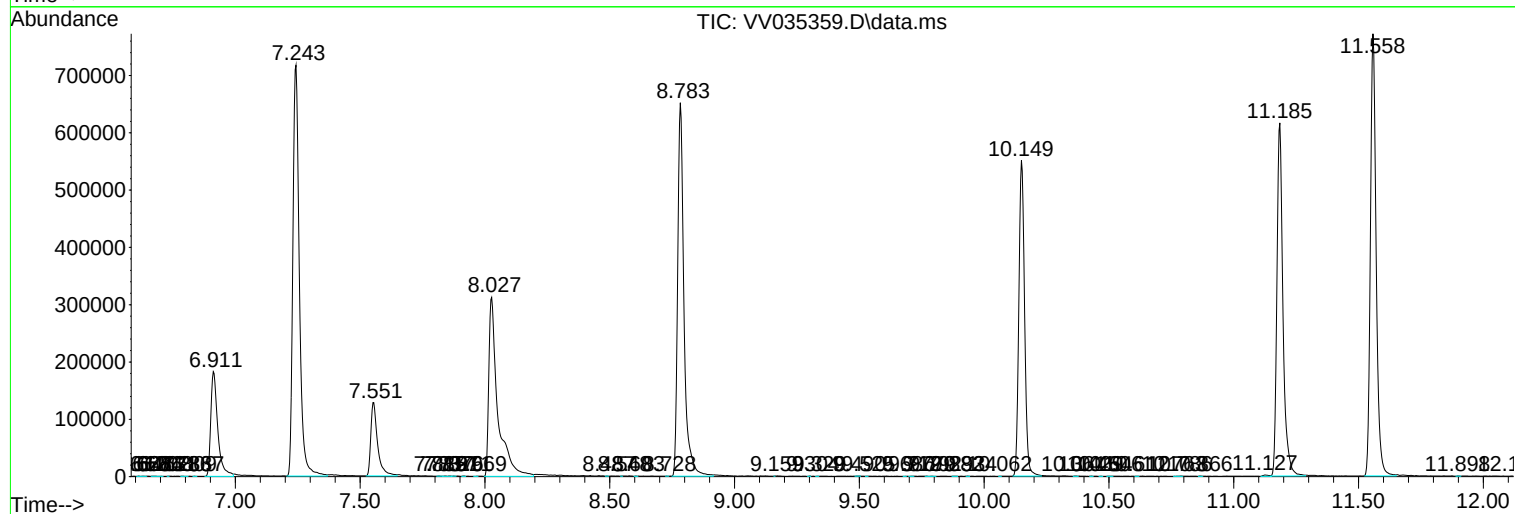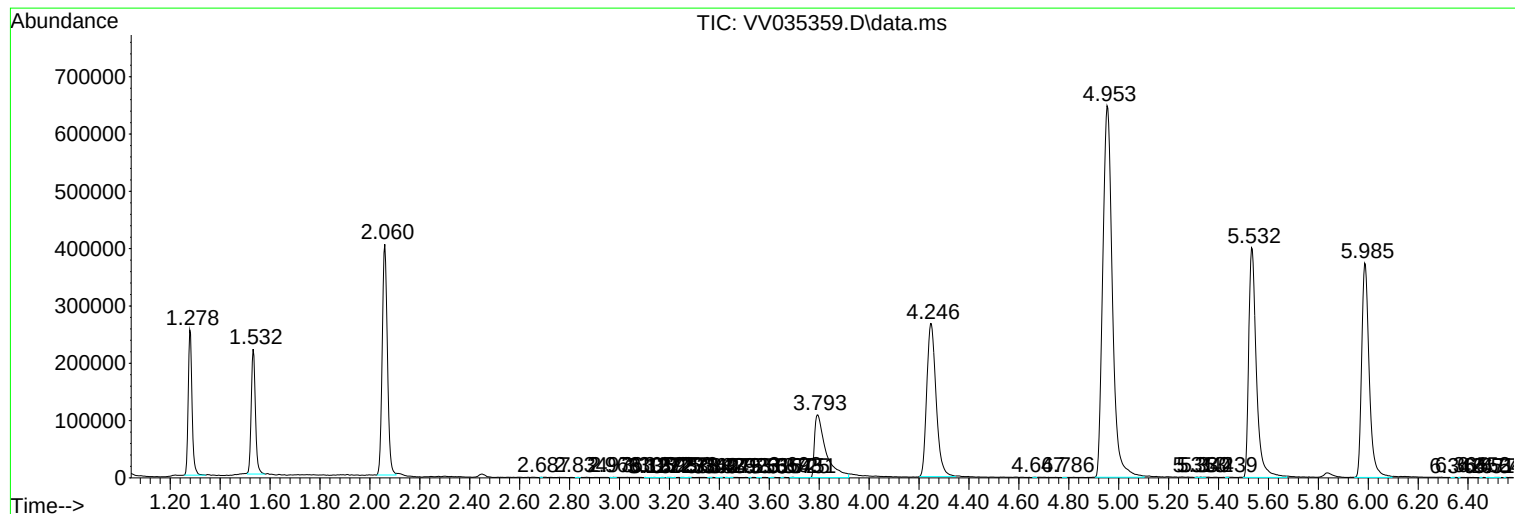

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035359.D
Acq On : 23 Apr 2024 14:24
Operator : SY/MD
Sample : VIBLK281
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK281

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035359.D
Acq On : 23 Apr 2024 14:24
Operator : SY/MD
Sample : VIBLK281
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK281

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------