

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035360.D
 Acq On : 23 Apr 2024 14:47
 Operator : SY/MD
 Sample : P2182-11 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035360.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rBV	270309	288780	5.92%	1.168%
2	1.532	146	153	172	rVB	238058	280022	5.74%	1.133%
3	2.060	307	317	335	rBV	427968	623720	12.79%	2.523%
4	2.516	456	459	461	rBV3	528	337	0.01%	0.001%
5	2.786	538	543	545	rBV2	444	349	0.01%	0.001%
6	2.822	551	554	557	rVB3	344	174	0.00%	0.001%
7	2.999	605	609	613	rBV3	281	299	0.01%	0.001%
8	3.066	627	630	632	rBV	180	129	0.00%	0.001%
9	3.201	669	672	675	rVB2	401	259	0.01%	0.001%
10	3.285	696	698	701	rVB	385	216	0.00%	0.001%
11	3.339	711	715	717	rBV2	200	174	0.00%	0.001%
12	3.388	727	730	738	rBV2	300	339	0.01%	0.001%
13	3.478	754	758	760	rBV2	225	177	0.00%	0.001%
14	3.507	764	767	769	rVV	205	126	0.00%	0.001%
15	3.519	769	771	774	rVB2	382	195	0.00%	0.001%
16	3.536	774	776	781	rVB	173	128	0.00%	0.001%
17	3.561	781	784	786	rBV	393	174	0.00%	0.001%
18	3.613	797	800	802	rBV2	166	128	0.00%	0.001%
19	3.674	815	819	824	rVB2	468	269	0.01%	0.001%
20	3.700	824	827	829	rBV2	201	167	0.00%	0.001%
21	3.793	847	856	903	rBV	120958	393375	8.07%	1.592%
22	4.246	983	997	1035	rBV	285063	745581	15.29%	3.016%
23	4.677	1128	1131	1137	rBV4	462	527	0.01%	0.002%
24	4.732	1142	1148	1149	rBV5	1513	1591	0.03%	0.006%
25	4.812	1170	1173	1177	rBV2	359	354	0.01%	0.001%
26	4.954	1201	1217	1228	rBV2	694830	1811737	37.15%	7.330%
27	5.410	1357	1359	1362	rVB2	586	233	0.00%	0.001%
28	5.445	1367	1370	1373	rBV3	324	250	0.01%	0.001%
29	5.474	1377	1379	1381	rBV2	499	300	0.01%	0.001%
30	5.532	1386	1397	1431	rBV	461988	974696	19.99%	3.943%
31	5.838	1483	1492	1493	rBV5	5058	6495	0.13%	0.026%
32	5.921	1516	1518	1521	rBV3	418	226	0.00%	0.001%
33	5.986	1525	1538	1570	rBV	400942	834361	17.11%	3.376%
34	6.375	1654	1659	1661	rBV	190	168	0.00%	0.001%
35	6.400	1665	1667	1669	rBV2	442	207	0.00%	0.001%
36	6.416	1669	1672	1675	rBV3	255	198	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042324\
 Data File : VW035360.D
 Acq On : 23 Apr 2024 14:47
 Operator : SY/MD
 Sample : P2182-11 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.445	1679	1681	1683	rVB	392	171	0.00%	0.001%
38	6.461	1683	1686	1687	rBV	278	181	0.00%	0.001%
39	6.535	1706	1709	1714	rVB2	347	251	0.01%	0.001%
40	6.577	1718	1722	1726	rBV3	145	137	0.00%	0.001%
41	6.600	1726	1729	1731	rBV2	311	225	0.00%	0.001%
42	6.654	1740	1746	1753	rBV5	535	688	0.01%	0.003%
43	6.744	1769	1774	1776	rBV2	199	186	0.00%	0.001%
44	6.838	1801	1803	1807	rVB2	282	133	0.00%	0.001%
45	6.860	1807	1810	1816	rVB2	198	200	0.00%	0.001%
46	6.912	1816	1826	1864	rBV	195546	383699	7.87%	1.552%
47	7.243	1918	1929	1963	rBV	782218	1402827	28.77%	5.676%
48	7.551	2016	2025	2056	rBV2	140526	261905	5.37%	1.060%
49	7.802	2101	2103	2106	rBV	427	375	0.01%	0.002%
50	7.957	2150	2151	2155	rVB3	451	215	0.00%	0.001%
51	7.989	2155	2161	2163	rBV2	370	284	0.01%	0.001%
52	8.027	2163	2173	2223	rBV2	344075	798144	16.37%	3.229%
53	8.513	2321	2324	2325	rBV2	323	169	0.00%	0.001%
54	8.542	2330	2333	2334	rBV	277	162	0.00%	0.001%
55	8.706	2381	2384	2387	rBV	460	234	0.00%	0.001%
56	8.809	2397	2416	2444	rBV2	2277164	4876441	100.00%	19.729%
57	9.272	2556	2560	2561	rBV2	482	289	0.01%	0.001%
58	9.368	2588	2590	2593	rVB	302	159	0.00%	0.001%
59	9.574	2652	2654	2657	rBV	336	203	0.00%	0.001%
60	9.616	2664	2667	2669	rBV	292	152	0.00%	0.001%
61	9.641	2673	2675	2680	rVB2	432	345	0.01%	0.001%
62	9.667	2681	2683	2689	rVB2	412	370	0.01%	0.001%
63	9.696	2690	2692	2695	rBV2	194	138	0.00%	0.001%
64	9.735	2702	2704	2707	rVB3	430	212	0.00%	0.001%
65	9.783	2715	2719	2724	rVB2	389	318	0.01%	0.001%
66	9.812	2724	2728	2731	rVB2	287	197	0.00%	0.001%
67	9.831	2731	2734	2737	rBV	215	158	0.00%	0.001%
68	9.866	2742	2745	2750	rBV3	284	294	0.01%	0.001%
69	9.928	2762	2764	2767	rBV	237	130	0.00%	0.001%
70	9.963	2772	2775	2776	rBV	204	125	0.00%	0.001%
71	10.005	2785	2788	2792	rBV	383	181	0.00%	0.001%
72	10.040	2794	2799	2803	rBV2	173	212	0.00%	0.001%
73	10.104	2815	2819	2821	rBV2	244	195	0.00%	0.001%
74	10.149	2821	2833	2858	rBV	589506	919845	18.86%	3.722%
75	10.391	2905	2908	2910	rBV	328	174	0.00%	0.001%
76	10.407	2910	2913	2917	rBV2	224	152	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035360.D
 Acq On : 23 Apr 2024 14:47
 Operator : SY/MD
 Sample : P2182-11 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.465	2926	2931	2932	rBV2	218	186	0.00%	0.001%
78	10.542	2952	2955	2956	rBV	255	126	0.00%	0.001%
79	10.709	3005	3007	3012	rVB2	257	130	0.00%	0.001%
80	10.735	3012	3015	3017	rBV2	369	192	0.00%	0.001%
81	10.870	3052	3057	3061	rVB3	442	384	0.01%	0.002%
82	10.895	3062	3065	3071	rVB2	384	307	0.01%	0.001%
83	10.924	3071	3074	3076	rBV2	271	191	0.00%	0.001%
84	10.963	3084	3086	3090	rBV2	288	197	0.00%	0.001%
85	10.982	3090	3092	3095	rVB2	272	133	0.00%	0.001%
86	10.998	3095	3097	3099	rBV	388	214	0.00%	0.001%
87	11.072	3116	3120	3122	rBV	189	154	0.00%	0.001%
88	11.117	3122	3134	3145	rBV	300703	474446	9.73%	1.920%
89	11.204	3145	3161	3186	rVB2	1753286	3813668	78.21%	15.429%
90	11.574	3258	3276	3306	rBV2	2159623	4454500	91.35%	18.022%
91	12.030	3416	3418	3421	rBV	454	244	0.01%	0.001%
92	12.108	3439	3442	3443	rBV2	303	185	0.00%	0.001%
93	12.349	3508	3517	3530	rBV8	4079	7903	0.16%	0.032%
94	12.487	3554	3560	3563	rBV4	626	618	0.01%	0.003%
95	12.693	3617	3624	3636	rBV7	2459	4903	0.10%	0.020%
96	12.882	3680	3683	3685	rBV3	543	420	0.01%	0.002%
97	13.059	3736	3738	3740	rBV	395	244	0.01%	0.001%
98	13.088	3744	3747	3751	rBV3	477	284	0.01%	0.001%
99	13.194	3769	3780	3803	rBV	648884	1015328	20.82%	4.108%
100	13.677	3920	3930	3951	rBV	201710	324923	6.66%	1.315%




Sum of corrected areas: 24716817

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035360.D
Acq On : 23 Apr 2024 14:47
Operator : SY/MD
Sample : P2182-11 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

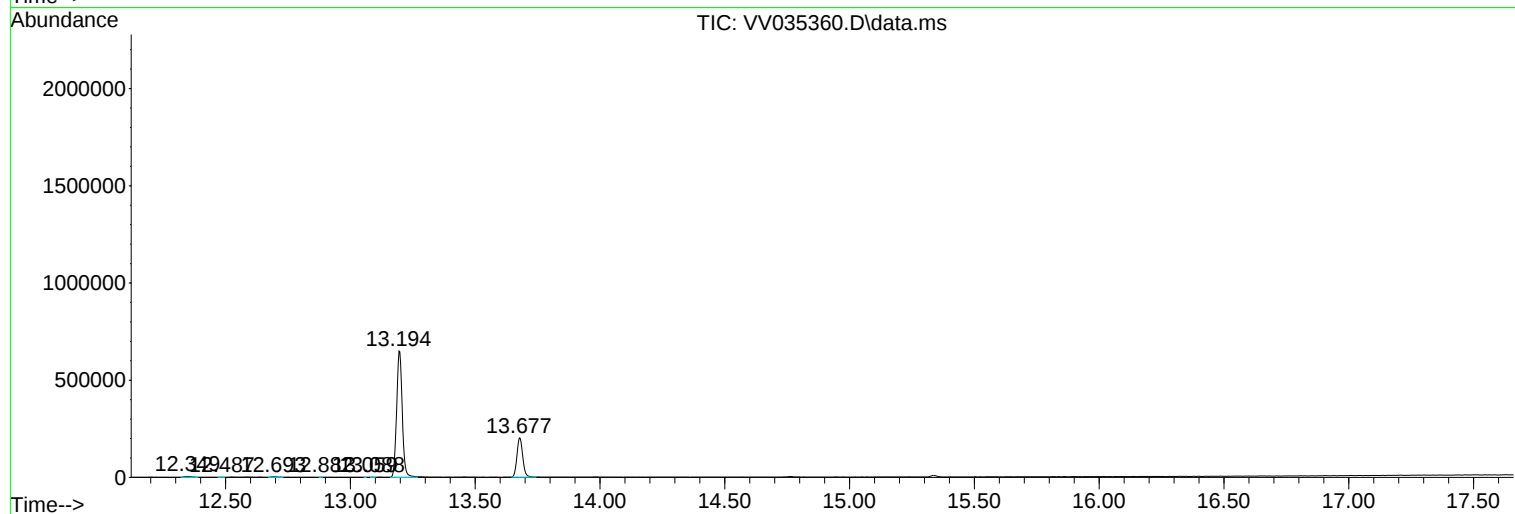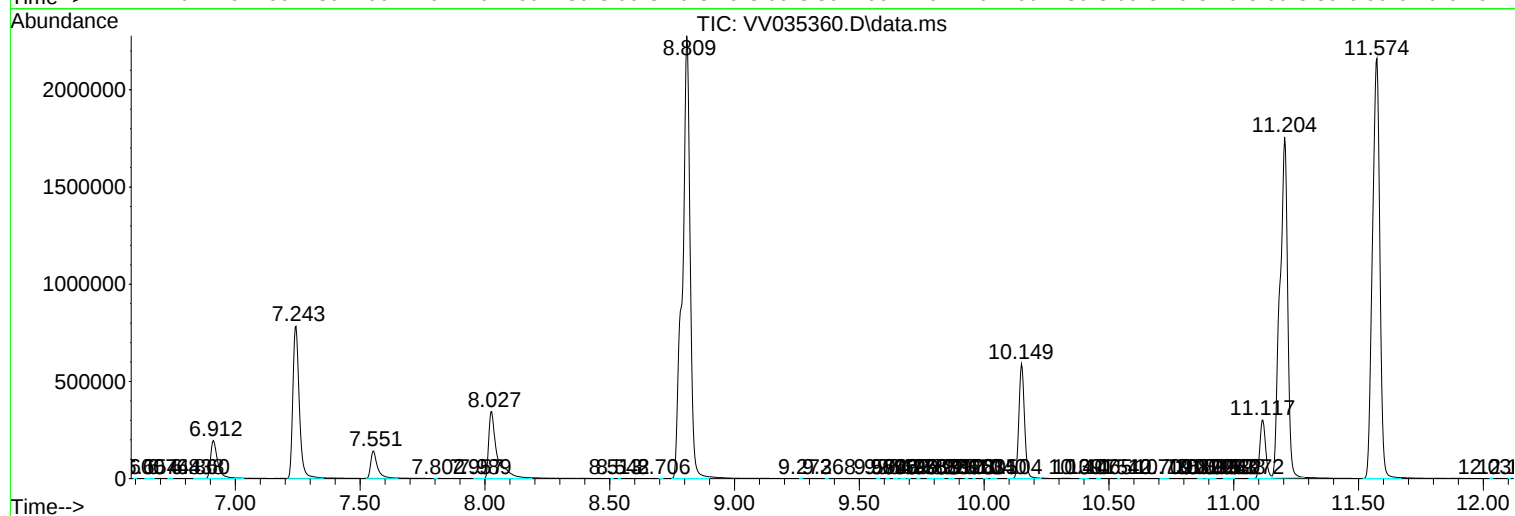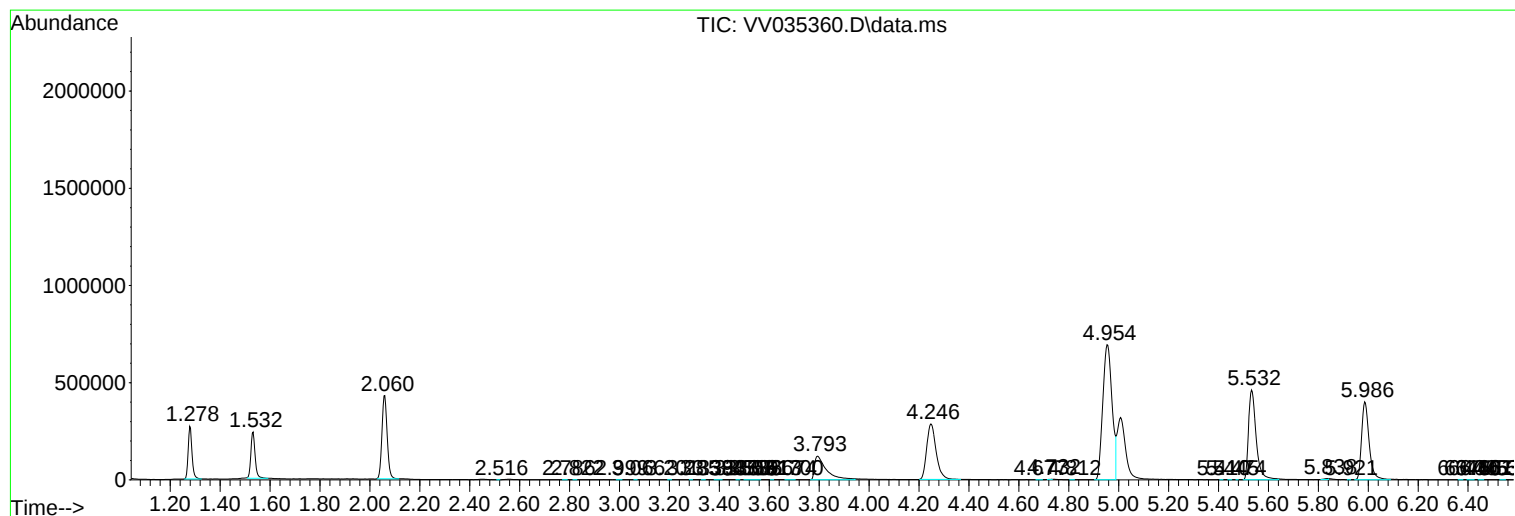

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035360.D
Acq On : 23 Apr 2024 14:47
Operator : SY/MD
Sample : P2182-11 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035360.D
Acq On : 23 Apr 2024 14:47
Operator : SY/MD
Sample : P2182-11 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------