

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035361.D
 Acq On : 23 Apr 2024 15:11
 Operator : SY/MD
 Sample : P2182-09 25X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035361.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	59	rBV4	1900	2175	0.04%	0.009%
2	1.278	67	74	91	rBV	270270	289349	5.88%	1.190%
3	1.532	146	153	170	rVB	237297	275895	5.60%	1.135%
4	2.060	307	317	334	rBV	432627	624799	12.69%	2.570%
5	2.275	382	384	385	rBV2	522	252	0.01%	0.001%
6	2.449	431	438	448	rVB4	2570	4491	0.09%	0.018%
7	2.494	450	452	457	rVB2	451	249	0.01%	0.001%
8	2.558	463	472	482	rBV3	1311	2604	0.05%	0.011%
9	2.622	488	492	500	rBV2	408	576	0.01%	0.002%
10	2.667	500	506	509	rBV3	345	449	0.01%	0.002%
11	2.928	582	587	589	rBV2	357	384	0.01%	0.002%
12	2.963	594	598	601	rVV2	498	455	0.01%	0.002%
13	2.979	601	603	609	rVB3	378	301	0.01%	0.001%
14	3.208	668	674	676	rBV3	290	317	0.01%	0.001%
15	3.359	719	721	728	rVB2	464	377	0.01%	0.002%
16	3.532	772	775	784	rVB	257	260	0.01%	0.001%
17	3.725	828	835	838	rBV2	270	285	0.01%	0.001%
18	3.793	847	856	906	rBV	124035	411357	8.35%	1.692%
19	4.246	980	997	1028	rBV	283602	736445	14.96%	3.030%
20	4.526	1080	1084	1085	rBV2	349	254	0.01%	0.001%
21	4.568	1094	1097	1099	rBV2	454	293	0.01%	0.001%
22	4.584	1100	1102	1107	rVB4	537	299	0.01%	0.001%
23	4.687	1132	1134	1139	rVB4	521	434	0.01%	0.002%
24	4.744	1139	1152	1161	rBV7	1362	3520	0.07%	0.014%
25	4.780	1161	1163	1168	rVB3	383	314	0.01%	0.001%
26	4.806	1168	1171	1174	rBV2	313	249	0.01%	0.001%
27	4.841	1178	1182	1184	rBV3	351	258	0.01%	0.001%
28	4.867	1185	1190	1193	rBV3	358	343	0.01%	0.001%
29	4.953	1201	1217	1227	rBV2	702767	1775677	36.07%	7.305%
30	5.259	1310	1312	1314	rBV3	527	275	0.01%	0.001%
31	5.420	1360	1362	1367	rVB4	633	515	0.01%	0.002%
32	5.532	1386	1397	1427	rBV	458568	958023	19.46%	3.941%
33	5.834	1482	1491	1504	rVV5	6467	14041	0.29%	0.058%
34	5.986	1526	1538	1576	rBV	393788	831428	16.89%	3.420%
35	6.246	1616	1619	1625	rVB5	605	525	0.01%	0.002%
36	6.346	1649	1650	1653	rBV2	455	247	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035361.D
 Acq On : 23 Apr 2024 15:11
 Operator : SY/MD
 Sample : P2182-09 25X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.400	1664	1667	1669	rVV	417	259	0.01%	0.001%
38	6.555	1708	1715	1720	rBV3	430	524	0.01%	0.002%
39	6.664	1745	1749	1755	rVV3	441	453	0.01%	0.002%
40	6.693	1755	1758	1760	rVV2	389	251	0.01%	0.001%
41	6.783	1779	1786	1791	rVV3	417	510	0.01%	0.002%
42	6.912	1815	1826	1857	rBV	195079	377557	7.67%	1.553%
43	7.243	1918	1929	1965	rBV	797435	1405781	28.55%	5.783%
44	7.551	2016	2025	2066	rBV	132989	256229	5.20%	1.054%
45	7.690	2066	2068	2078	rVB4	921	1186	0.02%	0.005%
46	7.780	2093	2096	2100	rBB2	356	271	0.01%	0.001%
47	7.886	2125	2129	2134	rVB3	545	356	0.01%	0.001%
48	7.912	2134	2137	2140	rVB3	668	512	0.01%	0.002%
49	7.953	2148	2150	2154	rVB2	353	270	0.01%	0.001%
50	7.982	2154	2159	2163	rBV2	291	336	0.01%	0.001%
51	8.027	2163	2173	2221	rBV2	341370	803144	16.31%	3.304%
52	8.339	2267	2270	2273	rBV4	570	370	0.01%	0.002%
53	8.375	2279	2281	2288	rVB5	830	857	0.02%	0.004%
54	8.429	2292	2298	2301	rVV4	399	458	0.01%	0.002%
55	8.445	2301	2303	2307	rVV3	651	405	0.01%	0.002%
56	8.471	2307	2311	2314	rVV4	344	313	0.01%	0.001%
57	8.683	2373	2377	2379	rBV2	578	386	0.01%	0.002%
58	8.809	2396	2416	2457	rBV2	2328231	4923499	100.00%	20.255%
59	9.085	2500	2502	2509	rBV4	477	492	0.01%	0.002%
60	9.230	2545	2547	2549	rBV	478	243	0.00%	0.001%
61	9.313	2569	2573	2576	rBV2	455	403	0.01%	0.002%
62	9.403	2596	2601	2604	rBV4	416	415	0.01%	0.002%
63	9.493	2626	2629	2635	rVB3	392	448	0.01%	0.002%
64	9.522	2635	2638	2642	rVB2	293	250	0.01%	0.001%
65	9.548	2642	2646	2651	rBV3	373	457	0.01%	0.002%
66	9.645	2673	2676	2681	rVB3	436	401	0.01%	0.002%
67	9.680	2681	2687	2690	rBV2	602	718	0.01%	0.003%
68	9.760	2708	2712	2715	rBV2	480	370	0.01%	0.002%
69	9.837	2733	2736	2744	rVB3	416	359	0.01%	0.001%
70	9.882	2744	2750	2754	rBV3	431	610	0.01%	0.003%
71	10.001	2784	2787	2790	rBV3	362	245	0.00%	0.001%
72	10.149	2821	2833	2864	rBV	584871	918599	18.66%	3.779%
73	10.297	2876	2879	2881	rBV5	331	239	0.00%	0.001%
74	10.426	2917	2919	2923	rVB3	342	237	0.00%	0.001%
75	10.487	2934	2938	2940	rBV3	483	321	0.01%	0.001%
76	10.526	2945	2950	2953	rVV2	328	326	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042324\
 Data File : VW035361.D
 Acq On : 23 Apr 2024 15:11
 Operator : SY/MD
 Sample : P2182-09 25X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.596	2966	2972	2974	rBV3	233	236	0.00%	0.001%
78	10.783	3025	3030	3031	rBV2	331	240	0.00%	0.001%
79	11.117	3124	3134	3144	rBV	94022	152366	3.09%	0.627%
80	11.204	3145	3161	3187	rVB2	1865018	3943071	80.09%	16.222%
81	11.442	3232	3235	3240	rVB3	827	542	0.01%	0.002%
82	11.571	3258	3275	3303	rBV2	1481688	3324794	67.53%	13.678%
83	11.735	3323	3326	3331	rBV7	780	640	0.01%	0.003%
84	12.005	3407	3410	3412	rBV2	411	261	0.01%	0.001%
85	12.021	3412	3415	3418	rBV4	463	303	0.01%	0.001%
86	12.185	3463	3466	3468	rBV2	368	241	0.00%	0.001%
87	12.342	3506	3515	3533	rBV4	9737	17256	0.35%	0.071%
88	12.525	3562	3572	3585	rBV6	3859	7906	0.16%	0.033%
89	12.590	3585	3592	3597	rBV4	2648	3347	0.07%	0.014%
90	12.693	3616	3624	3635	rVB5	5320	8675	0.18%	0.036%
91	12.857	3668	3675	3676	rBV2	480	426	0.01%	0.002%
92	12.960	3704	3707	3710	rVB3	590	458	0.01%	0.002%
93	12.979	3710	3713	3716	rVB3	414	282	0.01%	0.001%
94	13.024	3720	3727	3732	rVB4	499	733	0.01%	0.003%
95	13.194	3768	3780	3809	rBV	1120664	1756348	35.67%	7.226%
96	13.461	3857	3863	3868	rVB4	952	1308	0.03%	0.005%
97	13.677	3919	3930	3951	rBV	262824	418352	8.50%	1.721%
98	14.294	4120	4122	4127	rBV4	672	522	0.01%	0.002%
99	14.760	4260	4267	4277	rVB6	5811	9378	0.19%	0.039%
100	15.332	4438	4445	4463	rVB3	14300	22903	0.47%	0.094%




Sum of corrected areas: 24307363

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035361.D
Acq On : 23 Apr 2024 15:11
Operator : SY/MD
Sample : P2182-09 25X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

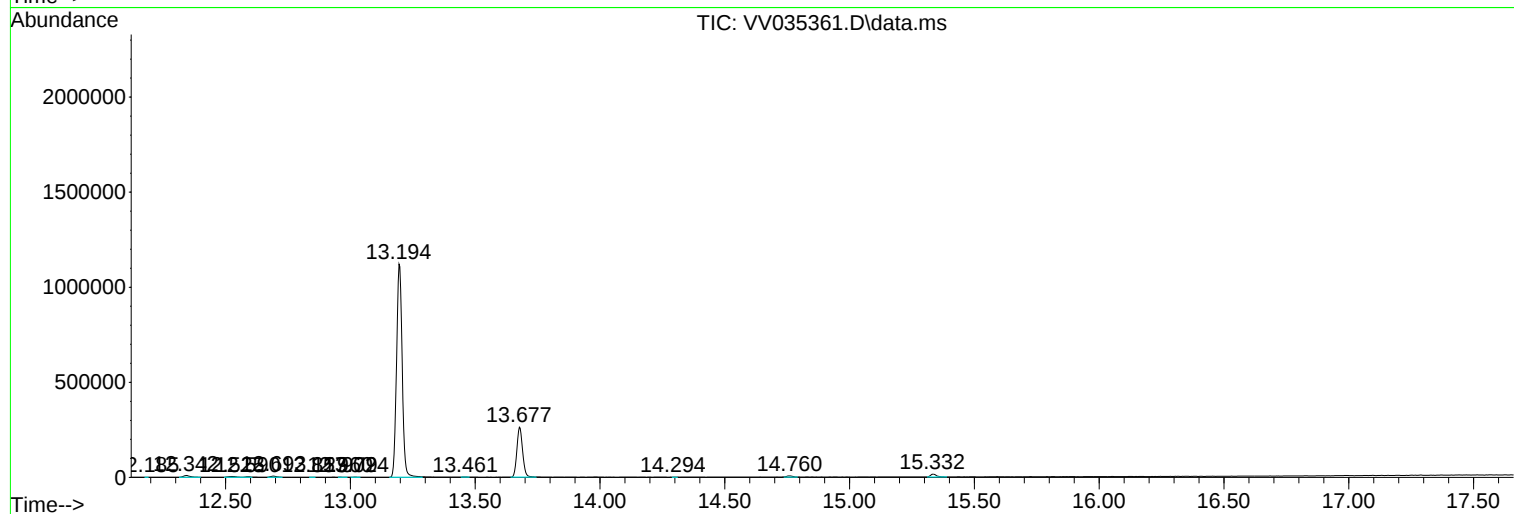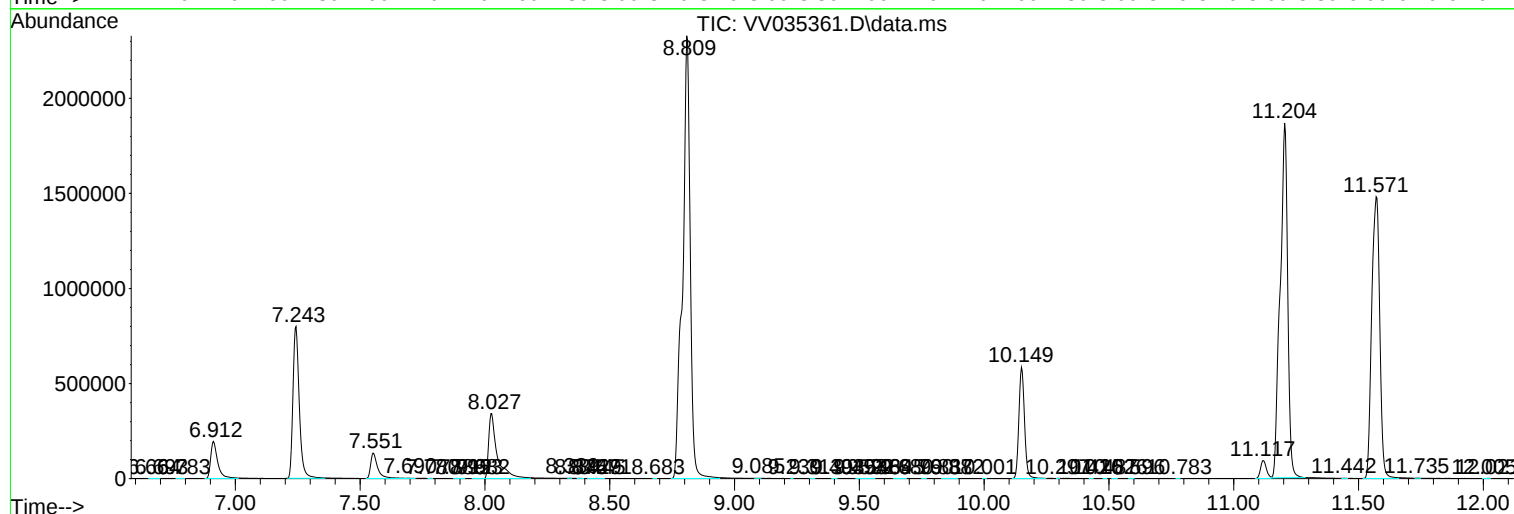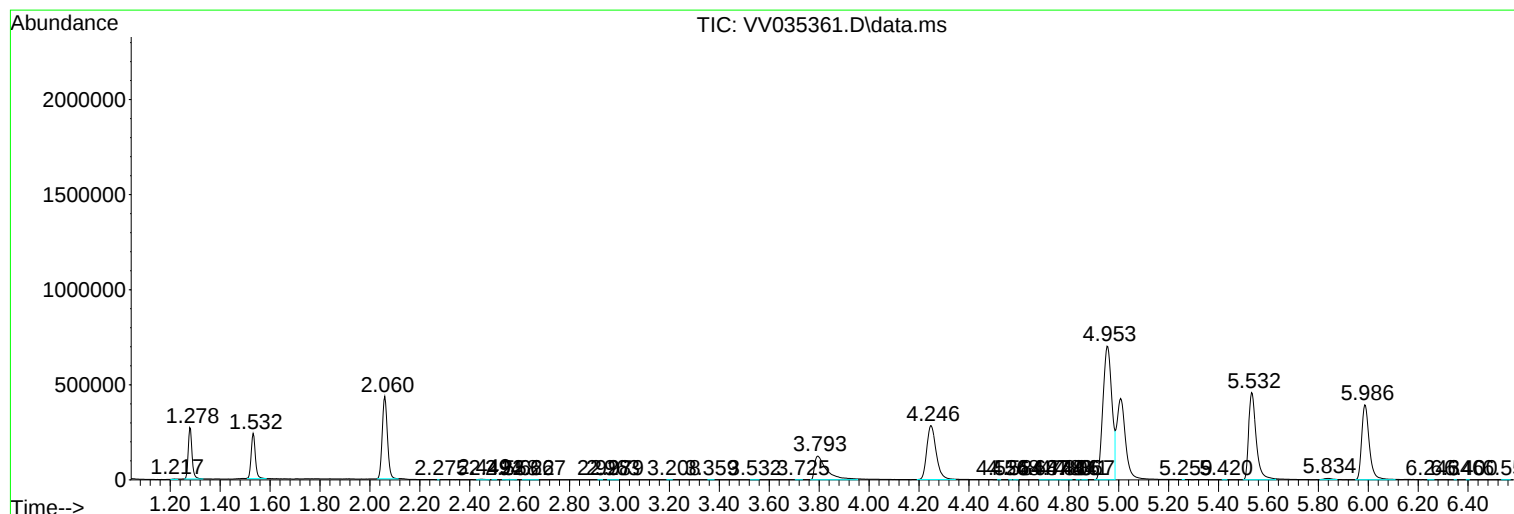

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035361.D
Acq On : 23 Apr 2024 15:11
Operator : SY/MD
Sample : P2182-09 25X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035361.D
Acq On : 23 Apr 2024 15:11
Operator : SY/MD
Sample : P2182-09 25X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------