

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035363.D
 Acq On : 23 Apr 2024 15:57
 Operator : SY/MD
 Sample : P2235-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0810

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.191	41	47	60	rBV	27435	28914	1.67%	0.226%
2	1.278	67	74	88	rVB	253835	275427	15.88%	2.152%
3	1.532	146	153	167	rVB	219167	253034	14.59%	1.977%
4	2.059	307	317	332	rBV	406625	590477	34.05%	4.615%
5	2.352	405	408	411	rBV2	869	775	0.04%	0.006%
6	2.555	466	471	472	rBV3	675	507	0.03%	0.004%
7	2.690	511	513	514	rBV3	549	227	0.01%	0.002%
8	2.725	523	524	526	rVB3	246	62	0.00%	0.000%
9	2.834	554	558	560	rBV	279	247	0.01%	0.002%
10	2.870	568	569	571	rVB2	296	90	0.01%	0.001%
11	2.892	571	576	580	rBV3	513	642	0.04%	0.005%
12	3.024	614	617	620	rBV2	371	290	0.02%	0.002%
13	3.230	678	681	683	rBV2	76	57	0.00%	0.000%
14	3.246	683	686	688	rBV	89	66	0.00%	0.001%
15	3.259	688	690	692	rBV	202	110	0.01%	0.001%
16	3.310	700	706	711	rBV3	319	386	0.02%	0.003%
17	3.339	711	715	717	rVV2	221	163	0.01%	0.001%
18	3.371	722	725	730	rBV2	350	252	0.01%	0.002%
19	3.407	734	736	739	rBV2	181	119	0.01%	0.001%
20	3.442	745	747	750	rBV	147	77	0.00%	0.001%
21	3.458	750	752	759	rBV	258	179	0.01%	0.001%
22	3.516	765	770	774	rVB2	311	319	0.02%	0.002%
23	3.551	774	781	784	rBV3	294	295	0.02%	0.002%
24	3.574	784	788	790	rBV2	129	90	0.01%	0.001%
25	3.596	791	795	798	rBV2	709	565	0.03%	0.004%
26	3.683	819	822	827	rBV2	190	149	0.01%	0.001%
27	3.706	827	829	831	rBV	235	157	0.01%	0.001%
28	3.796	848	857	895	rBV	107787	341125	19.67%	2.666%
29	4.249	983	998	1036	rBV2	281845	812056	46.83%	6.346%
30	4.667	1126	1128	1131	rBV2	204	128	0.01%	0.001%
31	4.699	1137	1138	1140	rBV	197	75	0.00%	0.001%
32	4.815	1171	1174	1175	rBV	212	86	0.00%	0.001%
33	4.854	1181	1186	1187	rBV	227	166	0.01%	0.001%
34	4.957	1202	1218	1265	rBV2	654258	1734158	100.00%	13.553%
35	5.291	1318	1322	1323	rBV2	380	226	0.01%	0.002%
36	5.384	1349	1351	1353	rBV	321	150	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035363.D
 Acq On : 23 Apr 2024 15:57
 Operator : SY/MD
 Sample : P2235-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0810

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.532	1386	1397	1430	rBV	413942	881772	50.85%	6.891%
38	5.837	1482	1492	1508	rBV3	9168	20702	1.19%	0.162%
39	5.985	1526	1538	1575	rBV	380295	790488	45.58%	6.178%
40	6.249	1617	1620	1622	rBV4	518	335	0.02%	0.003%
41	6.342	1646	1649	1652	rBV2	326	291	0.02%	0.002%
42	6.394	1662	1665	1666	rBV	241	111	0.01%	0.001%
43	6.442	1669	1680	1696	rBV2	12147	25921	1.49%	0.203%
44	6.545	1710	1712	1713	rBV	313	149	0.01%	0.001%
45	6.583	1721	1724	1725	rBV	151	85	0.00%	0.001%
46	6.603	1725	1730	1733	rBV3	407	347	0.02%	0.003%
47	6.641	1739	1742	1743	rBV	246	145	0.01%	0.001%
48	6.757	1776	1778	1780	rBV	193	110	0.01%	0.001%
49	6.809	1791	1794	1795	rBV2	185	100	0.01%	0.001%
50	6.873	1813	1814	1816	rVB2	230	64	0.00%	0.001%
51	6.911	1816	1826	1863	rBV	183255	361388	20.84%	2.824%
52	7.243	1918	1929	1955	rBV	741224	1309801	75.53%	10.236%
53	7.551	2016	2025	2049	rBV	127224	238789	13.77%	1.866%
54	7.860	2117	2121	2122	rBV2	571	422	0.02%	0.003%
55	7.934	2142	2144	2145	rBV	326	164	0.01%	0.001%
56	7.963	2151	2153	2155	rBV	191	115	0.01%	0.001%
57	8.027	2164	2173	2212	rBV2	306008	748461	43.16%	5.849%
58	8.638	2362	2363	2364	rBV2	162	46	0.00%	0.000%
59	8.667	2370	2372	2374	rBV	321	178	0.01%	0.001%
60	8.677	2374	2375	2376	rVB	217	53	0.00%	0.000%
61	8.783	2397	2408	2435	rBV	671453	1133437	65.36%	8.858%
62	9.085	2500	2502	2504	rBV3	463	292	0.02%	0.002%
63	9.204	2535	2539	2542	rBV2	467	373	0.02%	0.003%
64	9.265	2556	2558	2561	rBV	287	156	0.01%	0.001%
65	9.297	2565	2568	2569	rBV	280	107	0.01%	0.001%
66	9.307	2569	2571	2574	rBV2	286	135	0.01%	0.001%
67	9.384	2589	2595	2598	rBV2	239	262	0.02%	0.002%
68	9.406	2598	2602	2604	rVB	219	143	0.01%	0.001%
69	9.429	2604	2609	2611	rBV2	427	424	0.02%	0.003%
70	9.461	2616	2619	2622	rBV2	210	124	0.01%	0.001%
71	9.535	2638	2642	2645	rBV2	789	666	0.04%	0.005%
72	9.635	2670	2673	2674	rBV	203	101	0.01%	0.001%
73	9.673	2679	2685	2687	rBV	287	247	0.01%	0.002%
74	9.706	2692	2695	2697	rBV2	235	175	0.01%	0.001%
75	9.796	2719	2723	2726	rBV3	411	314	0.02%	0.002%
76	9.831	2731	2734	2736	rBV2	416	263	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035363.D
 Acq On : 23 Apr 2024 15:57
 Operator : SY/MD
 Sample : P2235-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0810

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.066	2802	2807	2809	rBV	162	150	0.01%	0.001%
78	10.149	2821	2833	2860	rBV	545266	865508	49.91%	6.764%
79	10.323	2883	2887	2899	rVB6	1911	2637	0.15%	0.021%
80	10.532	2949	2952	2954	rBV2	321	244	0.01%	0.002%
81	10.570	2958	2964	2966	rBV2	243	226	0.01%	0.002%
82	10.622	2975	2980	2983	rBB2	299	267	0.02%	0.002%
83	10.644	2984	2987	2990	rBV2	308	231	0.01%	0.002%
84	10.709	3000	3007	3009	rBV3	312	371	0.02%	0.003%
85	10.734	3013	3015	3022	rVB2	509	367	0.02%	0.003%
86	10.767	3022	3025	3027	rVB	169	91	0.01%	0.001%
87	10.795	3030	3034	3037	rVB	285	221	0.01%	0.002%
88	10.815	3037	3040	3045	rBV2	314	254	0.01%	0.002%
89	10.950	3080	3082	3085	rBV2	359	228	0.01%	0.002%
90	11.095	3124	3127	3128	rBV2	257	164	0.01%	0.001%
91	11.123	3133	3136	3144	rVV5	1418	1921	0.11%	0.015%
92	11.185	3144	3155	3183	rBV	654790	1067751	61.57%	8.345%
93	11.558	3259	3271	3295	rBV	776545	1255624	72.41%	9.813%
94	11.966	3396	3398	3403	rVB	407	237	0.01%	0.002%
95	12.030	3415	3418	3421	rVB	368	191	0.01%	0.001%
96	12.448	3545	3548	3551	rBV3	424	328	0.02%	0.003%
97	12.924	3693	3696	3700	rBV2	568	362	0.02%	0.003%
98	12.947	3700	3703	3708	rBV3	391	370	0.02%	0.003%
99	13.204	3772	3783	3796	rBV2	18823	31603	1.82%	0.247%
100	13.686	3926	3933	3942	rVB4	4484	7237	0.42%	0.057%




Sum of corrected areas: 12795685

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035363.D
Acq On : 23 Apr 2024 15:57
Operator : SY/MD
Sample : P2235-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0810

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

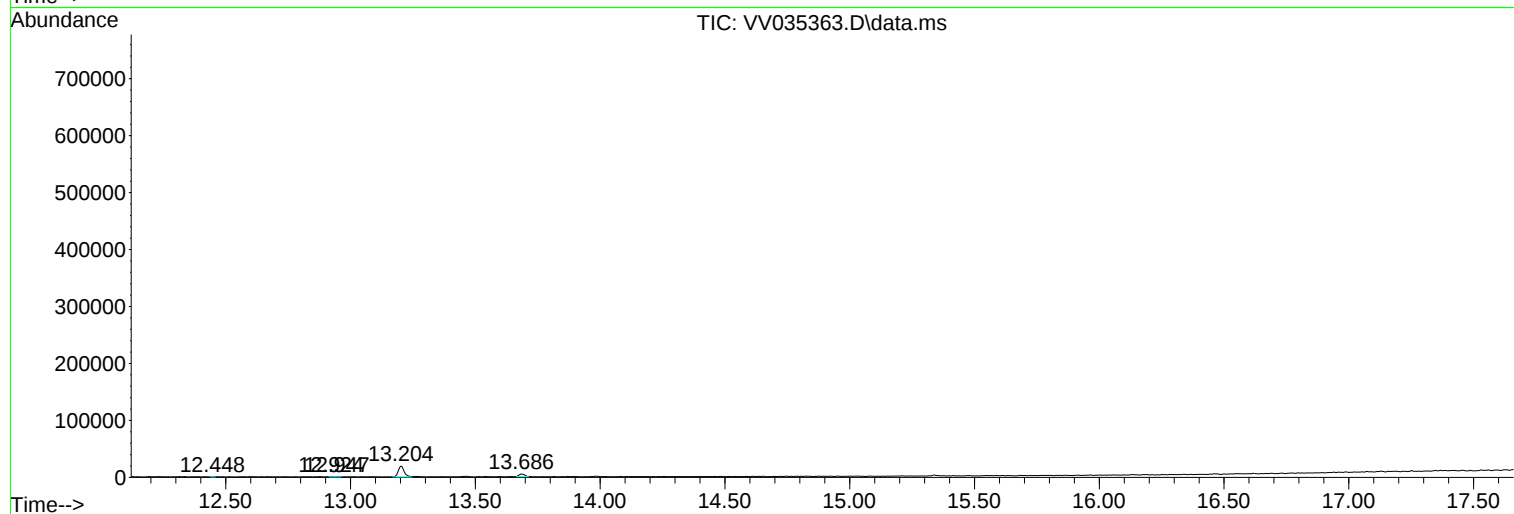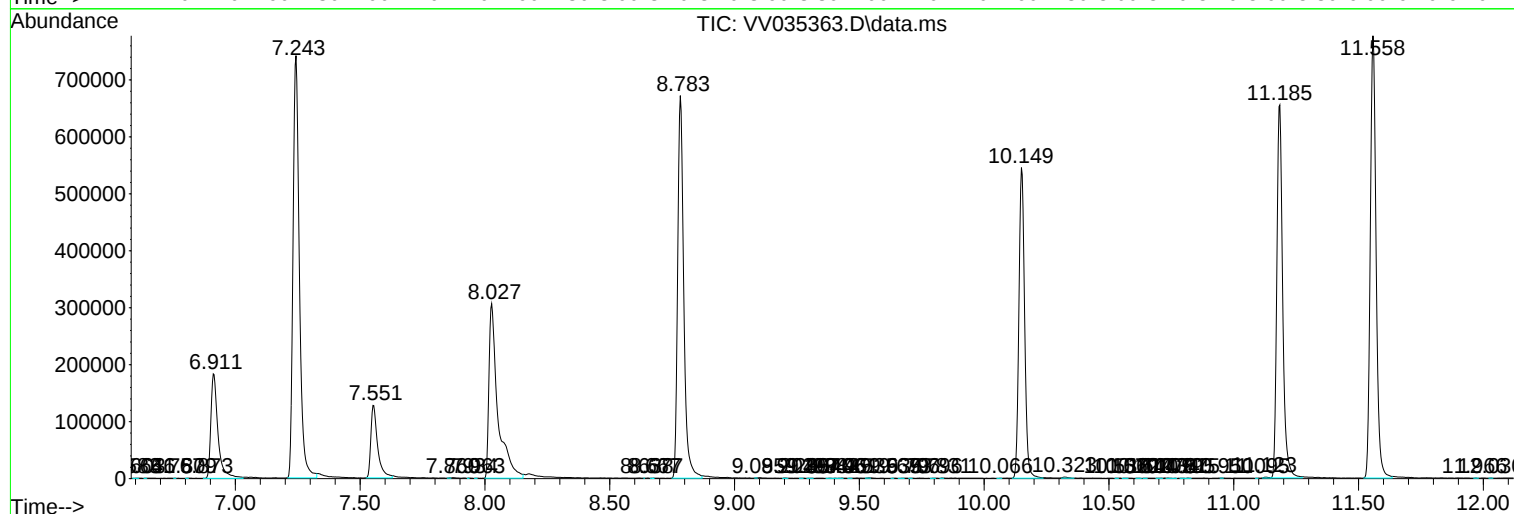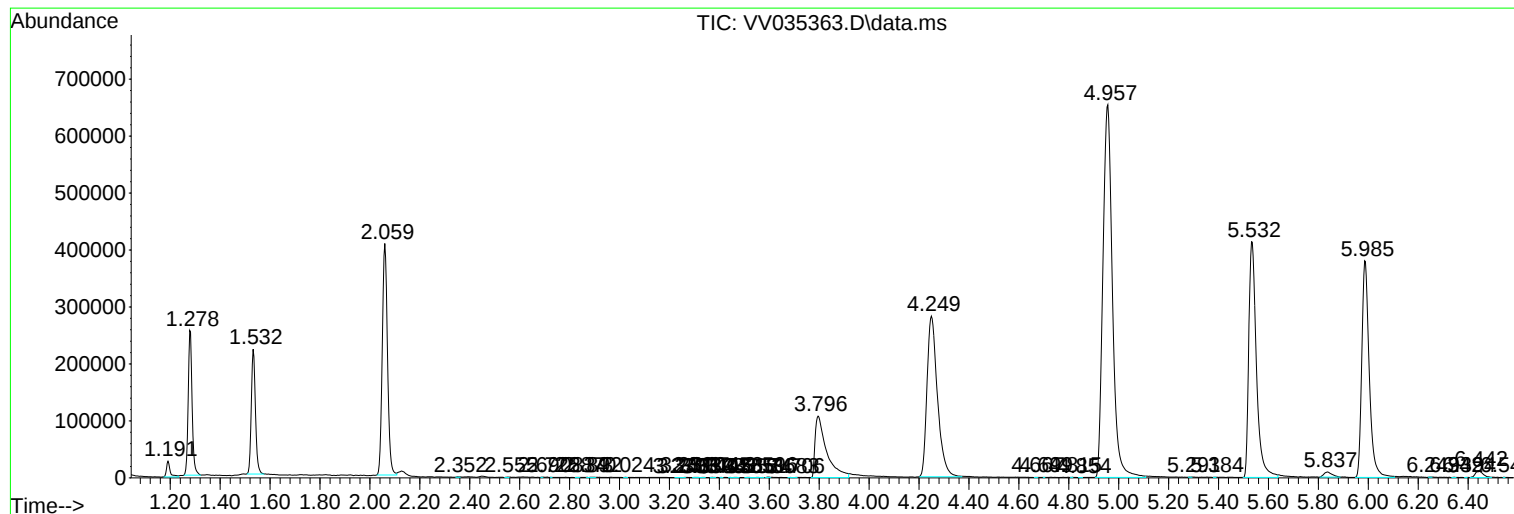

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035363.D
Acq On : 23 Apr 2024 15:57
Operator : SY/MD
Sample : P2235-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0810

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035363.D
Acq On : 23 Apr 2024 15:57
Operator : SY/MD
Sample : P2235-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0810

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------