

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035365.D
 Acq On : 23 Apr 2024 17:06
 Operator : SY/MD
 Sample : P2182-10 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035365.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	245118	263072	6.31%	1.312%
2	1.532	146	153	170	rVB	214640	252400	6.06%	1.259%
3	2.059	307	317	333	rBV	390763	563170	13.52%	2.808%
4	2.558	464	472	475	rBV5	1057	1581	0.04%	0.008%
5	2.629	491	494	496	rBV2	388	243	0.01%	0.001%
6	2.767	534	537	538	rBV	190	85	0.00%	0.000%
7	2.947	590	593	596	rBV2	298	245	0.01%	0.001%
8	2.973	600	601	605	rBV3	341	223	0.01%	0.001%
9	3.043	619	623	626	rBV	207	168	0.00%	0.001%
10	3.108	640	643	645	rBV2	334	137	0.00%	0.001%
11	3.162	657	660	663	rBV2	211	156	0.00%	0.001%
12	3.182	663	666	669	rVB	206	115	0.00%	0.001%
13	3.272	690	694	698	rBV	255	221	0.01%	0.001%
14	3.323	704	710	712	rBV2	220	232	0.01%	0.001%
15	3.358	718	721	724	rBV3	322	166	0.00%	0.001%
16	3.375	724	726	728	rBV	152	86	0.00%	0.000%
17	3.407	733	736	739	rBV2	227	179	0.00%	0.001%
18	3.506	763	767	771	rBV2	225	195	0.00%	0.001%
19	3.593	791	794	799	rBV2	333	261	0.01%	0.001%
20	3.641	805	809	812	rBV3	241	168	0.00%	0.001%
21	3.664	812	816	818	rBV3	456	377	0.01%	0.002%
22	3.680	820	821	823	rBV2	250	110	0.00%	0.001%
23	3.741	837	840	842	rBV	290	146	0.00%	0.001%
24	3.796	847	857	902	rBV	107063	364013	8.74%	1.815%
25	4.249	983	998	1031	rBV	264484	681515	16.36%	3.399%
26	4.709	1137	1141	1142	rBV2	362	200	0.00%	0.001%
27	4.731	1146	1148	1150	rBV	356	131	0.00%	0.001%
28	4.796	1166	1168	1169	rBV	301	105	0.00%	0.001%
29	4.841	1180	1182	1185	rBV2	311	135	0.00%	0.001%
30	4.860	1186	1188	1192	rVB	353	217	0.01%	0.001%
31	4.886	1192	1196	1199	rBV2	180	180	0.00%	0.001%
32	4.902	1199	1201	1202	rBV2	291	133	0.00%	0.001%
33	4.953	1202	1217	1267	rBV2	636899	1815924	43.59%	9.056%
34	5.326	1331	1333	1337	rBV3	348	229	0.01%	0.001%
35	5.426	1362	1364	1368	rVB3	482	230	0.01%	0.001%
36	5.445	1368	1370	1371	rBV	270	104	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035365.D
Acq On : 23 Apr 2024 17:06
Operator : SY/MD
Sample : P2182-10 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCD07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis

37	5.474	1377	1379	1380	rBV2	212	94	0.00%	0.000%
38	5.532	1386	1397	1436	rBV	400638	854669	20.51%	4.262%
39	5.841	1482	1493	1513	rVB3	6591	15620	0.37%	0.078%
40	5.985	1526	1538	1578	rBV	366857	775292	18.61%	3.866%
41	6.358	1652	1654	1657	rBV	226	117	0.00%	0.001%
42	6.461	1683	1686	1688	rVB	351	161	0.00%	0.001%
43	6.477	1688	1691	1693	rBV2	237	152	0.00%	0.001%
44	6.503	1697	1699	1704	rVB2	316	258	0.01%	0.001%
45	6.532	1704	1708	1710	rBV2	148	118	0.00%	0.001%
46	6.561	1715	1717	1718	rBV	184	85	0.00%	0.000%
47	6.596	1724	1728	1730	rBV	108	89	0.00%	0.000%
48	6.641	1739	1742	1745	rBV2	261	205	0.00%	0.001%
49	6.680	1753	1754	1756	rBV	281	146	0.00%	0.001%
50	6.767	1778	1781	1783	rBV2	239	131	0.00%	0.001%
51	6.812	1791	1795	1797	rVB	152	111	0.00%	0.001%
52	6.850	1803	1807	1812	rVB	260	204	0.00%	0.001%
53	6.911	1816	1826	1859	rBV	174385	342673	8.22%	1.709%
54	7.156	1898	1902	1904	rBV3	709	618	0.01%	0.003%
55	7.243	1917	1929	1965	rBV	704143	1251993	30.05%	6.243%
56	7.554	2017	2026	2054	rBV	125228	232368	5.58%	1.159%
57	7.818	2106	2108	2111	rBV2	331	227	0.01%	0.001%
58	7.911	2135	2137	2140	rVB2	535	248	0.01%	0.001%
59	7.931	2140	2143	2145	rBV2	284	178	0.00%	0.001%
60	7.943	2145	2147	2148	rBV2	353	138	0.00%	0.001%
61	8.027	2163	2173	2216	rBV2	303777	737672	17.71%	3.679%
62	8.442	2300	2302	2303	rBV	333	124	0.00%	0.001%
63	8.487	2312	2316	2320	rVB3	758	646	0.02%	0.003%
64	8.506	2320	2322	2326	rBV	368	336	0.01%	0.002%
65	8.808	2397	2416	2459	rBV2	1907112	4166312	100.00%	20.777%
66	9.378	2590	2593	2596	rBV2	477	324	0.01%	0.002%
67	9.429	2607	2609	2612	rBV3	296	167	0.00%	0.001%
68	9.471	2620	2622	2629	rVB2	332	265	0.01%	0.001%
69	9.503	2629	2632	2634	rBV	410	252	0.01%	0.001%
70	9.535	2638	2642	2644	rBV2	294	205	0.00%	0.001%
71	9.596	2659	2661	2663	rBV	273	139	0.00%	0.001%
72	9.654	2677	2679	2682	rBV	291	213	0.01%	0.001%
73	9.812	2725	2728	2730	rBV2	178	115	0.00%	0.001%
74	9.863	2741	2744	2747	rBV2	284	226	0.01%	0.001%
75	9.918	2758	2761	2766	rVB2	392	275	0.01%	0.001%
76	9.947	2766	2770	2773	rBV2	374	346	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035365.D
 Acq On : 23 Apr 2024 17:06
 Operator : SY/MD
 Sample : P2182-10 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.069	2805	2808	2811	rVB3	266	196	0.00%	0.001%
78	10.101	2815	2818	2821	rBV2	283	216	0.01%	0.001%
79	10.149	2821	2833	2859	rBV	553473	863892	20.74%	4.308%
80	10.506	2941	2944	2945	rBV	198	95	0.00%	0.000%
81	10.596	2970	2972	2979	rVB2	233	170	0.00%	0.001%
82	10.654	2986	2990	2992	rBV	340	312	0.01%	0.002%
83	10.744	3014	3018	3022	rBV2	378	274	0.01%	0.001%
84	10.783	3028	3030	3036	rVB3	589	456	0.01%	0.002%
85	10.863	3049	3055	3056	rBV2	322	300	0.01%	0.001%
86	11.033	3105	3108	3111	rBV2	344	243	0.01%	0.001%
87	11.072	3118	3120	3123	rVB	224	93	0.00%	0.000%
88	11.117	3123	3134	3145	rBV	140431	221507	5.32%	1.105%
89	11.204	3145	3161	3185	rVB2	973964	2433280	58.40%	12.134%
90	11.574	3259	3276	3302	rBV2	1728706	3624444	86.99%	18.074%
91	11.947	3388	3392	3393	rBV	520	348	0.01%	0.002%
92	11.992	3403	3406	3408	rBV	418	228	0.01%	0.001%
93	12.056	3424	3426	3429	rVB2	347	172	0.00%	0.001%
94	12.075	3429	3432	3434	rBV	308	165	0.00%	0.001%
95	12.326	3508	3510	3513	rBV3	325	188	0.00%	0.001%
96	12.500	3560	3564	3566	rBV2	460	432	0.01%	0.002%
97	12.583	3588	3590	3591	rBV	372	151	0.00%	0.001%
98	13.146	3762	3765	3767	rBV	335	217	0.01%	0.001%
99	13.194	3769	3780	3801	rBV	272168	442763	10.63%	2.208%
100	13.680	3921	3931	3949	rBV3	80902	132403	3.18%	0.660%




Sum of corrected areas: 20052909

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035365.D
Acq On : 23 Apr 2024 17:06
Operator : SY/MD
Sample : P2182-10 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

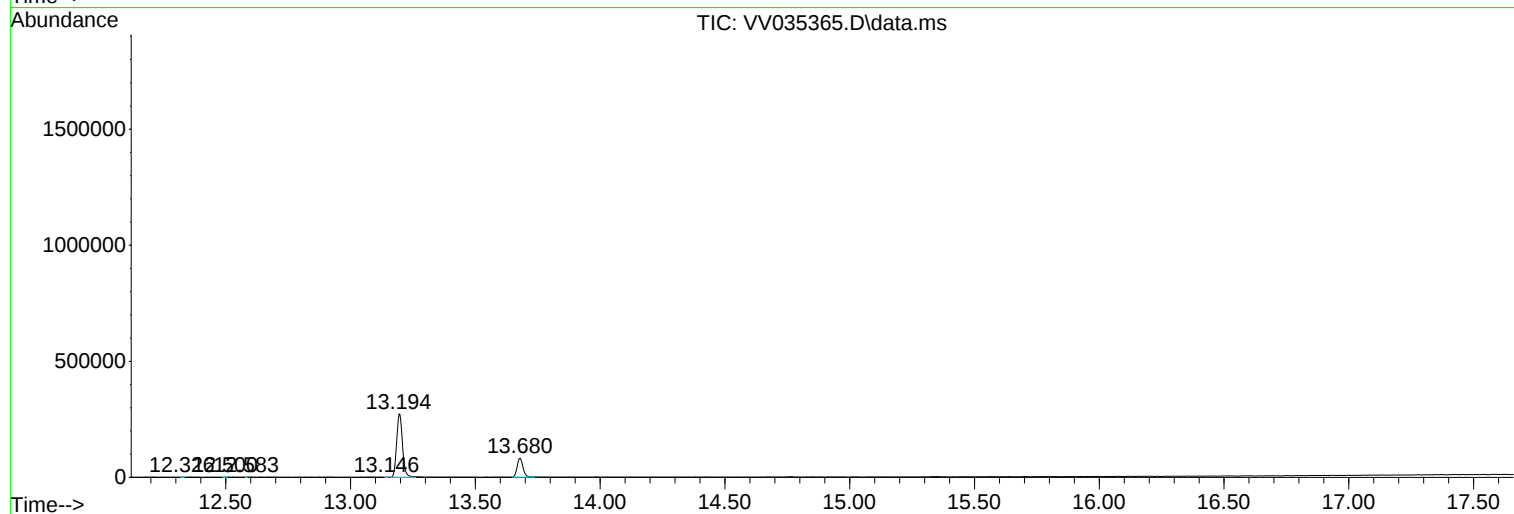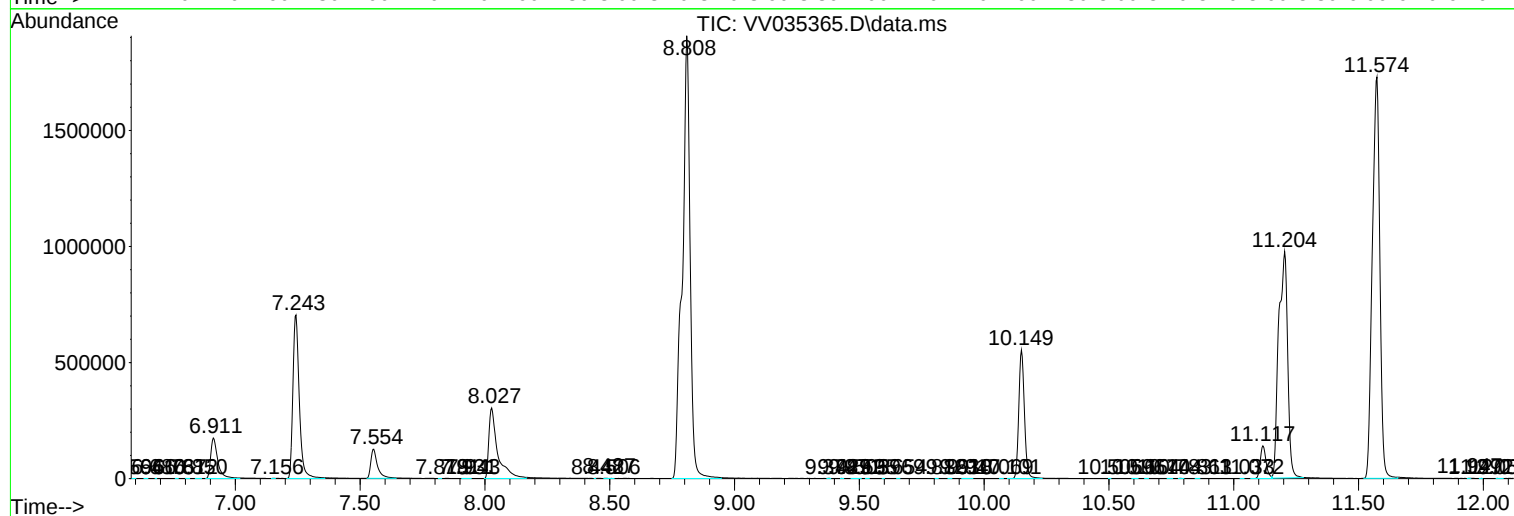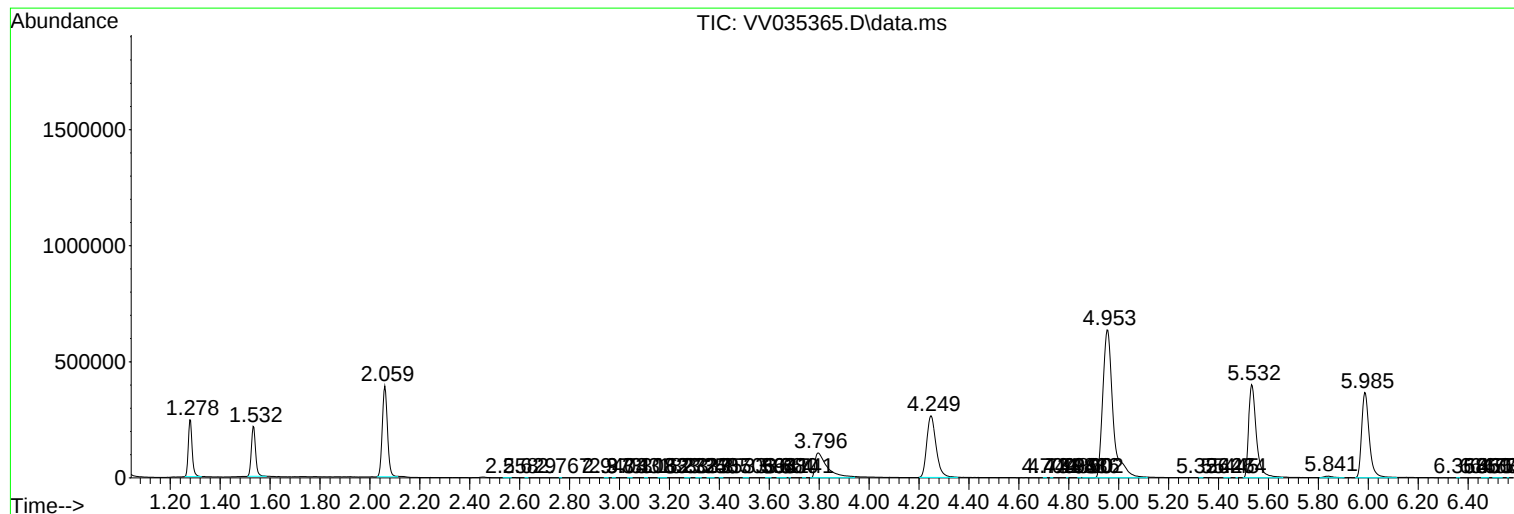

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035365.D
Acq On : 23 Apr 2024 17:06
Operator : SY/MD
Sample : P2182-10 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035365.D
Acq On : 23 Apr 2024 17:06
Operator : SY/MD
Sample : P2182-10 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------