

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035367.D
 Acq On : 23 Apr 2024 17:52
 Operator : SY/MD
 Sample : P2182-02 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035367.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	57	rBV4	1517	1607	0.04%	0.009%
2	1.278	67	74	89	rBV	254000	269067	5.93%	1.553%
3	1.532	146	153	168	rVB	219803	252837	5.57%	1.459%
4	2.060	307	317	334	rBV	400378	583071	12.84%	3.365%
5	2.330	398	401	405	rVB4	757	527	0.01%	0.003%
6	2.352	406	408	412	rVB3	441	255	0.01%	0.001%
7	2.375	412	415	419	rBV3	414	275	0.01%	0.002%
8	2.397	419	422	430	rBV4	593	578	0.01%	0.003%
9	2.449	430	438	448	rBV2	2620	4388	0.10%	0.025%
10	2.555	467	471	473	rBV2	365	317	0.01%	0.002%
11	2.568	473	475	480	rVB3	789	590	0.01%	0.003%
12	2.648	498	500	506	rVB3	318	287	0.01%	0.002%
13	2.712	515	520	523	rVB3	392	248	0.01%	0.001%
14	2.851	559	563	568	rBV3	449	473	0.01%	0.003%
15	2.892	573	576	585	rVB2	292	308	0.01%	0.002%
16	2.950	591	594	599	rBV	369	352	0.01%	0.002%
17	2.973	599	601	605	rBV3	228	210	0.00%	0.001%
18	3.198	668	671	676	rBV2	283	269	0.01%	0.002%
19	3.243	682	685	689	rVB	285	202	0.00%	0.001%
20	3.381	721	728	729	rBV	256	241	0.01%	0.001%
21	3.519	768	771	773	rBV3	398	252	0.01%	0.001%
22	3.796	848	857	903	rBV	112312	367901	8.10%	2.123%
23	4.246	981	997	1040	rBV	274874	718925	15.84%	4.149%
24	4.645	1115	1121	1123	rBV4	413	388	0.01%	0.002%
25	4.953	1202	1217	1227	rBV2	669757	1717368	37.83%	9.910%
26	5.400	1353	1356	1360	rBV4	443	410	0.01%	0.002%
27	5.532	1386	1397	1432	rBV	430999	906260	19.96%	5.230%
28	5.735	1458	1460	1463	rBV2	394	245	0.01%	0.001%
29	5.841	1481	1493	1506	rBV5	7553	17922	0.39%	0.103%
30	5.985	1525	1538	1572	rBV	377810	798136	17.58%	4.606%
31	6.587	1719	1725	1727	rBV2	313	355	0.01%	0.002%
32	6.600	1727	1729	1735	rVB2	327	316	0.01%	0.002%
33	6.674	1748	1752	1755	rBV2	407	358	0.01%	0.002%
34	6.770	1776	1782	1787	rVB4	482	620	0.01%	0.004%
35	6.911	1816	1826	1854	rBV	182907	355083	7.82%	2.049%
36	7.140	1893	1897	1899	rBV3	535	406	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042324\
 Data File : VW035367.D
 Acq On : 23 Apr 2024 17:52
 Operator : SY/MD
 Sample : P2182-02 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	7.243	1917	1929	1953	rBV	737382	1308929	28.83%	7.553%
38	7.551	2016	2025	2058	rBV	126066	243986	5.37%	1.408%
39	7.892	2129	2131	2138	rBV3	322	346	0.01%	0.002%
40	7.921	2138	2140	2143	rVB	521	260	0.01%	0.002%
41	7.985	2158	2160	2164	rBV	595	281	0.01%	0.002%
42	8.027	2164	2173	2221	rBV2	317550	780801	17.20%	4.506%
43	8.333	2264	2268	2271	rBV5	360	333	0.01%	0.002%
44	8.567	2340	2341	2347	rVB3	916	655	0.01%	0.004%
45	8.606	2350	2353	2354	rBV2	651	303	0.01%	0.002%
46	8.683	2374	2377	2383	rBV5	364	316	0.01%	0.002%
47	8.728	2387	2391	2395	rBV2	396	323	0.01%	0.002%
48	8.809	2395	2416	2464	rBV2	2089222	4539610	100.00%	26.197%
49	9.146	2518	2521	2524	rBV2	509	374	0.01%	0.002%
50	9.365	2585	2589	2596	rBV4	627	871	0.02%	0.005%
51	9.423	2604	2607	2612	rVB3	425	406	0.01%	0.002%
52	9.603	2661	2663	2670	rVB3	353	328	0.01%	0.002%
53	9.786	2714	2720	2725	rVB3	358	474	0.01%	0.003%
54	9.815	2725	2729	2734	rBV	601	502	0.01%	0.003%
55	9.853	2738	2741	2742	rBV3	334	208	0.00%	0.001%
56	9.998	2784	2786	2791	rVB2	359	206	0.00%	0.001%
57	10.149	2817	2833	2855	rBV	570758	890674	19.62%	5.140%
58	10.316	2883	2885	2887	rBV2	443	220	0.00%	0.001%
59	10.571	2958	2964	2967	rBV2	222	235	0.01%	0.001%
60	10.632	2978	2983	2986	rBV2	303	352	0.01%	0.002%
61	10.722	3008	3011	3015	rBV2	287	214	0.00%	0.001%
62	10.751	3016	3020	3028	rVB4	346	417	0.01%	0.002%
63	10.789	3029	3032	3037	rVB3	402	280	0.01%	0.002%
64	10.828	3039	3044	3048	rBV2	338	313	0.01%	0.002%
65	10.863	3053	3055	3058	rVV2	313	226	0.00%	0.001%
66	10.892	3062	3064	3069	rVB2	449	292	0.01%	0.002%
67	11.075	3118	3121	3125	rVB2	344	228	0.01%	0.001%
68	11.120	3126	3135	3144	rBV2	28431	45159	0.99%	0.261%
69	11.185	3144	3155	3158	rBV	764105	1096273	24.15%	6.326%
70	11.448	3235	3237	3241	rVB2	399	216	0.00%	0.001%
71	11.468	3241	3243	3249	rVB5	407	345	0.01%	0.002%
72	11.561	3258	3272	3303	rBV2	1007968	2346071	51.68%	13.539%
73	11.796	3341	3345	3347	rBV3	497	304	0.01%	0.002%
74	11.924	3382	3385	3388	rBV3	326	246	0.01%	0.001%
75	11.943	3388	3391	3394	rVV3	385	250	0.01%	0.001%
76	12.149	3450	3455	3460	rBV4	472	516	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035367.D
 Acq On : 23 Apr 2024 17:52
 Operator : SY/MD
 Sample : P2182-02 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	12.278	3492	3495	3501	rVB3	341	327	0.01%	0.002%
78	12.635	3603	3606	3613	rBV3	480	549	0.01%	0.003%
79	12.731	3634	3636	3640	rBV2	263	203	0.00%	0.001%
80	12.783	3647	3652	3658	rBV3	362	521	0.01%	0.003%
81	12.866	3670	3678	3681	rBV3	550	531	0.01%	0.003%
82	12.953	3702	3705	3708	rBV2	366	259	0.01%	0.001%
83	13.046	3731	3734	3738	rBV2	348	297	0.01%	0.002%
84	13.075	3739	3743	3747	rVV3	400	440	0.01%	0.003%
85	13.111	3752	3754	3757	rBV	281	222	0.00%	0.001%
86	13.201	3772	3782	3796	rBV	28577	47621	1.05%	0.275%
87	13.352	3826	3829	3832	rVB3	369	212	0.00%	0.001%
88	13.628	3912	3915	3917	rBV	360	214	0.00%	0.001%
89	13.686	3924	3933	3946	rVB3	6243	9925	0.22%	0.057%
90	13.783	3959	3963	3965	rBV3	443	302	0.01%	0.002%
91	13.857	3984	3986	3991	rVB2	805	635	0.01%	0.004%
92	13.879	3991	3993	3995	rBV	597	382	0.01%	0.002%
93	13.953	4014	4016	4018	rVV2	409	217	0.00%	0.001%
94	14.033	4039	4041	4045	rBV	367	232	0.01%	0.001%
95	14.316	4127	4129	4136	rVB3	566	445	0.01%	0.003%
96	14.548	4199	4201	4207	rVB4	601	417	0.01%	0.002%
97	14.577	4207	4210	4212	rBV2	486	280	0.01%	0.002%
98	14.728	4254	4257	4259	rBV2	706	453	0.01%	0.003%
99	14.853	4294	4296	4300	rVB2	831	452	0.01%	0.003%
100	14.876	4301	4303	4307	rVV3	470	326	0.01%	0.002%


Sum of corrected areas: 17328852

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035367.D
Acq On : 23 Apr 2024 17:52
Operator : SY/MD
Sample : P2182-02 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

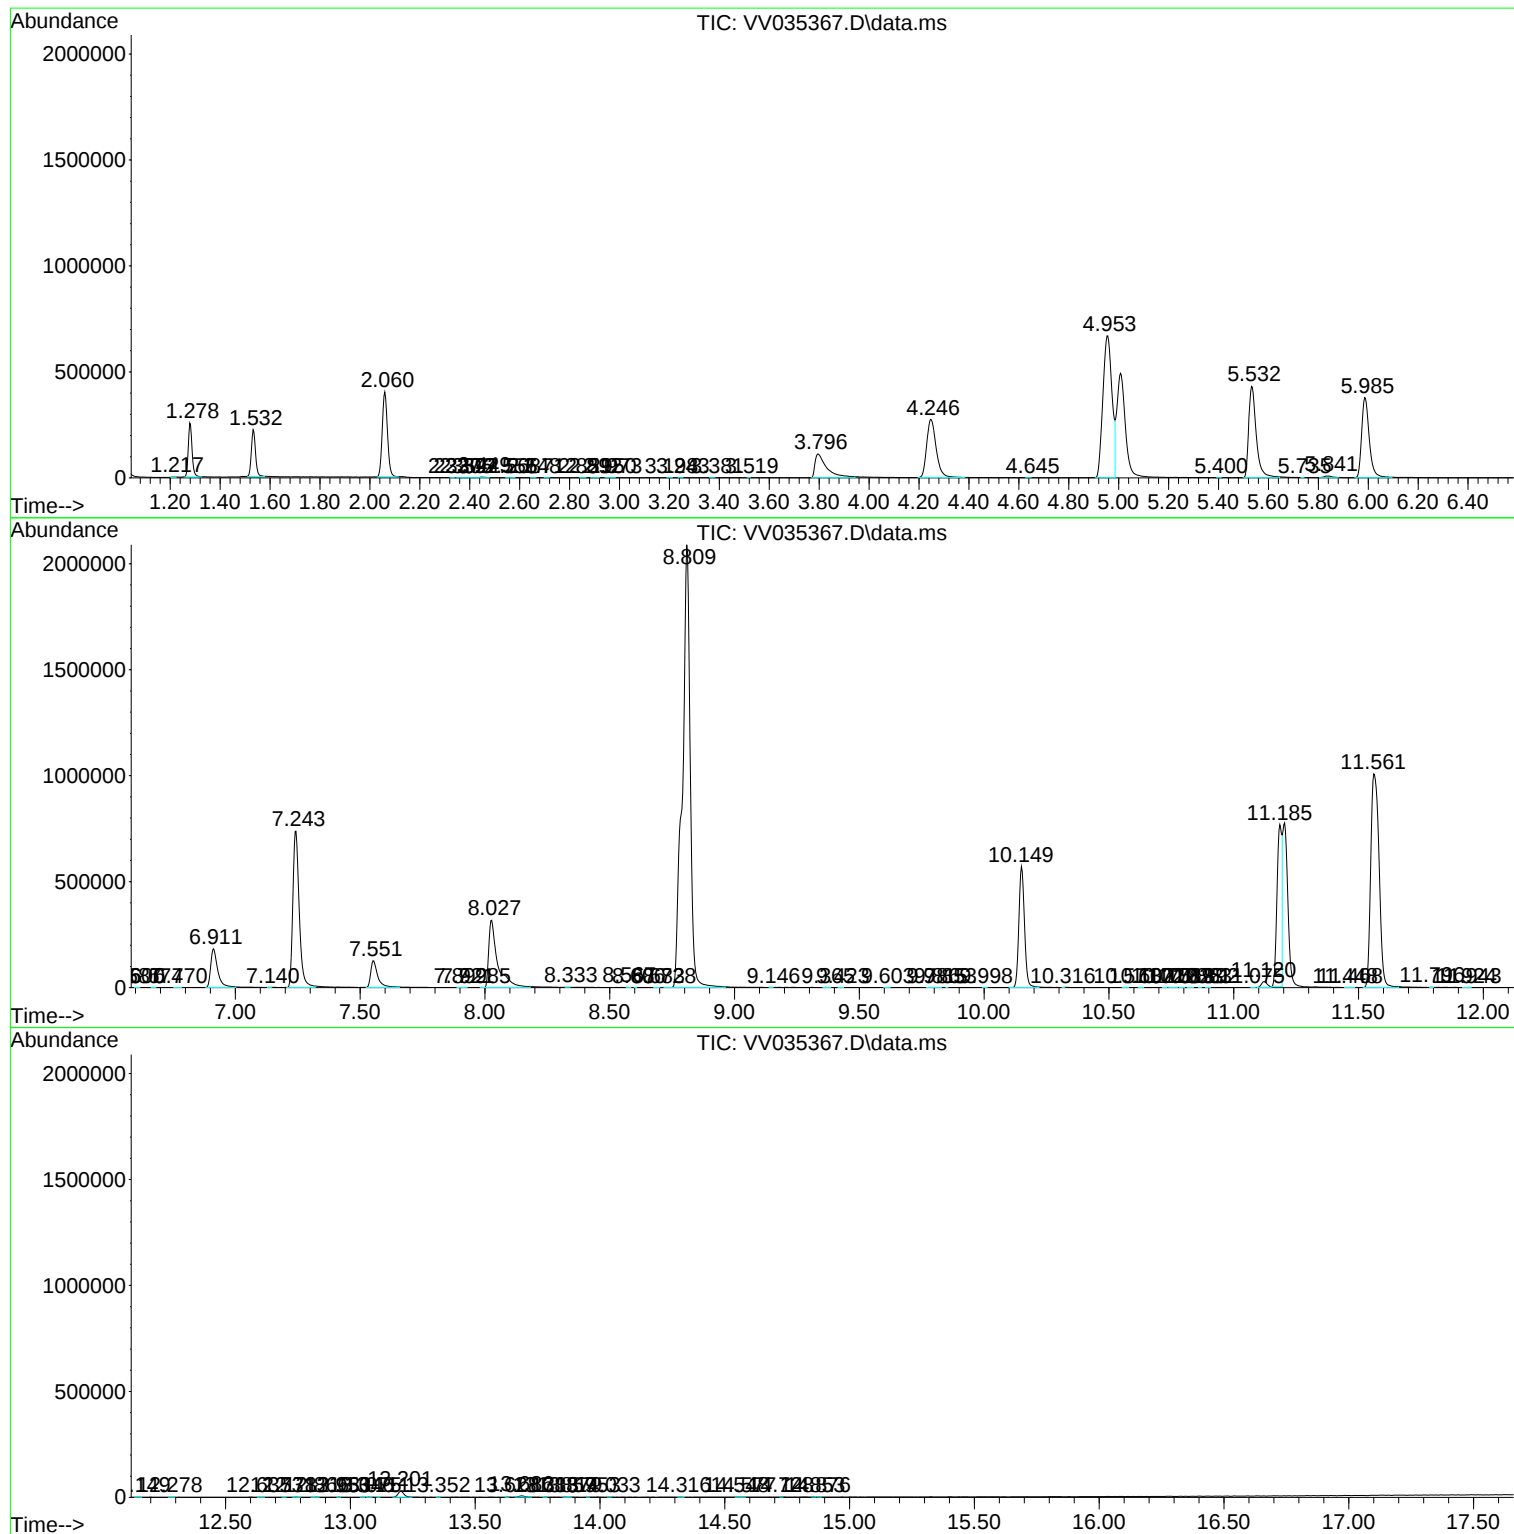

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035367.D
Acq On : 23 Apr 2024 17:52
Operator : SY/MD
Sample : P2182-02 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035367.D
Acq On : 23 Apr 2024 17:52
Operator : SY/MD
Sample : P2182-02 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------