

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035368.D
 Acq On : 23 Apr 2024 18:15
 Operator : SY/MD
 Sample : P2158-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035368.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	250026	265700	15.52%	2.096%
2	1.532	146	153	164	rBV	216080	250045	14.61%	1.973%
3	2.060	307	317	332	rBV	402289	582370	34.02%	4.594%
4	2.773	536	539	541	rBV2	347	167	0.01%	0.001%
5	2.924	582	586	589	rVB2	266	179	0.01%	0.001%
6	2.941	589	591	594	rBV2	369	142	0.01%	0.001%
7	2.953	594	595	598	rBV	312	166	0.01%	0.001%
8	2.998	605	609	612	rBV2	236	203	0.01%	0.002%
9	3.034	616	620	623	rBV2	223	197	0.01%	0.002%
10	3.105	639	642	644	rBV2	195	129	0.01%	0.001%
11	3.117	644	646	647	rBV	241	100	0.01%	0.001%
12	3.243	682	685	689	rVB3	260	219	0.01%	0.002%
13	3.326	707	711	712	rBV	222	123	0.01%	0.001%
14	3.355	717	720	722	rVV	340	213	0.01%	0.002%
15	3.391	726	731	737	rBV2	327	389	0.02%	0.003%
16	3.416	737	739	742	rVB3	252	160	0.01%	0.001%
17	3.439	742	746	747	rBV2	210	125	0.01%	0.001%
18	3.481	757	759	762	rBV	216	89	0.01%	0.001%
19	3.526	772	773	777	rVB	323	168	0.01%	0.001%
20	3.548	777	780	785	rBV2	340	365	0.02%	0.003%
21	3.632	802	806	810	rVB	310	214	0.01%	0.002%
22	3.658	810	814	816	rBV	162	121	0.01%	0.001%
23	3.670	816	818	820	rVB2	228	106	0.01%	0.001%
24	3.687	820	823	827	rVB2	288	192	0.01%	0.002%
25	3.712	827	831	834	rBV2	160	117	0.01%	0.001%
26	3.735	834	838	841	rBV2	173	107	0.01%	0.001%
27	3.751	841	843	845	rBV	130	82	0.00%	0.001%
28	3.796	848	857	902	rBV	101963	338772	19.79%	2.672%
29	4.249	982	998	1038	rBV	270056	726408	42.43%	5.730%
30	4.902	1198	1201	1202	rBV2	286	158	0.01%	0.001%
31	4.953	1202	1217	1254	rBV2	646923	1711931	100.00%	13.505%
32	5.445	1366	1370	1373	rBV2	408	345	0.02%	0.003%
33	5.465	1373	1376	1381	rVB2	278	218	0.01%	0.002%
34	5.532	1386	1397	1433	rBV	434993	917607	53.60%	7.239%
35	5.838	1482	1492	1506	rBV3	8763	19207	1.12%	0.152%
36	5.985	1526	1538	1566	rBV	372068	774602	45.25%	6.111%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035368.D
 Acq On : 23 Apr 2024 18:15
 Operator : SY/MD
 Sample : P2158-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.310	1637	1639	1642	rVB2	447	171	0.01%	0.001%
38	6.384	1660	1662	1663	rBV	298	158	0.01%	0.001%
39	6.426	1672	1675	1676	rBV	706	365	0.02%	0.003%
40	6.519	1700	1704	1709	rVB3	334	252	0.01%	0.002%
41	6.545	1709	1712	1714	rBV2	283	166	0.01%	0.001%
42	6.564	1714	1718	1722	rVB2	232	179	0.01%	0.001%
43	6.590	1722	1726	1728	rVB	316	180	0.01%	0.001%
44	6.609	1728	1732	1735	rBV2	247	240	0.01%	0.002%
45	6.651	1743	1745	1748	rBV2	338	172	0.01%	0.001%
46	6.690	1755	1757	1759	rBV2	294	193	0.01%	0.002%
47	6.741	1771	1773	1775	rVB2	415	163	0.01%	0.001%
48	6.754	1775	1777	1783	rBV3	219	152	0.01%	0.001%
49	6.812	1789	1795	1796	rBV2	135	112	0.01%	0.001%
50	6.828	1796	1800	1802	rBV2	112	89	0.01%	0.001%
51	6.911	1816	1826	1854	rBV	180183	350111	20.45%	2.762%
52	7.243	1918	1929	1966	rBV	731306	1296100	75.71%	10.224%
53	7.551	2016	2025	2057	rBV	123811	238045	13.91%	1.878%
54	7.908	2134	2136	2137	rBV2	517	238	0.01%	0.002%
55	7.956	2147	2151	2154	rBV2	288	224	0.01%	0.002%
56	8.027	2163	2173	2218	rBV3	289601	737220	43.06%	5.816%
57	8.619	2355	2357	2358	rBV	415	163	0.01%	0.001%
58	8.664	2366	2371	2376	rBV2	304	386	0.02%	0.003%
59	8.783	2397	2408	2443	rBV	701113	1196414	69.89%	9.438%
60	9.172	2527	2529	2531	rVB2	416	168	0.01%	0.001%
61	9.185	2531	2533	2534	rBV2	315	139	0.01%	0.001%
62	9.204	2537	2539	2542	rVV2	344	235	0.01%	0.002%
63	9.220	2542	2544	2548	rVB3	469	298	0.02%	0.002%
64	9.246	2548	2552	2559	rBV5	527	536	0.03%	0.004%
65	9.275	2559	2561	2569	rVV3	325	397	0.02%	0.003%
66	9.307	2569	2571	2576	rVV2	331	207	0.01%	0.002%
67	9.342	2579	2582	2585	rBV3	220	147	0.01%	0.001%
68	9.471	2620	2622	2624	rBV2	146	82	0.00%	0.001%
69	9.519	2634	2637	2640	rBV2	381	195	0.01%	0.002%
70	9.567	2648	2652	2653	rBV	307	201	0.01%	0.002%
71	9.709	2693	2696	2698	rBV	154	103	0.01%	0.001%
72	9.744	2705	2707	2711	rBV2	299	202	0.01%	0.002%
73	9.812	2724	2728	2732	rBV	265	211	0.01%	0.002%
74	9.873	2745	2747	2750	rBV2	319	202	0.01%	0.002%
75	9.937	2765	2767	2770	rBV2	129	83	0.00%	0.001%
76	9.956	2770	2773	2774	rBV	224	110	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035368.D
 Acq On : 23 Apr 2024 18:15
 Operator : SY/MD
 Sample : P2158-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.101	2812	2818	2822	rBV3	571	505	0.03%	0.004%
78	10.149	2822	2833	2861	rBV	537491	856213	50.01%	6.754%
79	10.304	2879	2881	2882	rBV	370	156	0.01%	0.001%
80	10.349	2893	2895	2897	rBV	231	133	0.01%	0.001%
81	10.361	2897	2899	2904	rVV3	420	301	0.02%	0.002%
82	10.387	2904	2907	2914	rVB3	436	512	0.03%	0.004%
83	10.503	2940	2943	2946	rBV2	282	148	0.01%	0.001%
84	10.599	2970	2973	2976	rBV	275	169	0.01%	0.001%
85	10.654	2987	2990	2993	rBV2	264	201	0.01%	0.002%
86	10.770	3024	3026	3027	rBV	195	90	0.01%	0.001%
87	10.802	3034	3036	3041	rBV	306	179	0.01%	0.001%
88	10.956	3081	3084	3087	rBV	290	150	0.01%	0.001%
89	11.133	3130	3139	3144	rBV6	2277	3086	0.18%	0.024%
90	11.185	3144	3155	3183	rVV	667972	1109452	64.81%	8.752%
91	11.558	3259	3271	3293	rBV	777032	1258890	73.54%	9.931%
92	11.847	3358	3361	3363	rBV3	640	375	0.02%	0.003%
93	12.040	3419	3421	3422	rBV3	303	107	0.01%	0.001%
94	12.104	3435	3441	3446	rBV3	410	466	0.03%	0.004%
95	12.374	3522	3525	3527	rBV	417	257	0.02%	0.002%
96	12.725	3632	3634	3638	rBV2	290	126	0.01%	0.001%
97	13.011	3717	3723	3725	rBV2	463	484	0.03%	0.004%
98	13.104	3749	3752	3755	rBV2	352	280	0.02%	0.002%
99	13.204	3774	3783	3795	rBV2	12004	21209	1.24%	0.167%
100	13.686	3926	3933	3945	rVB5	4120	6601	0.39%	0.052%




Sum of corrected areas: 12676535

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035368.D
Acq On : 23 Apr 2024 18:15
Operator : SY/MD
Sample : P2158-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

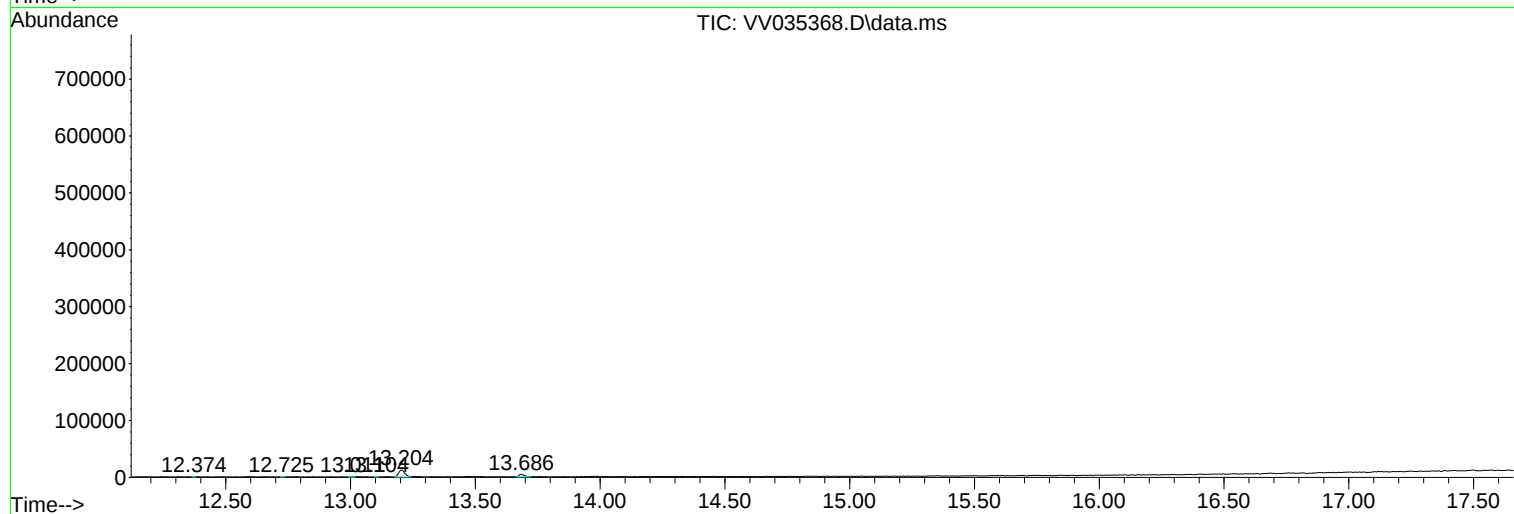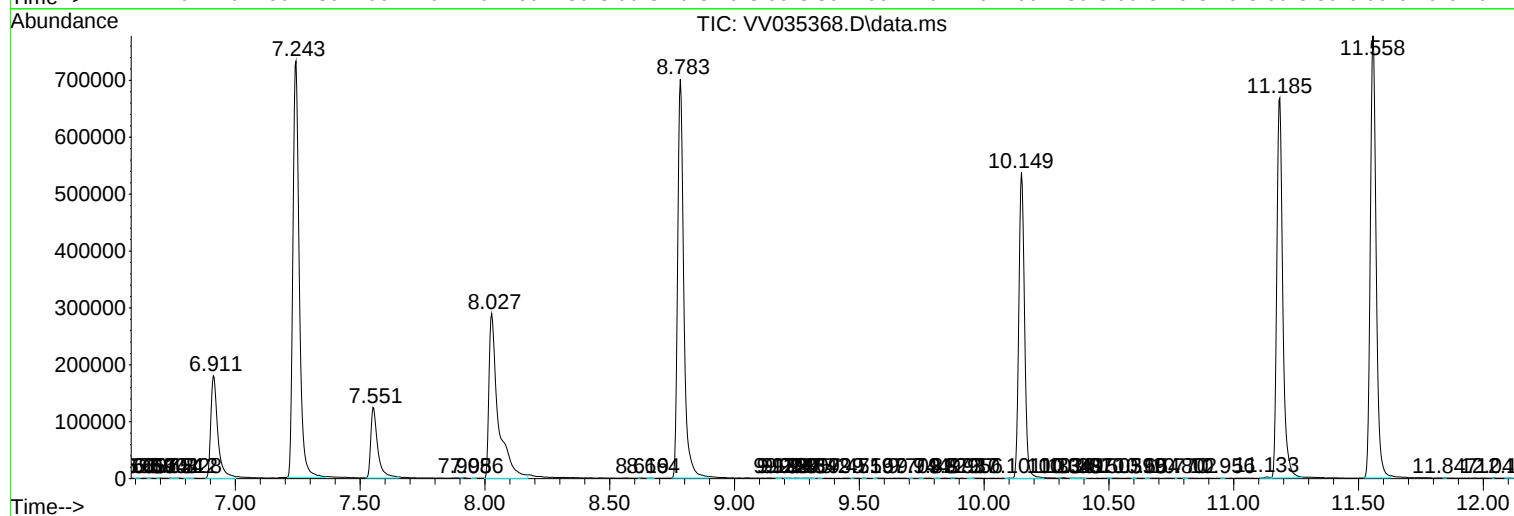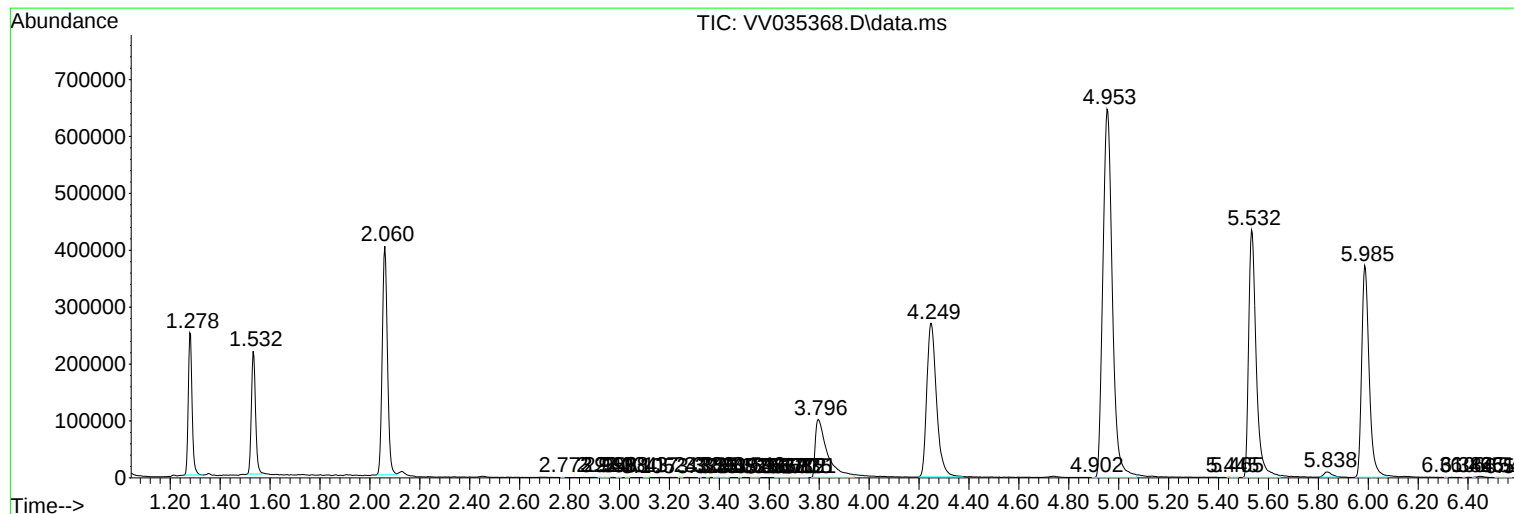

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035368.D
Acq On : 23 Apr 2024 18:15
Operator : SY/MD
Sample : P2158-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035368.D
Acq On : 23 Apr 2024 18:15
Operator : SY/MD
Sample : P2158-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------