

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035369.D
 Acq On : 23 Apr 2024 18:38
 Operator : SY/MD
 Sample : P2158-04DL2 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD0DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035369.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	93	rVB	255153	273934	14.82%	1.983%
2	1.532	146	153	169	rBV	219017	257321	13.93%	1.863%
3	2.060	308	317	334	rVB	409011	588587	31.85%	4.261%
4	2.449	430	438	452	rVB2	14156	23468	1.27%	0.170%
5	2.606	484	487	488	rBV2	304	194	0.01%	0.001%
6	2.719	518	522	525	rBV	253	210	0.01%	0.002%
7	2.748	528	531	533	rBV2	222	137	0.01%	0.001%
8	2.796	541	546	549	rBV3	430	414	0.02%	0.003%
9	2.841	557	560	561	rBV2	158	84	0.00%	0.001%
10	2.851	561	563	567	rVB2	404	259	0.01%	0.002%
11	2.934	586	589	593	rBV2	361	267	0.01%	0.002%
12	2.986	600	605	607	rBV2	240	215	0.01%	0.002%
13	3.014	611	614	618	rBV	410	324	0.02%	0.002%
14	3.060	625	628	629	rBV2	242	164	0.01%	0.001%
15	3.101	636	641	644	rVB	472	384	0.02%	0.003%
16	3.124	644	648	650	rBV2	370	233	0.01%	0.002%
17	3.150	654	656	658	rBV	117	74	0.00%	0.001%
18	3.243	680	685	690	rVB3	262	240	0.01%	0.002%
19	3.307	702	705	708	rBV2	221	137	0.01%	0.001%
20	3.323	708	710	713	rBV2	212	158	0.01%	0.001%
21	3.442	745	747	749	rBV	129	82	0.00%	0.001%
22	3.484	758	760	764	rVB	249	126	0.01%	0.001%
23	3.510	764	768	770	rBV	183	128	0.01%	0.001%
24	3.568	782	786	789	rVB2	213	123	0.01%	0.001%
25	3.587	789	792	795	rBV3	286	210	0.01%	0.002%
26	3.661	808	815	816	rBV	396	231	0.01%	0.002%
27	3.674	816	819	822	rVV	263	180	0.01%	0.001%
28	3.690	822	824	826	rVV2	207	88	0.00%	0.001%
29	3.796	848	857	894	rBV	104929	344329	18.63%	2.493%
30	4.249	982	998	1030	rBV	272223	707330	38.28%	5.121%
31	4.805	1165	1171	1173	rBV	289	363	0.02%	0.003%
32	4.957	1202	1218	1225	rBV2	672832	1624816	87.93%	11.763%
33	5.532	1386	1397	1434	rBV	432153	919856	49.78%	6.659%
34	5.838	1483	1492	1510	rVB5	7337	16535	0.89%	0.120%
35	5.985	1525	1538	1572	rBV	375093	791182	42.82%	5.728%
36	6.294	1630	1634	1636	rBV3	445	266	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035369.D
 Acq On : 23 Apr 2024 18:38
 Operator : SY/MD
 Sample : P2158-04DL2 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD0DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.326	1642	1644	1649	rVB3	647	416	0.02%	0.003%
38	6.381	1657	1661	1663	rBV3	386	316	0.02%	0.002%
39	6.416	1668	1672	1674	rBV3	512	333	0.02%	0.002%
40	6.481	1689	1692	1695	rBV2	214	134	0.01%	0.001%
41	6.503	1695	1699	1704	rBV3	312	312	0.02%	0.002%
42	6.622	1735	1736	1739	rVB	244	97	0.01%	0.001%
43	6.641	1739	1742	1747	rBV2	559	494	0.03%	0.004%
44	6.661	1747	1748	1749	rVV2	342	96	0.01%	0.001%
45	6.683	1753	1755	1758	rVV2	229	118	0.01%	0.001%
46	6.709	1760	1763	1766	rVB2	199	145	0.01%	0.001%
47	6.725	1766	1768	1770	rBV	203	99	0.01%	0.001%
48	6.847	1802	1806	1810	rVB2	221	165	0.01%	0.001%
49	6.866	1810	1812	1816	rVB3	289	164	0.01%	0.001%
50	6.911	1816	1826	1861	rBV	179906	354223	19.17%	2.564%
51	7.243	1918	1929	1965	rBV	737781	1319942	71.43%	9.556%
52	7.551	2016	2025	2047	rBV	123946	234960	12.72%	1.701%
53	7.911	2135	2137	2141	rVB4	400	229	0.01%	0.002%
54	7.985	2157	2160	2163	rVB2	458	232	0.01%	0.002%
55	8.027	2163	2173	2228	rBV2	318354	771707	41.76%	5.587%
56	8.616	2354	2356	2359	rBV	334	239	0.01%	0.002%
57	8.680	2374	2376	2377	rBV	242	87	0.00%	0.001%
58	8.786	2397	2409	2410	rBV	786287	936538	50.68%	6.780%
59	9.114	2509	2511	2513	rBV2	471	210	0.01%	0.002%
60	9.345	2578	2583	2585	rBV4	401	364	0.02%	0.003%
61	9.439	2608	2612	2614	rBV	324	213	0.01%	0.002%
62	9.461	2615	2619	2621	rVV2	370	280	0.02%	0.002%
63	9.487	2625	2627	2628	rBV	283	93	0.01%	0.001%
64	9.503	2628	2632	2636	rBV2	472	354	0.02%	0.003%
65	9.606	2662	2664	2666	rBV2	283	135	0.01%	0.001%
66	9.667	2681	2683	2685	rBV	291	119	0.01%	0.001%
67	9.706	2693	2695	2698	rVB2	210	117	0.01%	0.001%
68	9.725	2698	2701	2702	rBV2	136	83	0.00%	0.001%
69	9.731	2702	2703	2707	rVV	253	160	0.01%	0.001%
70	9.776	2715	2717	2719	rBV2	186	78	0.00%	0.001%
71	9.825	2729	2732	2733	rBV	201	114	0.01%	0.001%
72	9.905	2755	2757	2760	rBV2	144	107	0.01%	0.001%
73	9.988	2780	2783	2785	rBV2	202	118	0.01%	0.001%
74	10.101	2815	2818	2820	rBV	266	199	0.01%	0.001%
75	10.149	2821	2833	2856	rBV	548811	870686	47.12%	6.303%
76	10.439	2919	2923	2927	rVB3	284	223	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035369.D
 Acq On : 23 Apr 2024 18:38
 Operator : SY/MD
 Sample : P2158-04DL2 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD0DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.474	2932	2934	2936	rBV	189	81	0.00%	0.001%
78	10.622	2978	2980	2984	rBV3	271	207	0.01%	0.001%
79	10.657	2989	2991	2994	rBV	316	152	0.01%	0.001%
80	10.751	3017	3020	3021	rBV	140	85	0.00%	0.001%
81	10.779	3025	3029	3030	rBV	405	292	0.02%	0.002%
82	10.831	3042	3045	3048	rBV2	428	289	0.02%	0.002%
83	10.879	3059	3060	3066	rVB2	208	177	0.01%	0.001%
84	10.905	3066	3068	3070	rBV	195	114	0.01%	0.001%
85	11.024	3102	3105	3108	rBV2	218	163	0.01%	0.001%
86	11.123	3127	3136	3144	rBV2	16574	26467	1.43%	0.192%
87	11.185	3144	3155	3186	rVV2	753399	1831007	99.09%	13.256%
88	11.480	3244	3247	3249	rBV2	572	321	0.02%	0.002%
89	11.561	3259	3272	3306	rBV3	890597	1847872	100.00%	13.378%
90	11.837	3354	3358	3361	rBV3	347	332	0.02%	0.002%
91	11.873	3367	3369	3371	rBV2	325	176	0.01%	0.001%
92	12.001	3407	3409	3412	rBV	280	152	0.01%	0.001%
93	12.490	3556	3561	3565	rBV3	549	561	0.03%	0.004%
94	12.513	3565	3568	3571	rBV3	526	430	0.02%	0.003%
95	12.715	3629	3631	3634	rBV2	346	199	0.01%	0.001%
96	12.750	3640	3642	3646	rBV2	412	344	0.02%	0.002%
97	12.953	3702	3705	3711	rBV3	649	597	0.03%	0.004%
98	13.201	3773	3782	3801	rBV3	31311	50588	2.74%	0.366%
99	13.326	3819	3821	3826	rVB2	567	330	0.02%	0.002%
100	13.683	3927	3932	3945	rVB5	2937	4767	0.26%	0.035%




Sum of corrected areas: 13813051

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035369.D
Acq On : 23 Apr 2024 18:38
Operator : SY/MD
Sample : P2158-04DL2 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD0DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

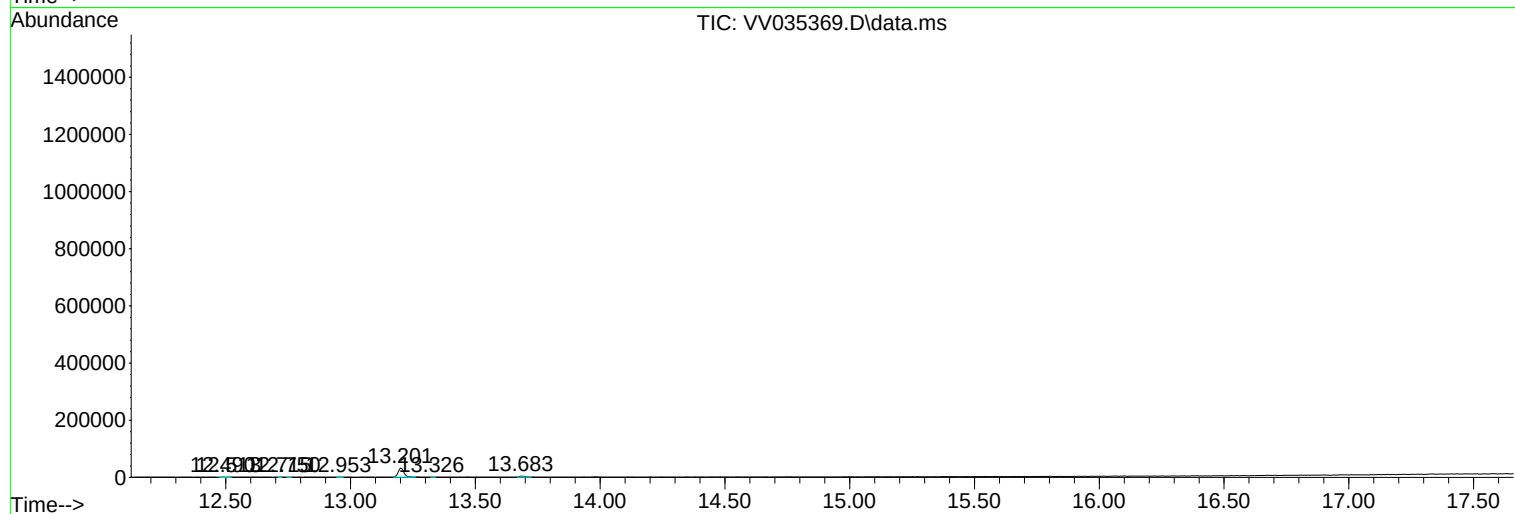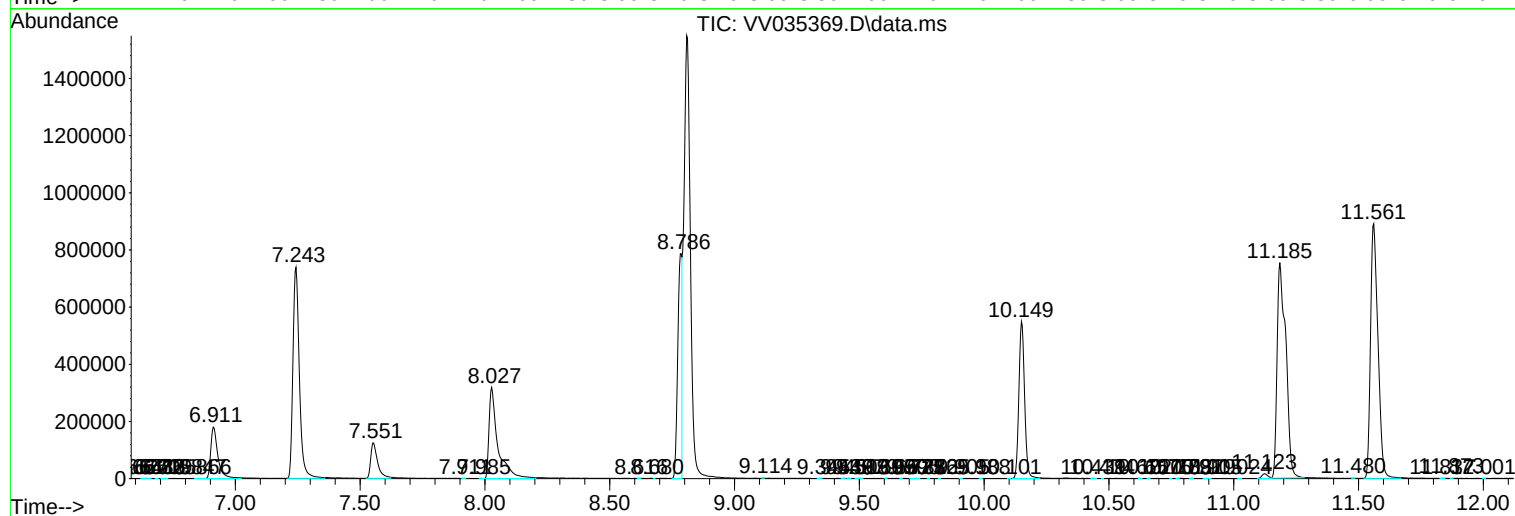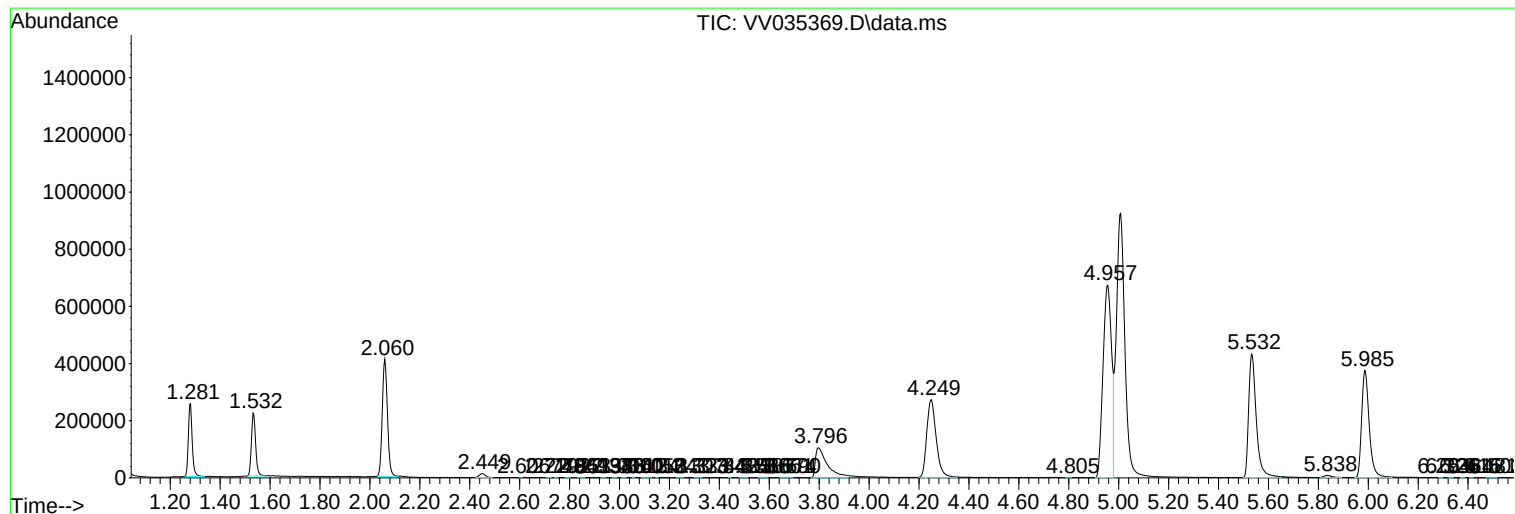

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035369.D
Acq On : 23 Apr 2024 18:38
Operator : SY/MD
Sample : P2158-04DL2 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD0DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035369.D
Acq On : 23 Apr 2024 18:38
Operator : SY/MD
Sample : P2158-04DL2 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD0DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
