

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035370.D
 Acq On : 23 Apr 2024 19:01
 Operator : SY/MD
 Sample : P2158-12DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RE2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035370.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.227	48	58	59	rBV4	2145	3295	0.13%	0.023%
2	1.281	67	75	96	rVB	251430	269038	10.89%	1.876%
3	1.532	146	153	174	rVB	215057	253166	10.25%	1.766%
4	2.059	307	317	336	rBV	408137	589426	23.86%	4.111%
5	2.452	428	439	452	rVB	14656	25765	1.04%	0.180%
6	2.638	494	497	500	rBV	338	260	0.01%	0.002%
7	2.703	515	517	521	rVV3	295	254	0.01%	0.002%
8	2.895	573	577	582	rVB3	251	258	0.01%	0.002%
9	2.950	591	594	597	rBV	401	263	0.01%	0.002%
10	3.153	651	657	660	rVB2	482	359	0.01%	0.003%
11	3.272	689	694	699	rVB2	217	253	0.01%	0.002%
12	3.307	703	705	713	rBV2	236	280	0.01%	0.002%
13	3.619	796	802	805	rBV2	242	224	0.01%	0.002%
14	3.674	814	819	825	rBV3	385	304	0.01%	0.002%
15	3.799	849	858	913	rBV	101249	354512	14.35%	2.472%
16	4.246	980	997	1037	rBV	270112	704614	28.52%	4.914%
17	4.635	1114	1118	1119	rBV	639	376	0.02%	0.003%
18	4.725	1140	1146	1148	rBV2	907	852	0.03%	0.006%
19	4.809	1168	1172	1173	rBV2	367	230	0.01%	0.002%
20	4.844	1181	1183	1186	rVV	362	276	0.01%	0.002%
21	4.956	1202	1218	1227	rBV2	659482	1666687	67.47%	11.624%
22	5.326	1330	1333	1335	rBV4	548	397	0.02%	0.003%
23	5.416	1358	1361	1364	rBV5	601	382	0.02%	0.003%
24	5.497	1383	1386	1387	rBV2	524	255	0.01%	0.002%
25	5.532	1387	1397	1429	rBV	439040	927471	37.54%	6.468%
26	5.841	1481	1493	1507	rBV5	7481	17325	0.70%	0.121%
27	5.985	1523	1538	1572	rBV	373291	786744	31.85%	5.487%
28	6.275	1626	1628	1633	rVB2	445	305	0.01%	0.002%
29	6.297	1633	1635	1638	rBV4	412	299	0.01%	0.002%
30	6.317	1638	1641	1647	rVB3	448	372	0.02%	0.003%
31	6.442	1679	1680	1685	rVB	422	240	0.01%	0.002%
32	6.468	1685	1688	1694	rBV2	228	264	0.01%	0.002%
33	6.522	1701	1705	1711	rVV2	393	385	0.02%	0.003%
34	6.622	1732	1736	1738	rBV	422	297	0.01%	0.002%
35	6.664	1746	1749	1751	rVB2	551	311	0.01%	0.002%
36	6.712	1762	1764	1769	rVB2	290	224	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035370.D
 Acq On : 23 Apr 2024 19:01
 Operator : SY/MD
 Sample : P2158-12DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RE2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.744	1769	1774	1775	rBV	334	224	0.01%	0.002%
38	6.828	1798	1800	1806	rVB2	338	268	0.01%	0.002%
39	6.873	1806	1814	1815	rBV2	230	244	0.01%	0.002%
40	6.911	1815	1826	1853	rBV	178923	350215	14.18%	2.442%
41	7.127	1890	1893	1896	rVB3	552	405	0.02%	0.003%
42	7.149	1896	1900	1901	rBV3	605	391	0.02%	0.003%
43	7.194	1912	1914	1917	rVB3	477	261	0.01%	0.002%
44	7.243	1917	1929	1968	rBV	731331	1312338	53.12%	9.152%
45	7.554	2016	2026	2056	rBV	126226	240828	9.75%	1.680%
46	7.741	2082	2084	2087	rBV3	486	263	0.01%	0.002%
47	7.921	2136	2140	2143	rVB3	561	444	0.02%	0.003%
48	7.950	2146	2149	2153	rBV2	227	226	0.01%	0.002%
49	8.027	2164	2173	2215	rBV2	304278	749438	30.34%	5.227%
50	8.394	2285	2287	2292	rVB4	513	285	0.01%	0.002%
51	8.599	2348	2351	2354	rVB2	326	222	0.01%	0.002%
52	8.635	2354	2362	2364	rBV3	379	434	0.02%	0.003%
53	8.693	2376	2380	2386	rVB4	421	496	0.02%	0.003%
54	8.738	2392	2394	2397	rBV	353	286	0.01%	0.002%
55	8.786	2397	2409	2410	rBV	810084	957793	38.77%	6.680%
56	9.075	2495	2499	2500	rBV3	623	406	0.02%	0.003%
57	9.201	2532	2538	2545	rBV4	768	1092	0.04%	0.008%
58	9.284	2560	2564	2568	rVB4	296	273	0.01%	0.002%
59	9.419	2603	2606	2609	rVV3	397	321	0.01%	0.002%
60	9.471	2617	2622	2624	rVV2	284	297	0.01%	0.002%
61	9.506	2627	2633	2637	rVB3	617	501	0.02%	0.003%
62	9.538	2637	2643	2645	rBV2	508	350	0.01%	0.002%
63	9.590	2657	2659	2663	rVB	436	241	0.01%	0.002%
64	9.699	2689	2693	2696	rVB3	334	263	0.01%	0.002%
65	9.744	2700	2707	2709	rVB3	377	354	0.01%	0.002%
66	9.805	2722	2726	2731	rVB	412	466	0.02%	0.003%
67	10.027	2791	2795	2798	rBV3	341	228	0.01%	0.002%
68	10.149	2821	2833	2858	rBV	552609	873471	35.36%	6.092%
69	10.413	2912	2915	2920	rBV3	297	288	0.01%	0.002%
70	10.715	3004	3009	3012	rBV	281	230	0.01%	0.002%
71	10.792	3028	3033	3035	rBV2	377	266	0.01%	0.002%
72	10.892	3060	3064	3069	rVB2	325	255	0.01%	0.002%
73	11.120	3125	3135	3144	rBV	57803	92948	3.76%	0.648%
74	11.185	3144	3155	3157	rBV	825245	1013440	41.02%	7.068%
75	11.448	3234	3237	3240	rBV2	420	308	0.01%	0.002%
76	11.564	3259	3273	3305	rBV2	1051390	2470398	100.00%	17.229%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035370.D
 Acq On : 23 Apr 2024 19:01
 Operator : SY/MD
 Sample : P2158-12DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RE2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	11.808	3347	3349	3351	rVV2	511	224	0.01%	0.002%
78	11.844	3355	3360	3366	rVB3	698	549	0.02%	0.004%
79	12.133	3448	3450	3456	rVB2	410	259	0.01%	0.002%
80	12.188	3460	3467	3470	rBV3	646	773	0.03%	0.005%
81	12.265	3489	3491	3494	rVB3	422	257	0.01%	0.002%
82	12.361	3512	3521	3529	rBV7	1648	2955	0.12%	0.021%
83	12.519	3566	3570	3571	rBV	378	252	0.01%	0.002%
84	12.586	3586	3591	3592	rBV2	731	608	0.02%	0.004%
85	12.676	3615	3619	3620	rBV2	450	307	0.01%	0.002%
86	12.693	3620	3624	3630	rVB3	780	962	0.04%	0.007%
87	12.834	3666	3668	3673	rBV3	266	244	0.01%	0.002%
88	12.959	3703	3707	3709	rVB2	328	231	0.01%	0.002%
89	13.024	3723	3727	3732	rBV4	291	264	0.01%	0.002%
90	13.107	3745	3753	3756	rBV3	481	569	0.02%	0.004%
91	13.197	3769	3781	3809	rVV	316108	505134	20.45%	3.523%
92	13.680	3921	3931	3949	rBV	85010	133136	5.39%	0.929%
93	13.979	4021	4024	4032	rVB2	1148	1251	0.05%	0.009%
94	14.326	4130	4132	4133	rBV	431	230	0.01%	0.002%
95	14.641	4228	4230	4237	rVB5	606	572	0.02%	0.004%
96	14.692	4242	4246	4250	rBV2	792	654	0.03%	0.005%
97	14.763	4259	4268	4277	rVB7	2027	3637	0.15%	0.025%
98	14.995	4338	4340	4345	rBV3	721	658	0.03%	0.005%
99	15.271	4422	4426	4430	rBV4	1149	1293	0.05%	0.009%
100	15.335	4440	4446	4457	rBV7	3849	6286	0.25%	0.044%




Sum of corrected areas: 14338725

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035370.D
Acq On : 23 Apr 2024 19:01
Operator : SY/MD
Sample : P2158-12DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

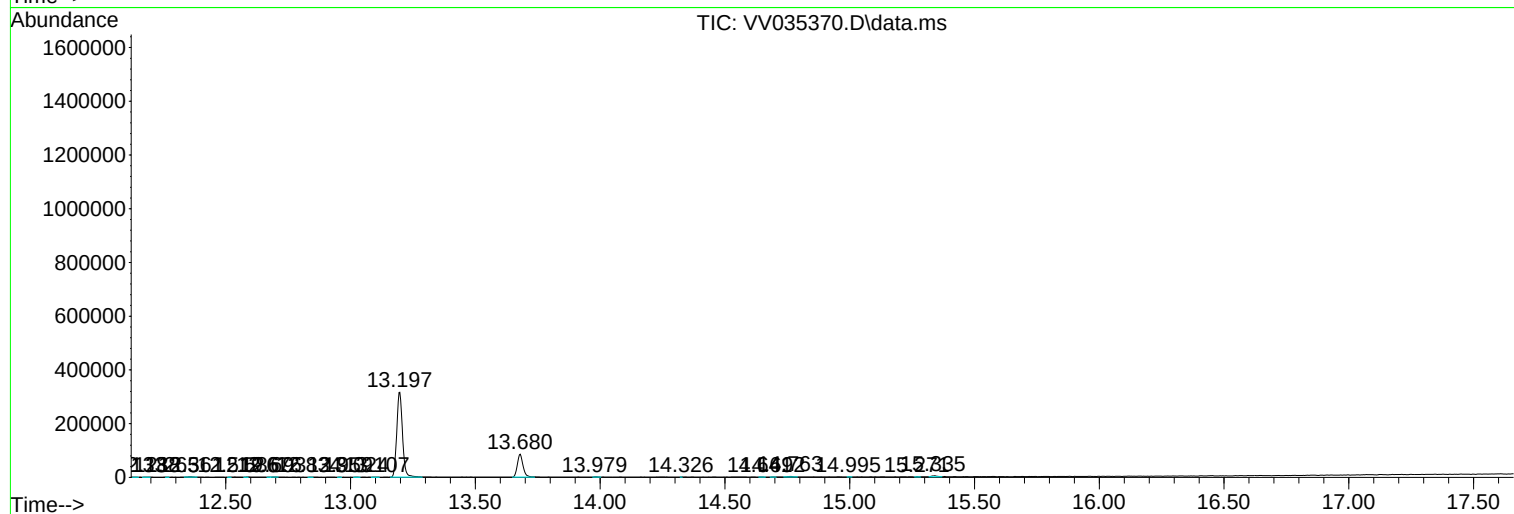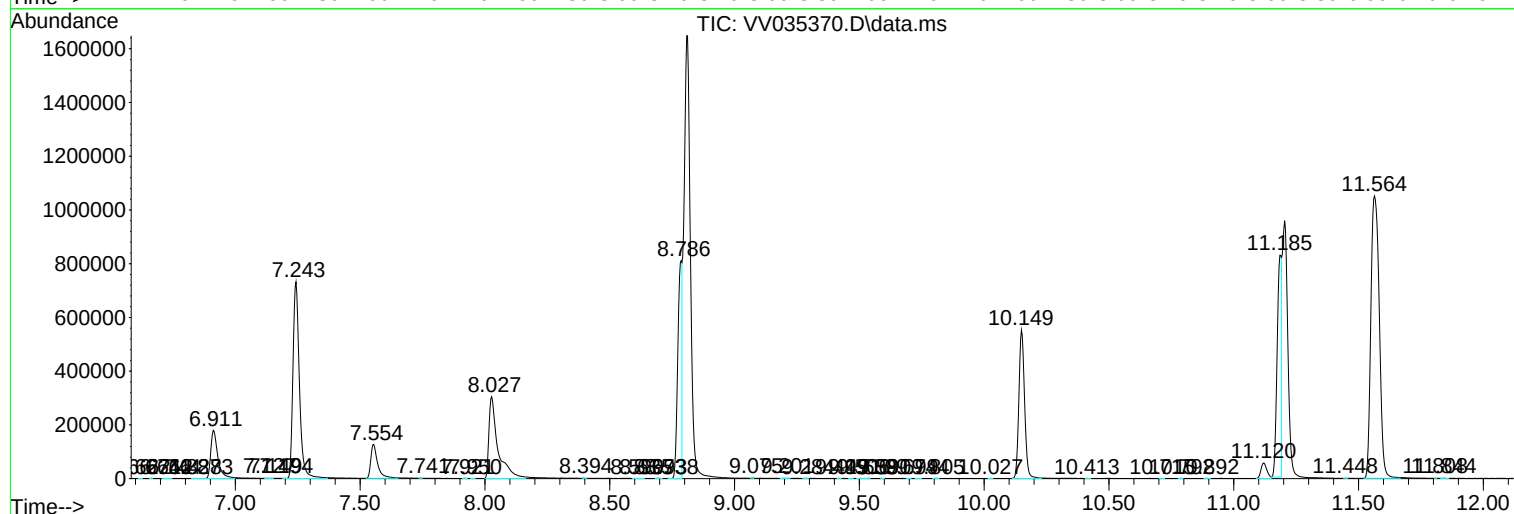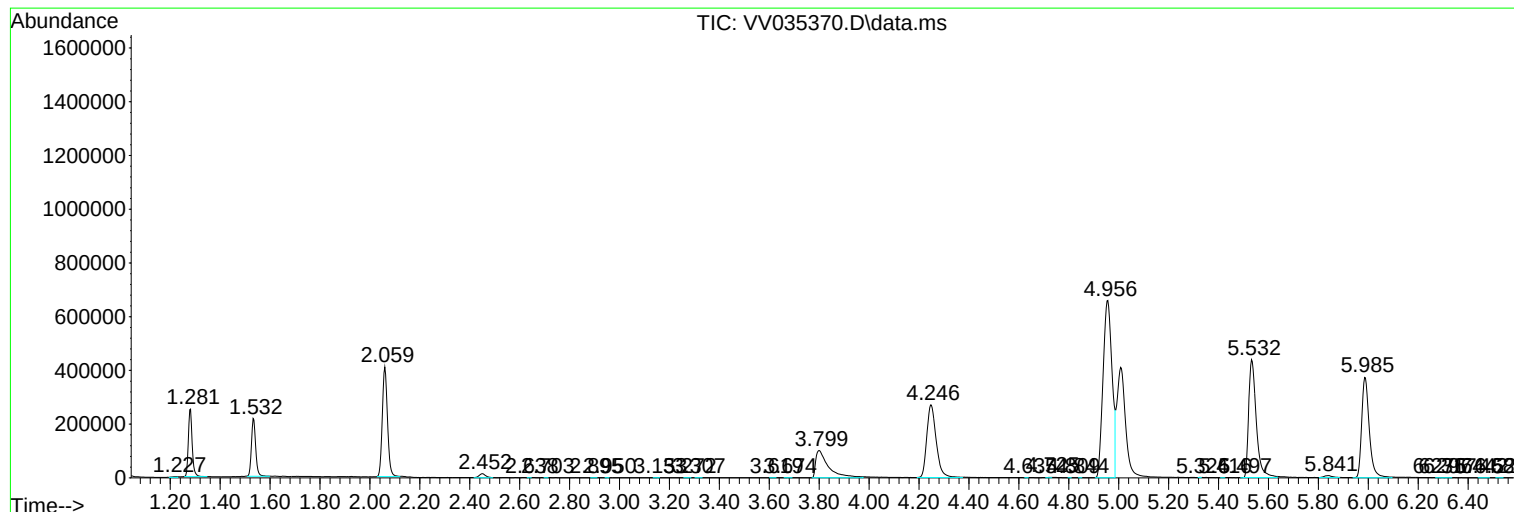

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035370.D
Acq On : 23 Apr 2024 19:01
Operator : SY/MD
Sample : P2158-12DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035370.D
Acq On : 23 Apr 2024 19:01
Operator : SY/MD
Sample : P2158-12DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------