

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035371.D
 Acq On : 23 Apr 2024 19:24
 Operator : SY/MD
 Sample : P2158-10DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035371.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rBV	259608	277350	11.37%	1.854%
2	1.532	146	153	169	rBV	222716	259539	10.64%	1.735%
3	2.060	307	317	349	rVB	420058	625312	25.63%	4.179%
4	2.285	384	387	390	rBV2	672	502	0.02%	0.003%
5	2.449	428	438	458	rVB2	15295	25522	1.05%	0.171%
6	2.667	503	506	508	rBV3	380	302	0.01%	0.002%
7	2.931	586	588	589	rBV	232	90	0.00%	0.001%
8	2.947	589	593	594	rBV2	324	169	0.01%	0.001%
9	2.992	605	607	610	rBV2	268	170	0.01%	0.001%
10	3.018	613	615	623	rVB3	288	304	0.01%	0.002%
11	3.050	623	625	631	rVB3	280	155	0.01%	0.001%
12	3.076	631	633	641	rVB2	292	296	0.01%	0.002%
13	3.127	641	649	651	rBV2	342	407	0.02%	0.003%
14	3.269	688	693	695	rVB2	282	213	0.01%	0.001%
15	3.384	726	729	734	rBV2	260	225	0.01%	0.002%
16	3.429	741	743	745	rBV2	254	152	0.01%	0.001%
17	3.458	749	752	754	rBV	170	123	0.01%	0.001%
18	3.497	761	764	769	rBV3	193	174	0.01%	0.001%
19	3.535	773	776	779	rBV	215	178	0.01%	0.001%
20	3.638	803	808	810	rBV2	219	126	0.01%	0.001%
21	3.658	811	814	816	rVB	225	127	0.01%	0.001%
22	3.719	827	833	836	rBV2	162	156	0.01%	0.001%
23	3.767	845	848	849	rBV2	216	95	0.00%	0.001%
24	3.799	849	858	897	rBV	105116	356927	14.63%	2.385%
25	4.246	982	997	1039	rBV	278208	729995	29.92%	4.879%
26	4.696	1133	1137	1138	rBV2	302	219	0.01%	0.001%
27	4.715	1141	1143	1146	rBV2	713	518	0.02%	0.003%
28	4.793	1166	1167	1169	rBV	320	140	0.01%	0.001%
29	4.828	1174	1178	1183	rBV	378	369	0.02%	0.002%
30	4.953	1201	1217	1229	rBV2	680793	1767616	72.45%	11.814%
31	5.410	1356	1359	1360	rBV2	297	172	0.01%	0.001%
32	5.532	1386	1397	1432	rBV	450938	948982	38.89%	6.342%
33	5.834	1481	1491	1513	rBV3	7928	19263	0.79%	0.129%
34	5.986	1525	1538	1565	rBV	388057	807843	33.11%	5.399%
35	6.313	1637	1640	1643	rBV3	300	252	0.01%	0.002%
36	6.407	1666	1669	1672	rBV3	281	172	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035371.D
 Acq On : 23 Apr 2024 19:24
 Operator : SY/MD
 Sample : P2158-10DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.423	1672	1674	1679	rVB	267	194	0.01%	0.001%
38	6.455	1681	1684	1685	rBV2	308	131	0.01%	0.001%
39	6.510	1698	1701	1705	rBV2	168	162	0.01%	0.001%
40	6.555	1711	1715	1717	rVB3	320	237	0.01%	0.002%
41	6.590	1721	1726	1728	rBV2	181	164	0.01%	0.001%
42	6.606	1728	1731	1737	rVB2	261	191	0.01%	0.001%
43	6.635	1737	1740	1745	rBV3	285	363	0.01%	0.002%
44	6.709	1759	1763	1767	rBV	471	504	0.02%	0.003%
45	6.731	1767	1770	1772	rBV3	380	246	0.01%	0.002%
46	6.767	1775	1781	1785	rBV4	389	414	0.02%	0.003%
47	6.809	1791	1794	1795	rBV	225	116	0.00%	0.001%
48	6.841	1799	1804	1806	rBV3	254	173	0.01%	0.001%
49	6.870	1810	1813	1815	rBV2	307	145	0.01%	0.001%
50	6.912	1815	1826	1865	rBV	185863	369407	15.14%	2.469%
51	7.243	1917	1929	1958	rBV	756478	1359430	55.72%	9.086%
52	7.551	2016	2025	2050	rBV2	129389	245763	10.07%	1.643%
53	7.854	2115	2119	2121	rBV2	546	488	0.02%	0.003%
54	7.944	2145	2147	2149	rVB2	277	130	0.01%	0.001%
55	8.027	2163	2173	2217	rBV2	308790	764766	31.34%	5.111%
56	8.529	2326	2329	2330	rBV3	387	225	0.01%	0.002%
57	8.606	2346	2353	2355	rVB3	523	410	0.02%	0.003%
58	8.674	2372	2374	2375	rBV3	268	103	0.00%	0.001%
59	8.728	2388	2391	2393	rBV	267	184	0.01%	0.001%
60	8.744	2393	2396	2397	rBV2	324	181	0.01%	0.001%
61	8.786	2397	2409	2410	rBV	816506	973866	39.91%	6.509%
62	9.275	2559	2561	2563	rBV3	305	182	0.01%	0.001%
63	9.445	2611	2614	2616	rBV2	324	245	0.01%	0.002%
64	9.497	2628	2630	2633	rVB2	305	146	0.01%	0.001%
65	9.551	2644	2647	2649	rBV	347	178	0.01%	0.001%
66	9.609	2663	2665	2666	rBV	199	93	0.00%	0.001%
67	9.635	2671	2673	2676	rBV	357	180	0.01%	0.001%
68	9.677	2682	2686	2688	rBV2	308	174	0.01%	0.001%
69	9.706	2692	2695	2697	rBV	200	132	0.01%	0.001%
70	9.773	2712	2716	2719	rBV2	253	193	0.01%	0.001%
71	9.844	2731	2738	2740	rBV2	367	419	0.02%	0.003%
72	9.947	2768	2770	2773	rBV	234	98	0.00%	0.001%
73	10.024	2792	2794	2797	rVB2	284	153	0.01%	0.001%
74	10.040	2797	2799	2801	rBV2	180	100	0.00%	0.001%
75	10.149	2821	2833	2857	rBV	566658	898770	36.84%	6.007%
76	10.435	2919	2922	2923	rBV	325	142	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035371.D
 Acq On : 23 Apr 2024 19:24
 Operator : SY/MD
 Sample : P2158-10DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.728	3011	3013	3016	rBV2	246	143	0.01%	0.001%
78	10.789	3028	3032	3035	rVV2	428	312	0.01%	0.002%
79	10.834	3043	3046	3049	rVB2	172	117	0.00%	0.001%
80	10.853	3049	3052	3055	rBV	236	185	0.01%	0.001%
81	10.866	3055	3056	3060	rVB2	336	200	0.01%	0.001%
82	10.892	3060	3064	3069	rVB2	270	260	0.01%	0.002%
83	10.921	3069	3073	3074	rBV	271	155	0.01%	0.001%
84	10.956	3079	3084	3089	rBV3	360	320	0.01%	0.002%
85	10.982	3089	3092	3098	rVB2	323	267	0.01%	0.002%
86	11.017	3098	3103	3104	rBV2	223	176	0.01%	0.001%
87	11.075	3118	3121	3124	rBV3	281	232	0.01%	0.002%
88	11.120	3125	3135	3144	rBV	73956	117379	4.81%	0.784%
89	11.185	3145	3155	3159	rBV	802378	1275128	52.26%	8.522%
90	11.561	3255	3272	3306	rBV2	1040410	2439938	100.00%	16.307%
91	12.053	3422	3425	3429	rBV2	362	373	0.02%	0.002%
92	12.127	3446	3448	3456	rBV2	300	321	0.01%	0.002%
93	12.252	3485	3487	3489	rBV	424	269	0.01%	0.002%
94	12.490	3559	3561	3563	rBV	395	245	0.01%	0.002%
95	12.696	3619	3625	3629	rBV5	1573	1987	0.08%	0.013%
96	12.805	3658	3659	3661	rBV	297	98	0.00%	0.001%
97	13.088	3745	3747	3753	rBV3	376	436	0.02%	0.003%
98	13.194	3770	3780	3804	rBV	327468	528473	21.66%	3.532%
99	13.423	3848	3851	3854	rBV2	609	505	0.02%	0.003%
100	13.680	3921	3931	3951	rBV2	94743	151707	6.22%	1.014%




Sum of corrected areas: 14962579

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035371.D
Acq On : 23 Apr 2024 19:24
Operator : SY/MD
Sample : P2158-10DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORE0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

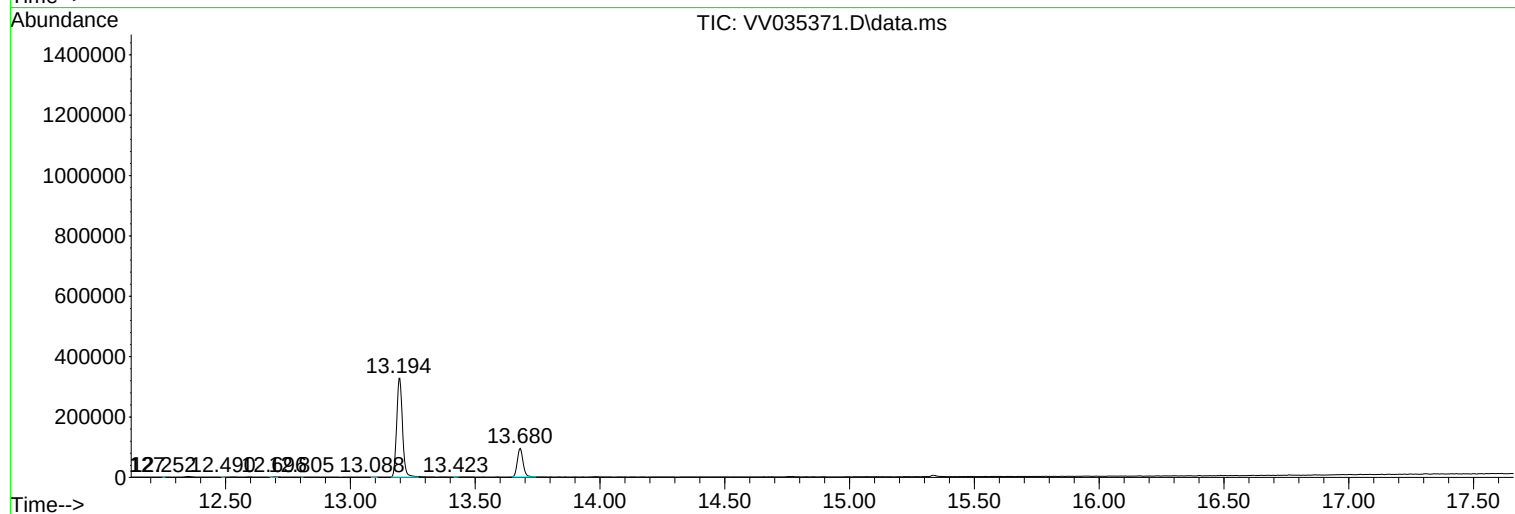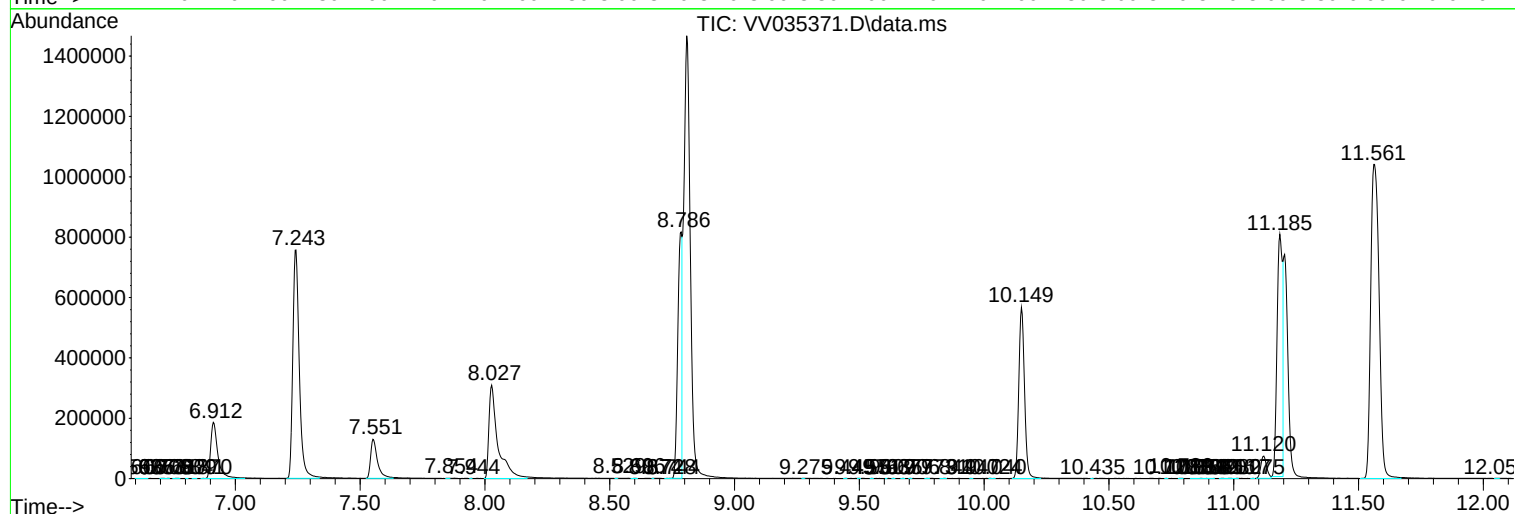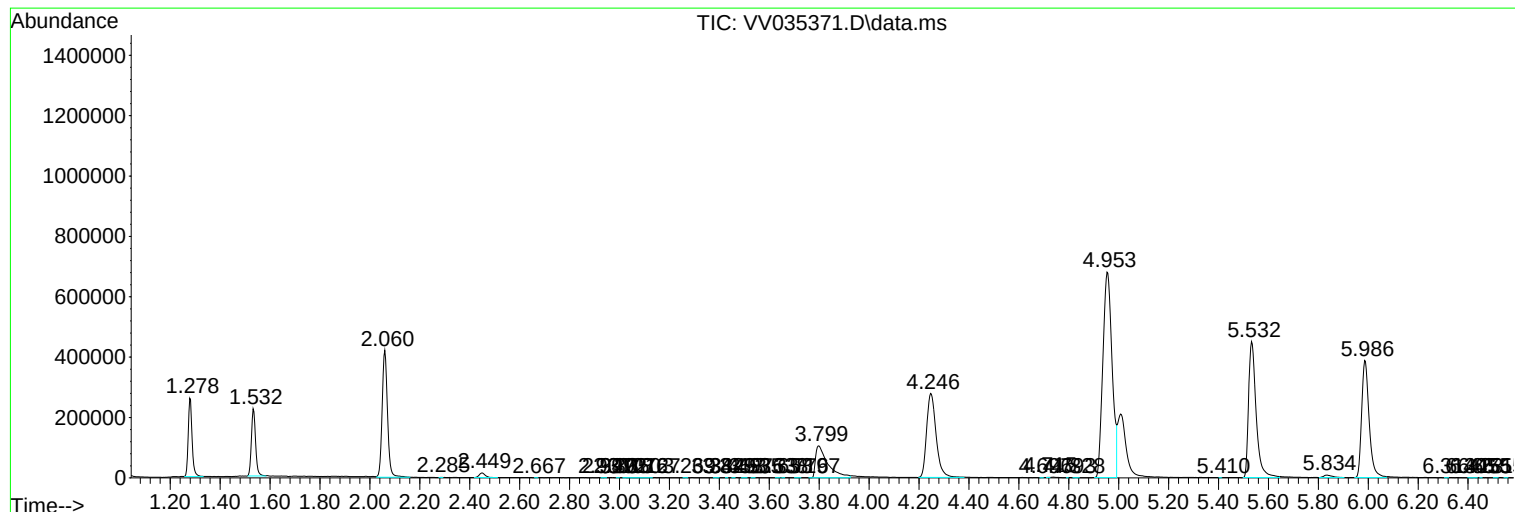

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035371.D
Acq On : 23 Apr 2024 19:24
Operator : SY/MD
Sample : P2158-10DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035371.D
Acq On : 23 Apr 2024 19:24
Operator : SY/MD
Sample : P2158-10DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------