

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035372.D
 Acq On : 23 Apr 2024 19:47
 Operator : SY/MD
 Sample : P2158-11DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RE1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035372.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	93	rVB	255161	275636	6.21%	1.384%
2	1.535	146	154	171	rBV	227733	263611	5.94%	1.324%
3	2.060	308	317	336	rVB	418015	603138	13.60%	3.029%
4	2.452	430	439	454	rVB2	6752	11364	0.26%	0.057%
5	2.693	513	514	516	rBV	261	90	0.00%	0.000%
6	2.838	556	559	560	rBV	188	114	0.00%	0.001%
7	2.899	575	578	579	rBV2	174	97	0.00%	0.000%
8	2.979	599	603	607	rBV2	341	337	0.01%	0.002%
9	3.037	617	621	622	rBV2	327	228	0.01%	0.001%
10	3.082	633	635	639	rBV2	192	130	0.00%	0.001%
11	3.153	654	657	660	rBV2	236	175	0.00%	0.001%
12	3.175	660	664	666	rVV2	291	210	0.00%	0.001%
13	3.304	700	704	709	rVB2	262	276	0.01%	0.001%
14	3.326	709	711	713	rBV2	218	111	0.00%	0.001%
15	3.387	728	730	733	rVB2	255	130	0.00%	0.001%
16	3.404	733	735	737	rBV	249	146	0.00%	0.001%
17	3.474	753	757	760	rBV2	307	258	0.01%	0.001%
18	3.519	770	771	773	rBV	151	50	0.00%	0.000%
19	3.564	782	785	789	rBV3	193	209	0.00%	0.001%
20	3.629	802	805	807	rBV2	97	65	0.00%	0.000%
21	3.667	812	817	820	rBV2	295	235	0.01%	0.001%
22	3.696	824	826	829	rVB3	213	110	0.00%	0.001%
23	3.712	829	831	837	rVB2	332	249	0.01%	0.001%
24	3.738	837	839	841	rBV	108	57	0.00%	0.000%
25	3.802	849	859	907	rBV	103377	367070	8.27%	1.844%
26	4.246	982	997	1032	rBV	277441	726983	16.39%	3.651%
27	4.767	1156	1159	1163	rBV2	336	254	0.01%	0.001%
28	4.828	1174	1178	1183	rBV2	266	237	0.01%	0.001%
29	4.957	1202	1218	1264	rBV2	674685	1801817	40.62%	9.049%
30	5.407	1356	1358	1361	rBV3	345	138	0.00%	0.001%
31	5.426	1361	1364	1368	rBV2	287	246	0.01%	0.001%
32	5.532	1386	1397	1443	rBV	434197	921918	20.78%	4.630%
33	5.834	1482	1491	1510	rBV4	7589	18537	0.42%	0.093%
34	5.985	1525	1538	1577	rBV	392899	821257	18.51%	4.125%
35	6.329	1642	1645	1648	rBV2	414	315	0.01%	0.002%
36	6.362	1652	1655	1656	rBV	258	120	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035372.D
 Acq On : 23 Apr 2024 19:47
 Operator : SY/MD
 Sample : P2158-11DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORE1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.374	1657	1659	1662	rBV2	210	89	0.00%	0.000%
38	6.432	1676	1677	1678	rBV2	204	59	0.00%	0.000%
39	6.481	1689	1692	1693	rBV	221	114	0.00%	0.001%
40	6.542	1709	1711	1715	rBV2	186	123	0.00%	0.001%
41	6.583	1720	1724	1726	rBV	205	169	0.00%	0.001%
42	6.612	1729	1733	1737	rVB2	373	255	0.01%	0.001%
43	6.638	1739	1741	1743	rBV2	305	141	0.00%	0.001%
44	6.680	1748	1754	1757	rVB3	311	297	0.01%	0.001%
45	6.693	1757	1758	1760	rVB3	271	78	0.00%	0.000%
46	6.709	1760	1763	1766	rBV2	342	232	0.01%	0.001%
47	6.722	1766	1767	1770	rVB	338	130	0.00%	0.001%
48	6.757	1773	1778	1782	rBV2	419	425	0.01%	0.002%
49	6.799	1788	1791	1792	rBV	244	119	0.00%	0.001%
50	6.834	1799	1802	1804	rBV	166	77	0.00%	0.000%
51	6.911	1816	1826	1862	rBV	187154	370324	8.35%	1.860%
52	7.156	1899	1902	1903	rBV	554	305	0.01%	0.002%
53	7.243	1917	1929	1961	rBV	778943	1376779	31.04%	6.915%
54	7.551	2017	2025	2059	rBV	131015	246445	5.56%	1.238%
55	7.918	2135	2139	2141	rBV2	478	318	0.01%	0.002%
56	7.963	2149	2153	2155	rBV2	356	227	0.01%	0.001%
57	8.027	2158	2173	2220	rBV4	320331	793652	17.89%	3.986%
58	8.452	2303	2305	2306	rBV2	427	176	0.00%	0.001%
59	8.657	2367	2369	2370	rBV	153	43	0.00%	0.000%
60	8.667	2370	2372	2374	rVV	139	74	0.00%	0.000%
61	8.689	2377	2379	2382	rBV2	366	215	0.00%	0.001%
62	8.735	2391	2393	2396	rVB3	358	214	0.00%	0.001%
63	8.812	2396	2417	2450	rBV2	2025018	4435961	100.00%	22.279%
64	9.416	2604	2605	2608	rVB2	280	120	0.00%	0.001%
65	9.468	2615	2621	2622	rBV2	332	269	0.01%	0.001%
66	9.554	2645	2648	2651	rVB2	310	218	0.00%	0.001%
67	9.570	2651	2653	2654	rBV2	250	114	0.00%	0.001%
68	9.706	2693	2695	2697	rBV	257	128	0.00%	0.001%
69	9.741	2701	2706	2707	rBV	210	152	0.00%	0.001%
70	9.770	2713	2715	2722	rBV2	218	220	0.00%	0.001%
71	9.940	2765	2768	2772	rBV	137	125	0.00%	0.001%
72	9.960	2772	2774	2775	rBV	141	77	0.00%	0.000%
73	10.017	2790	2792	2793	rBV	260	112	0.00%	0.001%
74	10.091	2813	2815	2820	rVB3	434	300	0.01%	0.002%
75	10.149	2820	2833	2867	rBV	577940	911421	20.55%	4.577%
76	10.374	2902	2903	2906	rBV2	139	43	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
 Data File : VV035372.D
 Acq On : 23 Apr 2024 19:47
 Operator : SY/MD
 Sample : P2158-11DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RE1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.390	2906	2908	2911	rBV	245	132	0.00%	0.001%
78	10.519	2947	2948	2950	rVB	221	81	0.00%	0.000%
79	10.542	2950	2955	2959	rBV2	299	359	0.01%	0.002%
80	10.596	2971	2972	2973	rBV	119	44	0.00%	0.000%
81	10.641	2984	2986	2988	rBV	211	136	0.00%	0.001%
82	10.654	2988	2990	2994	rVV2	272	173	0.00%	0.001%
83	10.722	3007	3011	3017	rVV3	394	396	0.01%	0.002%
84	10.747	3017	3019	3022	rVV2	257	125	0.00%	0.001%
85	10.821	3039	3042	3043	rBV2	89	43	0.00%	0.000%
86	10.853	3050	3052	3054	rBV2	96	60	0.00%	0.000%
87	10.866	3054	3056	3059	rVB2	292	146	0.00%	0.001%
88	10.889	3059	3063	3065	rBV2	212	190	0.00%	0.001%
89	11.040	3106	3110	3112	rBV2	264	179	0.00%	0.001%
90	11.075	3119	3121	3125	rVB3	283	173	0.00%	0.001%
91	11.120	3125	3135	3145	rBV	58923	96783	2.18%	0.486%
92	11.185	3145	3155	3189	rVB2	748597	1593282	35.92%	8.002%
93	11.574	3258	3276	3302	rBV2	1843803	3889770	87.69%	19.535%
94	11.927	3384	3386	3389	rVB	367	230	0.01%	0.001%
95	11.998	3405	3408	3412	rBV3	306	281	0.01%	0.001%
96	12.866	3674	3678	3679	rBV2	482	344	0.01%	0.002%
97	12.943	3699	3702	3705	rBV2	344	254	0.01%	0.001%
98	13.011	3721	3723	3725	rBV2	341	224	0.01%	0.001%
99	13.197	3770	3781	3800	rBV	198485	315617	7.11%	1.585%
100	13.680	3923	3931	3947	rVB2	34850	56022	1.26%	0.281%




Sum of corrected areas: 19911302

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035372.D
Acq On : 23 Apr 2024 19:47
Operator : SY/MD
Sample : P2158-11DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

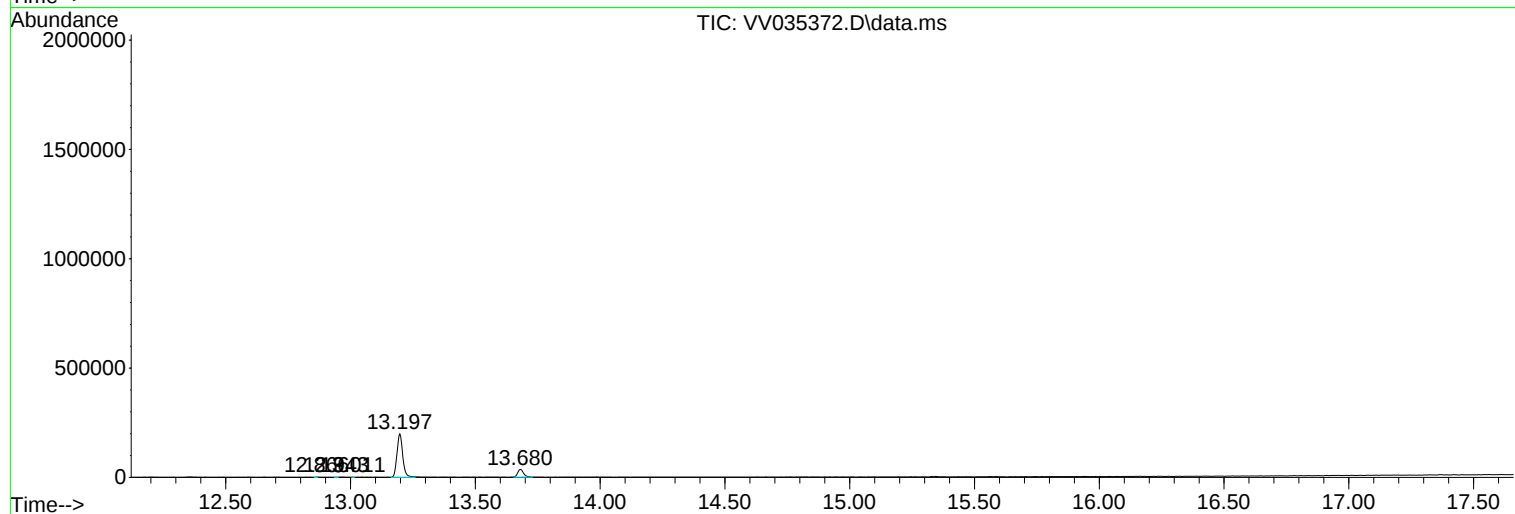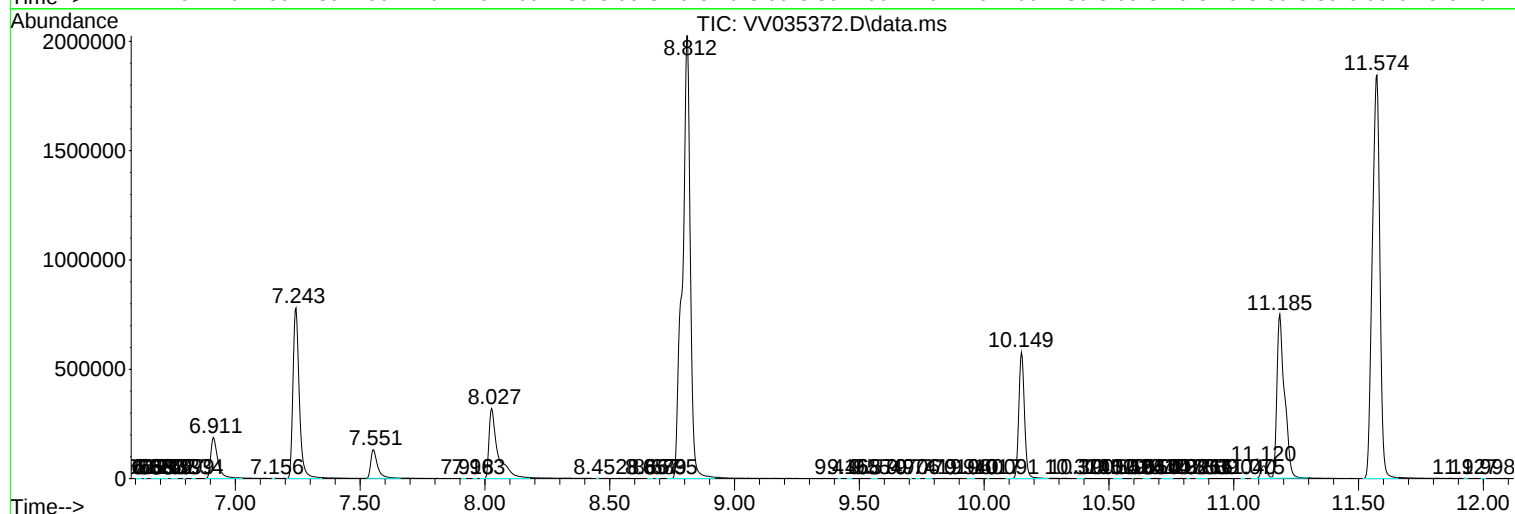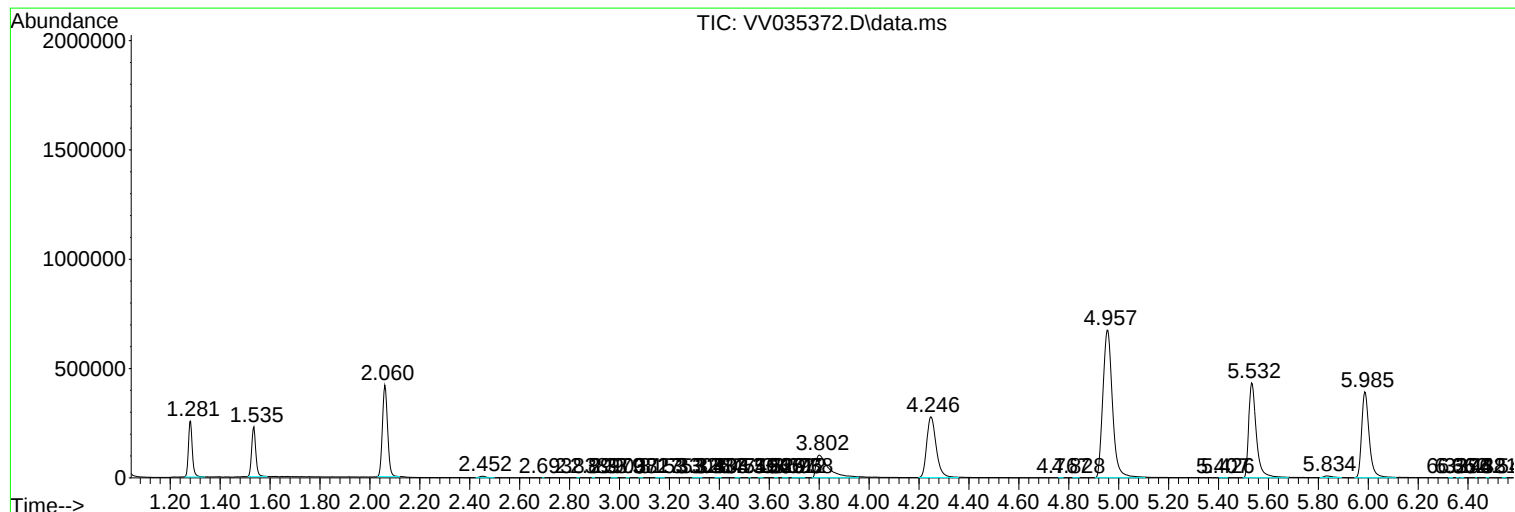

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035372.D
Acq On : 23 Apr 2024 19:47
Operator : SY/MD
Sample : P2158-11DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035372.D
Acq On : 23 Apr 2024 19:47
Operator : SY/MD
Sample : P2158-11DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RE1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc