


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042324\
Data File : VV035346.D
Acq On : 23 Apr 2024 08:50
Operator : SY/MD
Sample : BFB289
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB289

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis
Last Update : Tue Apr 23 23:26:51 2024

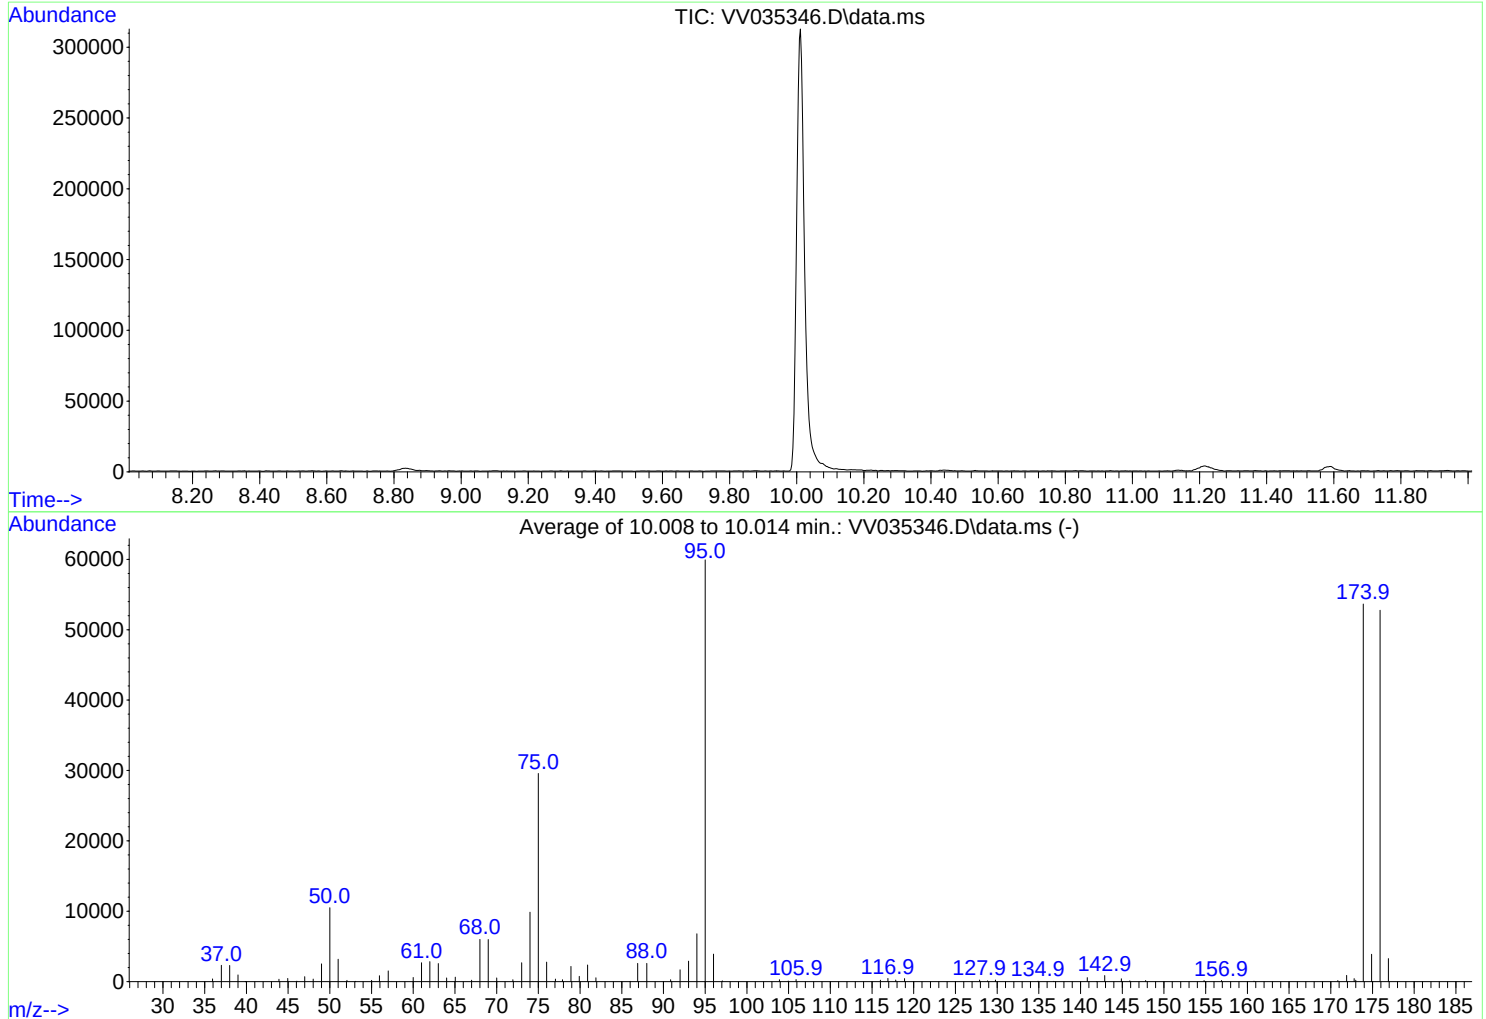

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	10514	PASS
75	95	30	80	49.4	29581	PASS
95	95	100	100	100.0	59928	PASS
96	95	5	9	6.5	3907	PASS
173	174	0.00	2	0.8	437	PASS
174	95	50	120	89.5	53643	PASS
175	174	5	9	7.2	3878	PASS
176	174	95	105	98.3	52752	PASS
177	176	5	10	6.2	3264	PASS

m/z	Abundance
39.90	203.0
43.90	395.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289

m/z	Abundance
36.00	413.0
37.00	2377.0
38.00	2406.0
39.00	958.0
39.90	192.0
44.00	782.0
45.00	432.0
46.10	111.0
47.00	683.0
48.00	347.0
49.00	2564.0
50.00	10967.0
51.00	3313.0
52.00	215.0
55.00	176.0
56.00	773.0
57.00	1505.0
60.00	528.0
61.00	2852.0
62.00	2949.0
63.00	2418.0
64.00	464.0
65.10	602.0
67.00	215.0
68.00	6317.0
69.00	6152.0
70.00	534.0
72.10	282.0
73.00	2904.0
74.00	10499.0
75.00	29792.0
76.00	2773.0
77.10	446.0
77.90	295.0
78.90	2160.0
79.90	805.0
80.90	2365.0
81.90	542.0
86.00	144.0
86.90	2576.0
88.00	2540.0
90.80	260.0
92.00	1739.0
93.00	2986.0
94.00	7003.0
95.00	60552.0
96.00	3959.0
97.10	130.0
103.90	330.0
105.90	310.0
116.00	178.0
116.90	461.0
117.80	218.0
118.90	421.0
127.90	211.0
128.80	124.0
129.80	235.0
136.80	117.0
140.80	547.0
142.90	844.0
144.90	347.0
145.90	113.0
147.80	152.0
154.80	133.0
156.90	184.0
171.00	178.0
171.90	823.0
172.80	657.0
173.90	53584.0
174.90	3933.0
175.90	52504.0
176.90	3325.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289

m/z	Abundance
35.90	389.0
37.00	2324.0
38.00	2360.0
39.00	977.0
39.90	196.0
44.00	758.0
44.90	470.0
46.00	109.0
47.00	740.0
48.00	372.0
49.00	2604.0
50.00	10827.0
51.00	3288.0
52.10	166.0
55.00	205.0
55.90	861.0
57.00	1557.0
60.00	612.0
61.00	2694.0
62.00	2863.0
63.00	2645.0
64.00	581.0
65.10	639.0
67.00	211.0
68.00	6208.0
69.00	6207.0
70.00	549.0
71.90	274.0
73.00	2789.0
74.00	10203.0
75.00	30536.0
76.00	2858.0
77.10	365.0
77.90	270.0
78.90	2210.0
79.90	779.0
80.90	2421.0
81.90	569.0
86.90	2651.0
88.00	2728.0
90.80	269.0
92.00	1744.0
93.00	3035.0
94.00	6983.0
95.00	61840.0
96.00	4029.0
97.00	130.0
103.90	283.0
105.00	140.0
105.90	313.0
116.00	216.0
116.90	459.0
117.90	244.0
118.90	450.0
127.90	237.0
128.80	125.0
129.80	249.0
134.90	110.0
140.80	603.0
141.90	106.0
142.90	910.0
144.90	429.0
145.90	125.0
147.80	168.0
154.80	159.0
156.90	177.0
160.80	117.0
170.80	152.0
171.90	931.0
172.80	654.0
173.90	55456.0
174.90	3993.0
175.90	54632.0
176.90	3343.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289

m/z	Abundance
35.90	390.0
37.00	2235.0
38.00	2148.0
39.00	925.0
39.80	239.0
43.90	697.0
44.90	446.0
47.00	709.0
48.00	360.0
49.00	2433.0
50.00	9749.0
51.00	2928.0
52.10	141.0
53.10	118.0
55.00	179.0
55.90	902.0
57.00	1504.0
60.00	628.0
61.00	2473.0
62.00	2689.0
63.00	2636.0
64.00	561.0
65.00	663.0
67.00	161.0
68.00	5499.0
69.00	5553.0
70.00	464.0
71.90	276.0
73.00	2380.0
74.00	8935.0
75.00	28416.0
76.00	2681.0
76.90	300.0
77.90	252.0
78.90	2119.0
79.90	678.0
80.90	2296.0
81.90	525.0
86.90	2533.0
88.00	2514.0
90.90	288.0
92.00	1554.0
93.00	2740.0
94.00	6380.0
95.00	57392.0
96.00	3732.0
97.00	110.0
103.90	234.0
104.90	144.0
105.90	257.0
116.00	241.0
116.90	426.0
117.90	252.0
118.90	441.0
127.90	255.0
128.90	103.0
129.80	205.0
134.90	128.0
140.80	591.0
142.90	857.0
144.90	441.0
145.90	108.0
147.80	172.0
154.80	163.0
156.90	145.0
160.80	115.0
170.80	121.0
171.90	927.0
173.00	637.0
173.90	51888.0
174.90	3707.0
175.90	51120.0
176.90	3125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB289