

Data File : VV010460.D
Acq On : 24 Apr 2019 14:11
Operator : SY/MD
Sample : K2428-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XF9

Quant Time: Apr 29 04:57:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 25 02:19:56 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	240424	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	237616	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	117350	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	74609	5.32	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.40%
7) Chloroethane-d5	1.59	69	58802	5.60	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.00%
11) 1,1-Dichloroethene-d2	2.13	63	110651	4.08	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.60%
20) 2-Butanone-d5	3.95	46	142321	47.89	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.78%
24) Chloroform-d	4.40	84	126584	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.20%
26) 1,2-Dichloroethane-d4	5.08	65	78130	5.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.80%
32) Benzene-d6	5.10	84	301796	5.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.40%
36) 1,2-Dichloropropane-d6	6.12	67	86518	5.20	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.00%
41) Toluene-d8	7.36	98	286950	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.40%
43) trans-1,3-Dichloropropene-	7.67	79	31313	4.77	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.40%
46) 2-Hexanone-d5	8.14	63	126749	50.61	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.22%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	63188	5.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	116306	5.36	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.20%


Target Compounds					Qvalue
13) Acetone	2.19	43	5891	3.295 ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV010460.D
Acq On : 24 Apr 2019 14:11
Operator : SY/MD
Sample : K2428-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XF9

Quant Time: Apr 29 04:57:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 25 02:19:56 2019
Response via : Initial Calibration

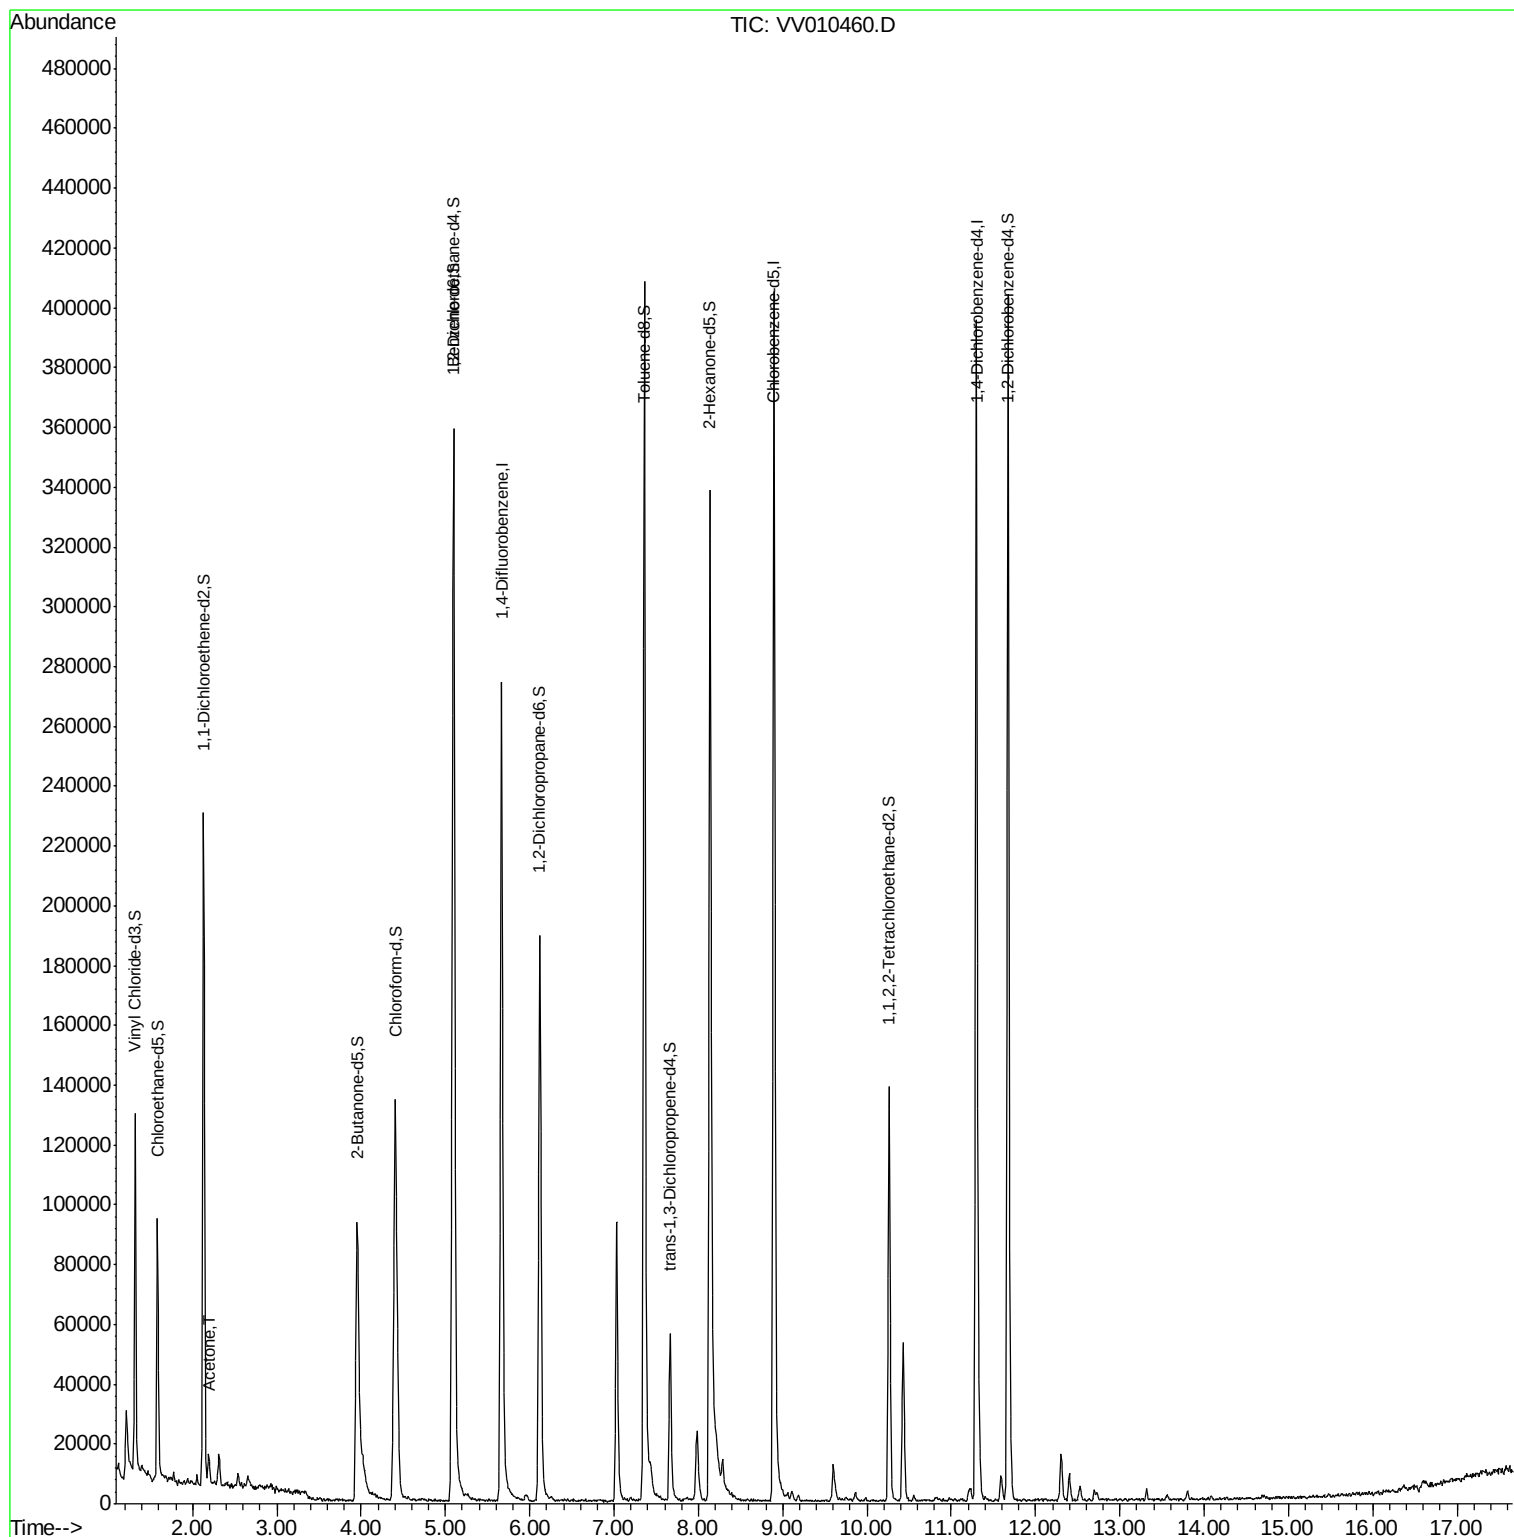

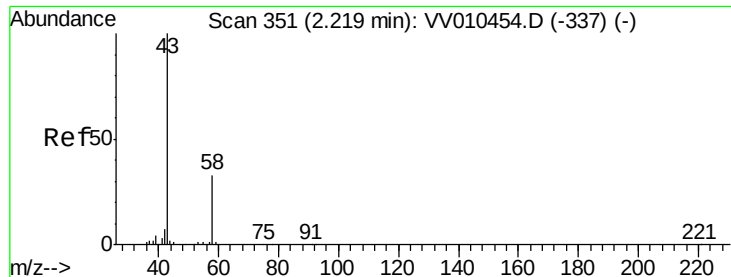

#13

Acetone

Concen: 3.295 ug/L

RT: 2.19 min Scan# 343

Delta R.T. -0.03 min

Lab File: VV010460.D

Acq: 24 Apr 2019 14:11


Instrument :
MSVOA_V
ClientSampleId :
C0XF9

Tgt Ion: 43 Resp: 5891

Ion Ratio Lower Upper

43 100

58 37.5 0.0 59.6

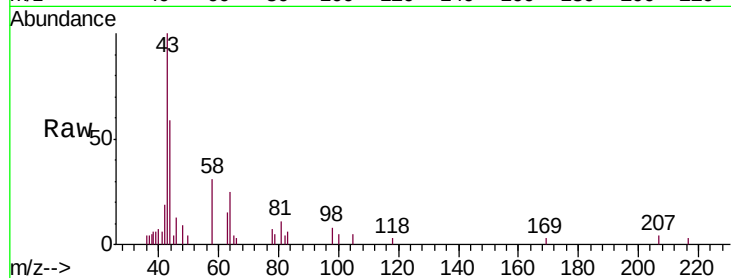

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

