

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042419\
 Data File : VV010464.D
 Acq On : 24 Apr 2019 15:53
 Operator : SY/MD
 Sample : K2478-02
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XC9

Quant Time: Apr 25 09:38:23 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 25 02:19:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	232003	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	232617	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	114723	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	66824	4.94	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.80%
7) Chloroethane-d5	1.58	69	52830	5.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.40%
11) 1,1-Dichloroethene-d2	2.13	63	97950	3.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.80%
20) 2-Butanone-d5	3.96	46	134637	46.95	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.90%
24) Chloroform-d	4.41	84	107067	3.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.40%
26) 1,2-Dichloroethane-d4	5.09	65	71796	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.80%
32) Benzene-d6	5.10	84	268248	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
36) 1,2-Dichloropropane-d6	6.12	67	80084	4.92	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.40%
41) Toluene-d8	7.36	98	257285	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
43) trans-1,3-Dichloropropene-	7.67	79	27847	4.33	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.60%
46) 2-Hexanone-d5	8.14	63	118093	48.16	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.32%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	59441	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	104346	4.92	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.40%


Target Compounds					Ovalue
13) Acetone	2.19	43	16595	9.618 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042419\
Data File : VV010464.D
Acq On : 24 Apr 2019 15:53
Operator : SY/MD
Sample : K2478-02
Misc : 25mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XC9

Quant Time: Apr 25 09:38:23 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 25 02:19:56 2019
Response via : Initial Calibration

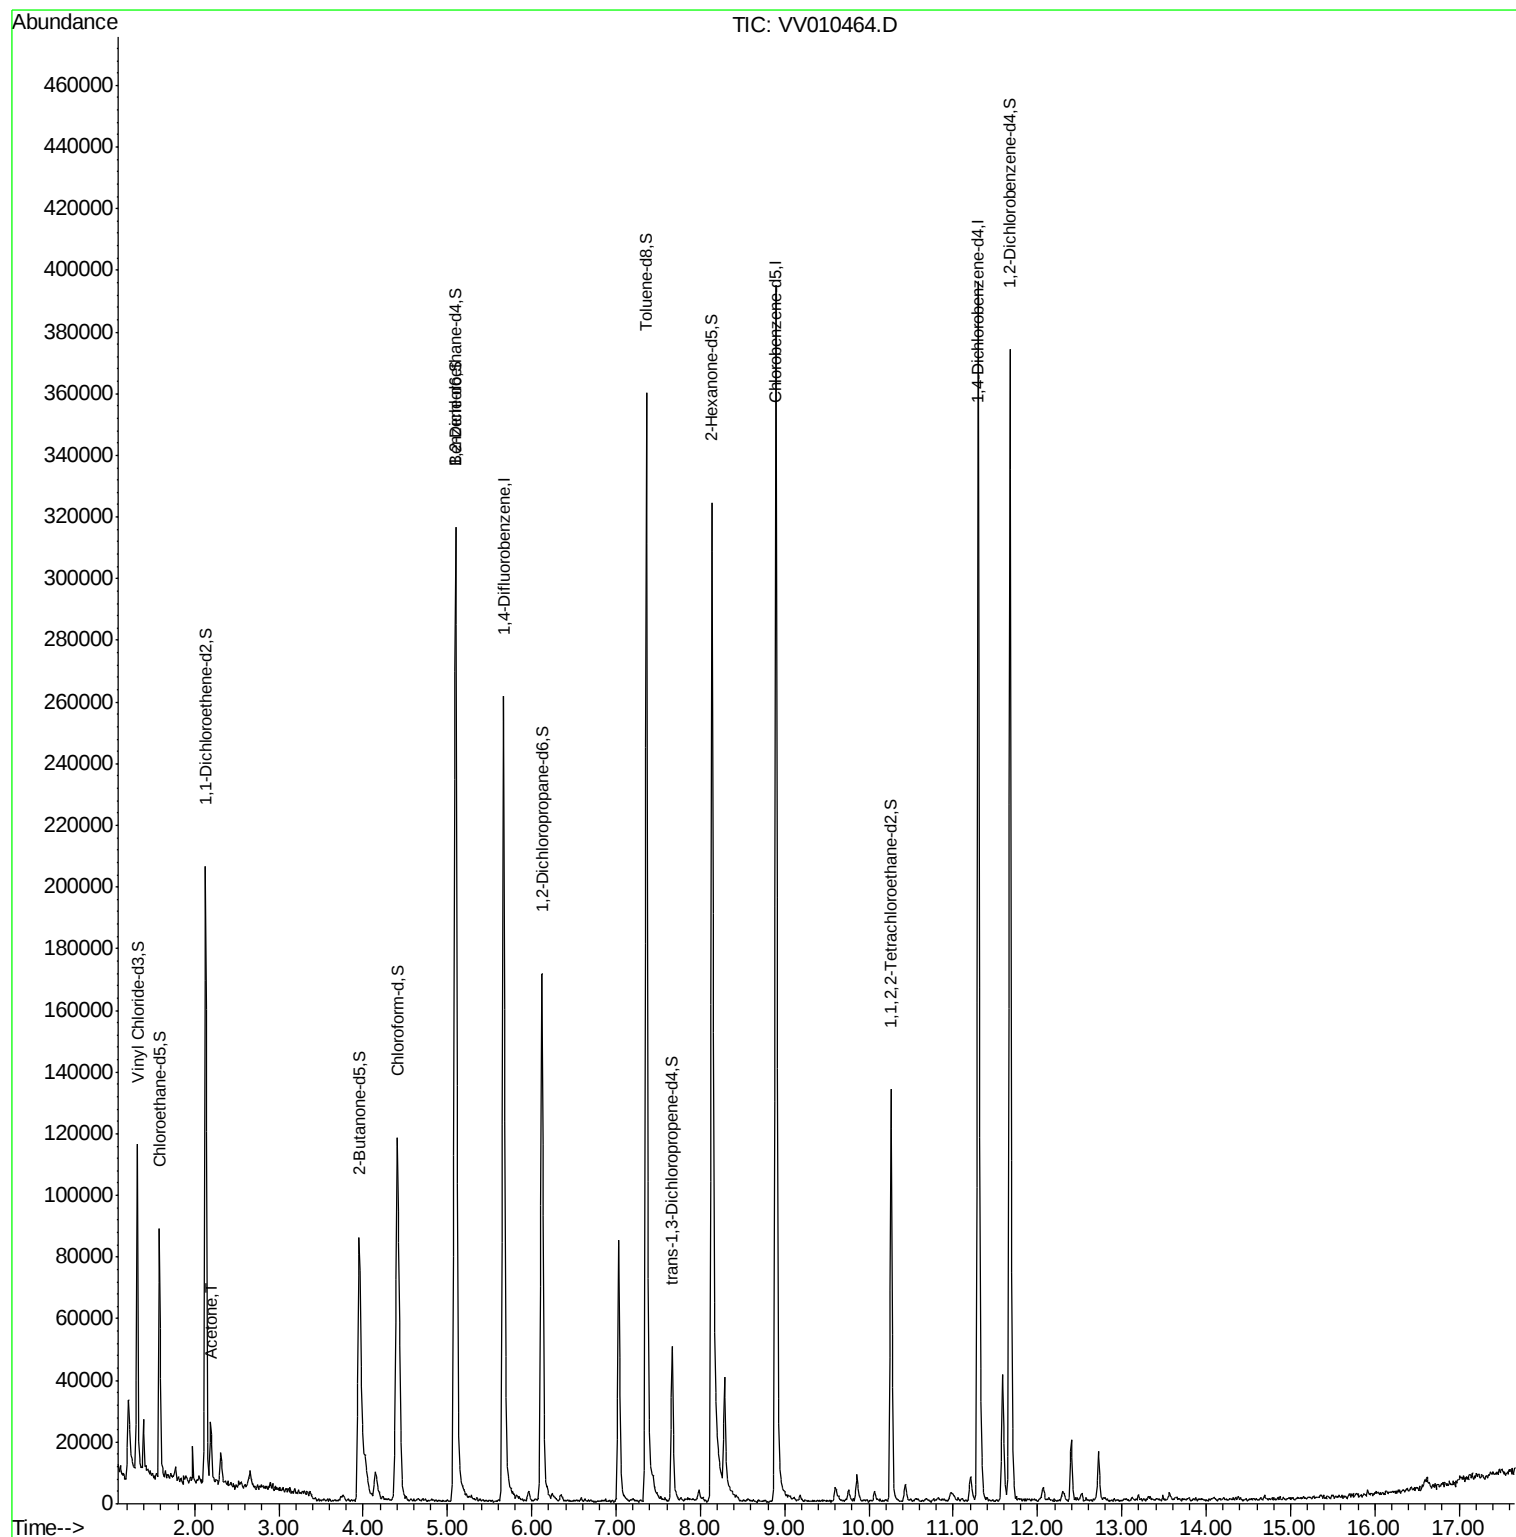

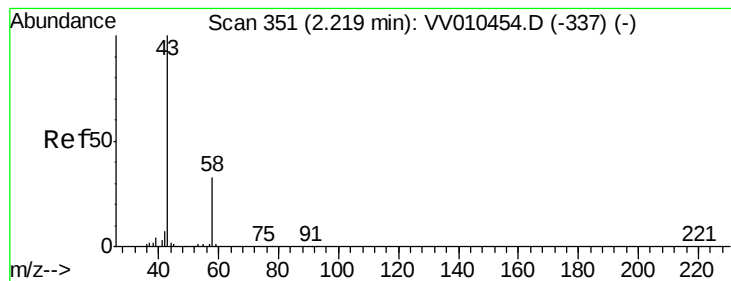

#13

Acetone

Concen: 9.618 ug/L

RT: 2.19 min Scan# 343

Delta R.T. -0.03 min

Lab File: VV010464.D

Acq: 24 Apr 2019 15:53


Instrument :
MSVOA_V
ClientSampleId :
C0XC9

Tot Ion: 43 Resp: 16595

Ion Ratio Lower Upper

43 100

58 32.1 0.0 59.6

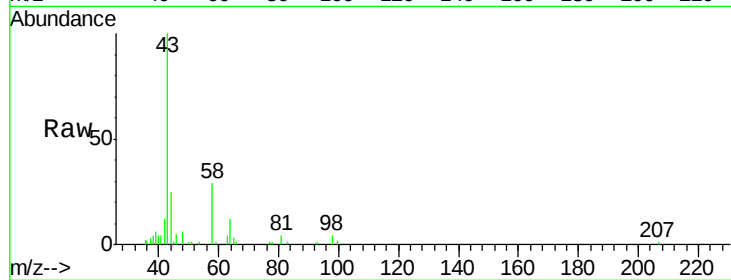

Abundance Ion 43.05 (42.75 to 43.75): VV0
Ion 58.05 (57.75 to 58.75): VV0

