

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042419\
 Data File : VV010465.D
 Acq On : 24 Apr 2019 16:19
 Operator : SY/MD
 Sample : K2478-03
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XD0

Quant Time: Apr 25 09:38:47 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 25 02:19:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	232282	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	235684	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	112891	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	72157	5.33	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.60%
7) Chloroethane-d5	1.58	69	56931	5.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.40%
11) 1,1-Dichloroethene-d2	2.13	63	106460	4.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.20%
20) 2-Butanone-d5	3.95	46	138691	48.31	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.62%
24) Chloroform-d	4.40	84	118085	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.20%
26) 1,2-Dichloroethane-d4	5.09	65	76221	5.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.00%
32) Benzene-d6	5.10	84	288800	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.80%
36) 1,2-Dichloropropane-d6	6.12	67	85956	5.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.20%
41) Toluene-d8	7.36	98	272263	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.00%
43) trans-1,3-Dichloropropene-	7.67	79	29769	4.57	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.40%
46) 2-Hexanone-d5	8.13	63	126663	50.99	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.98%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	60994	4.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	114445	5.48	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.60%


Target Compounds					Ovalue
13) Acetone	2.19	43	19155	11.089 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042419\
Data File : VV010465.D
Acq On : 24 Apr 2019 16:19
Operator : SY/MD
Sample : K2478-03
Misc : 25mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XD0

Quant Time: Apr 25 09:38:47 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 25 02:19:56 2019
Response via : Initial Calibration

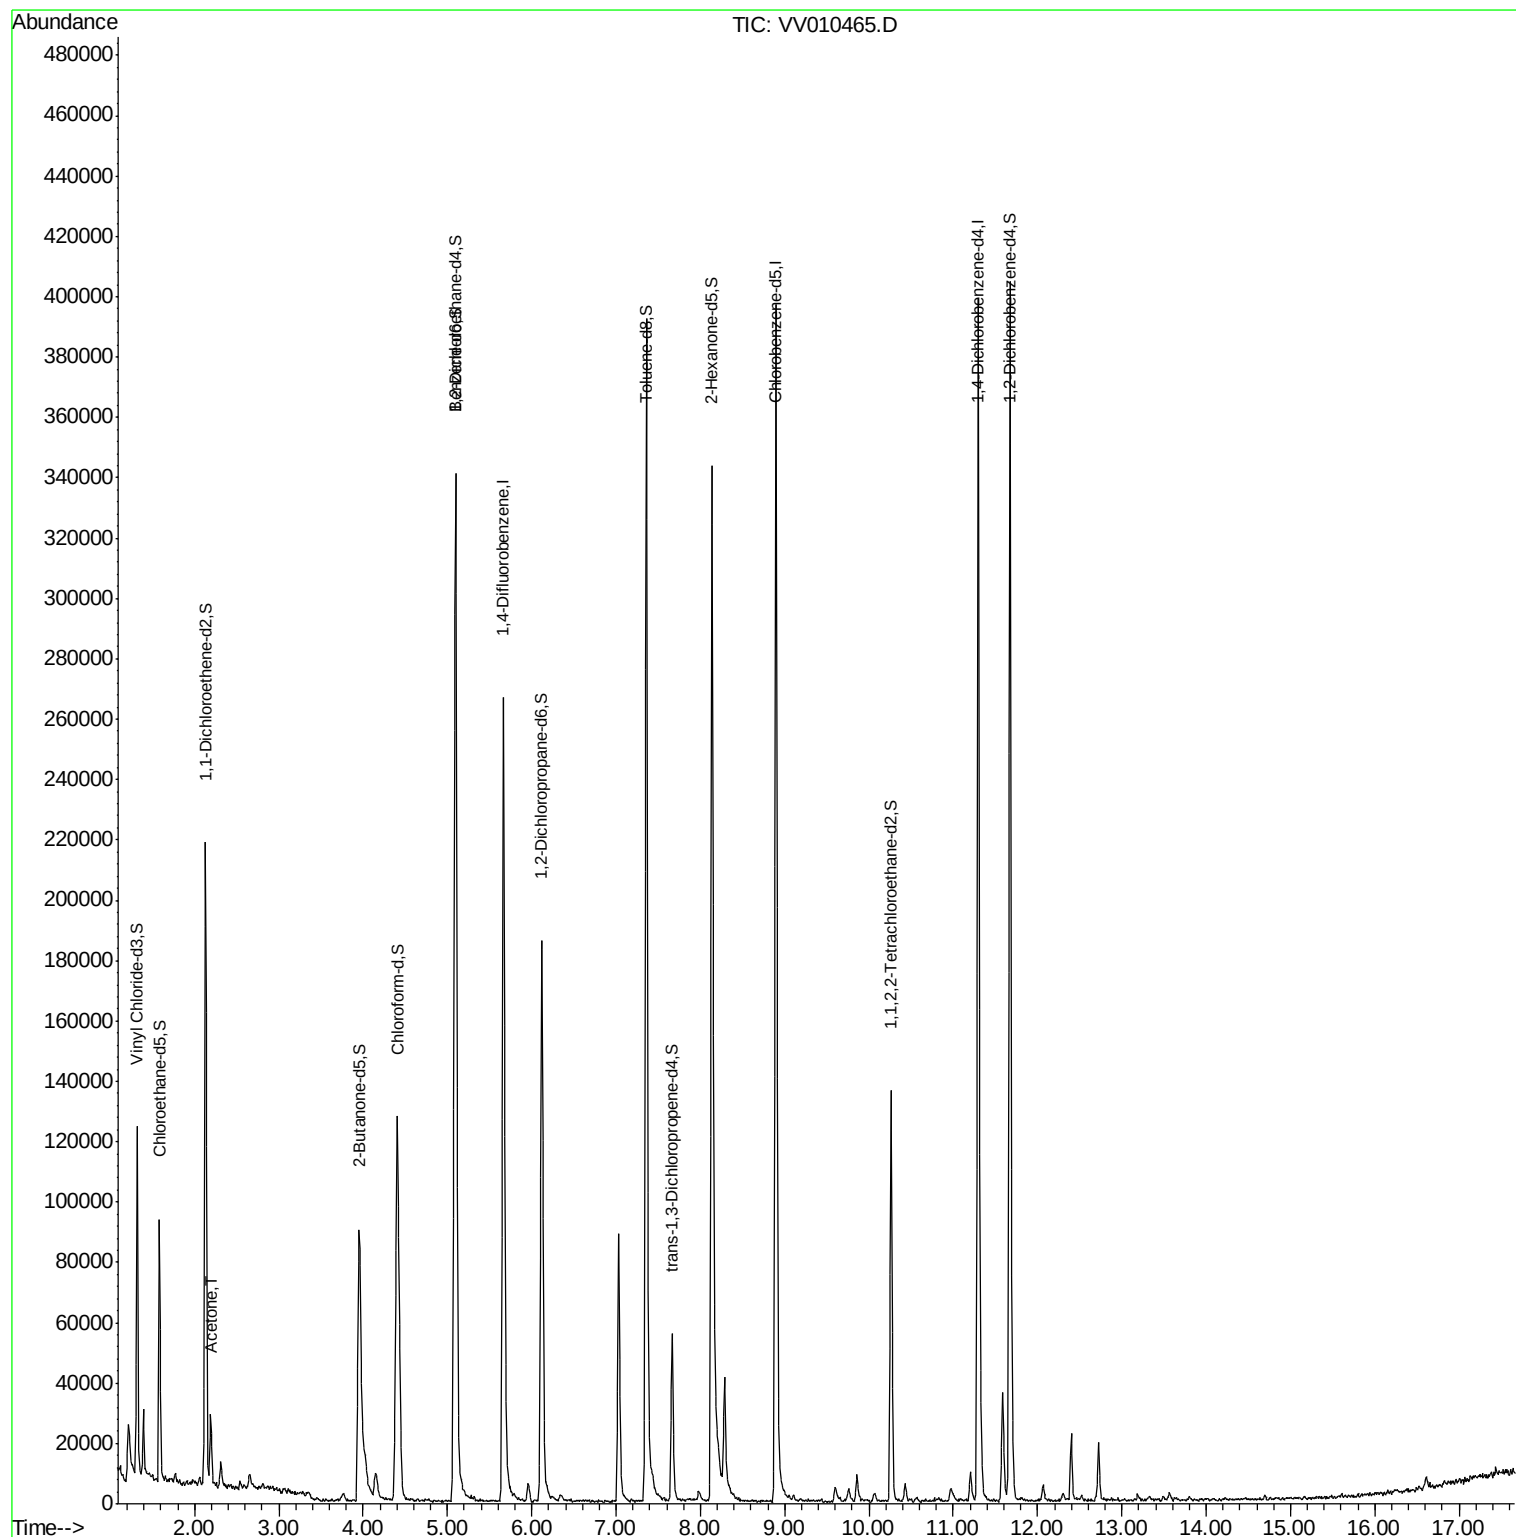

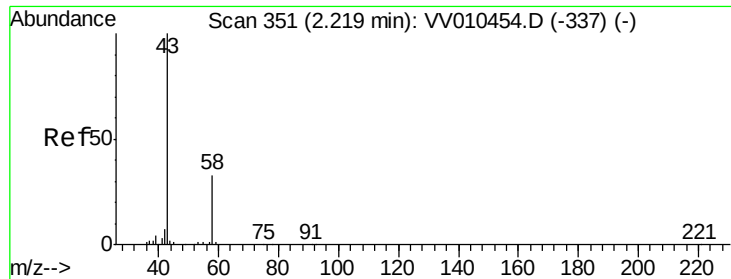

#13

Acetone

Concen: 11.089 ug/L

RT: 2.19 min Scan# 342

Delta R.T. -0.03 min

Lab File: VV010465.D

Acq: 24 Apr 2019 16:19

Instrument :
MSVOA_V
ClientSampleId :
C0XD0

Tot Ion: 43 Resp: 19155

Ion Ratio Lower Upper

43 100

58 32.2 0.0 59.6

