

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042419\
 Data File : VV010466.D
 Acq On : 24 Apr 2019 16:44
 Operator : SY/MD
 Sample : K2478-04
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XD3

Quant Time: Apr 25 09:39:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 25 02:19:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	220569	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	222126	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	109464	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	65837	5.12	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.40%
7) Chloroethane-d5	1.58	69	53106	5.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.40%
11) 1,1-Dichloroethene-d2	2.13	63	97207	3.91	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.20%
20) 2-Butanone-d5	3.95	46	134543	49.35	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.70%
24) Chloroform-d	4.41	84	111133	4.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.40%
26) 1,2-Dichloroethane-d4	5.09	65	69323	5.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.40%
32) Benzene-d6	5.10	84	271773	5.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.60%
36) 1,2-Dichloropropane-d6	6.12	67	80607	5.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.60%
41) Toluene-d8	7.36	98	252369	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.20%
43) trans-1,3-Dichloropropene-	7.67	79	28954	4.72	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.40%
46) 2-Hexanone-d5	8.14	63	119217	50.92	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.84%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	57701	4.99	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	107322	5.30	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.00%


Target Compounds					Ovalue
13) Acetone	2.19	43	20281	12.364 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042419\
Data File : VV010466.D
Acq On : 24 Apr 2019 16:44
Operator : SY/MD
Sample : K2478-04
Misc : 25mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XD3

Quant Time: Apr 25 09:39:10 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 25 02:19:56 2019
Response via : Initial Calibration

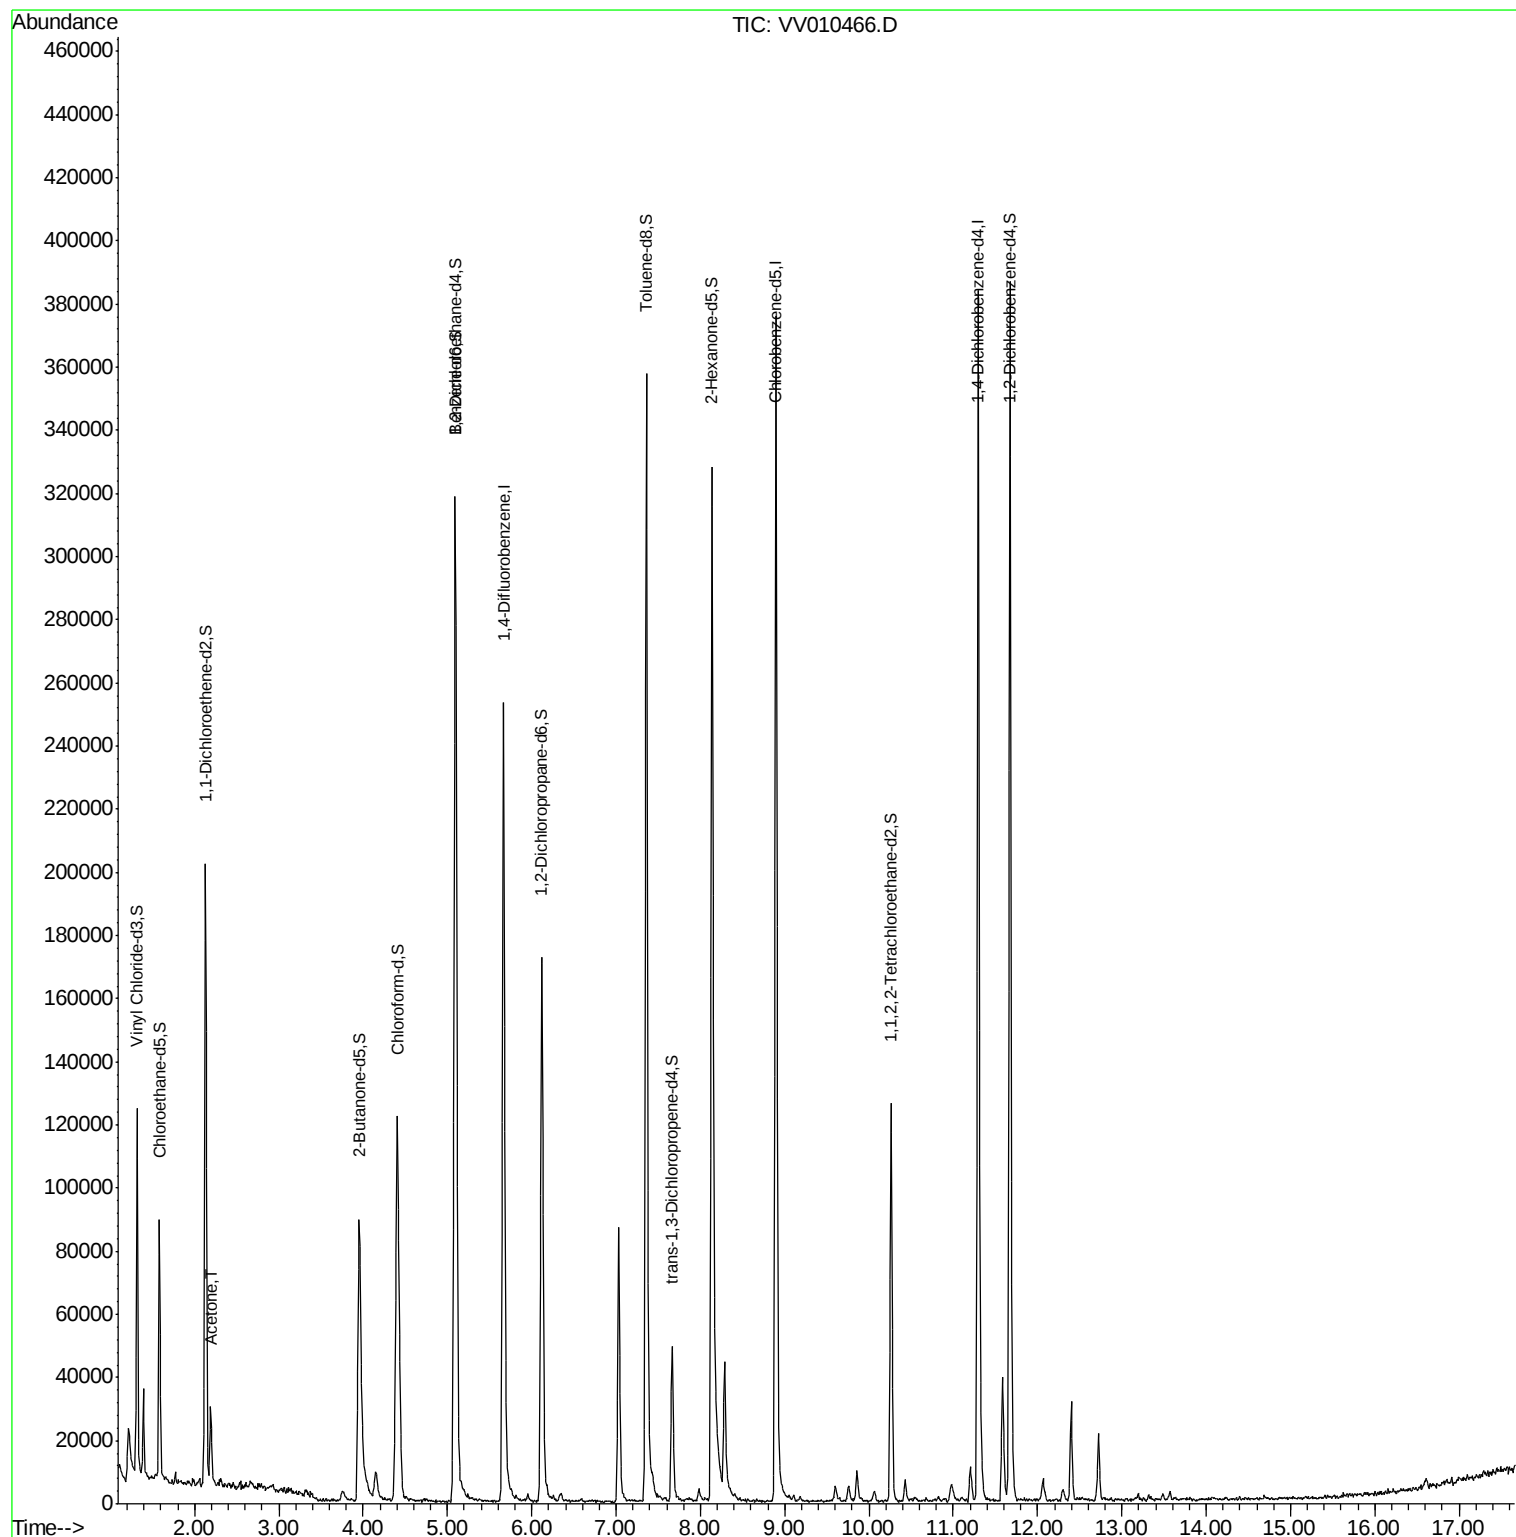

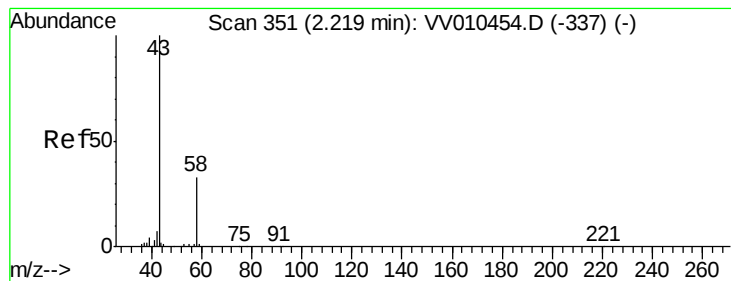

#13

Acetone

Concen: 12.364 ug/L

RT: 2.19 min Scan# 343

Delta R.T. -0.03 min

Lab File: VV010466.D

Acq: 24 Apr 2019 16:44


Instrument :
MSVOA_V
ClientSampleId :
C0XD3

Tot Ion: 43 Resp: 20281

Ion Ratio Lower Upper

43 100

58 33.4 0.0 59.6

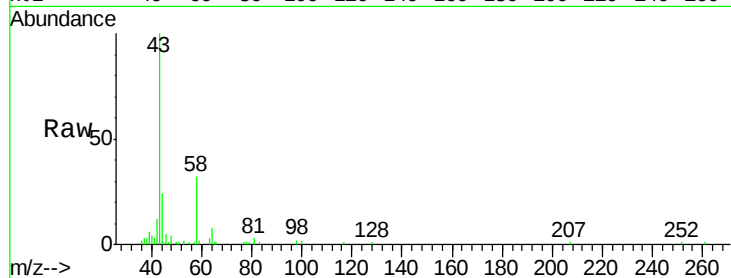

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

