


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042419\
Data File : VV010451.D
Acq On : 24 Apr 2019 09:14
Operator : SY/MD
Sample : BFB36
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB36

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042419WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Apr 25 04:02:34 2019

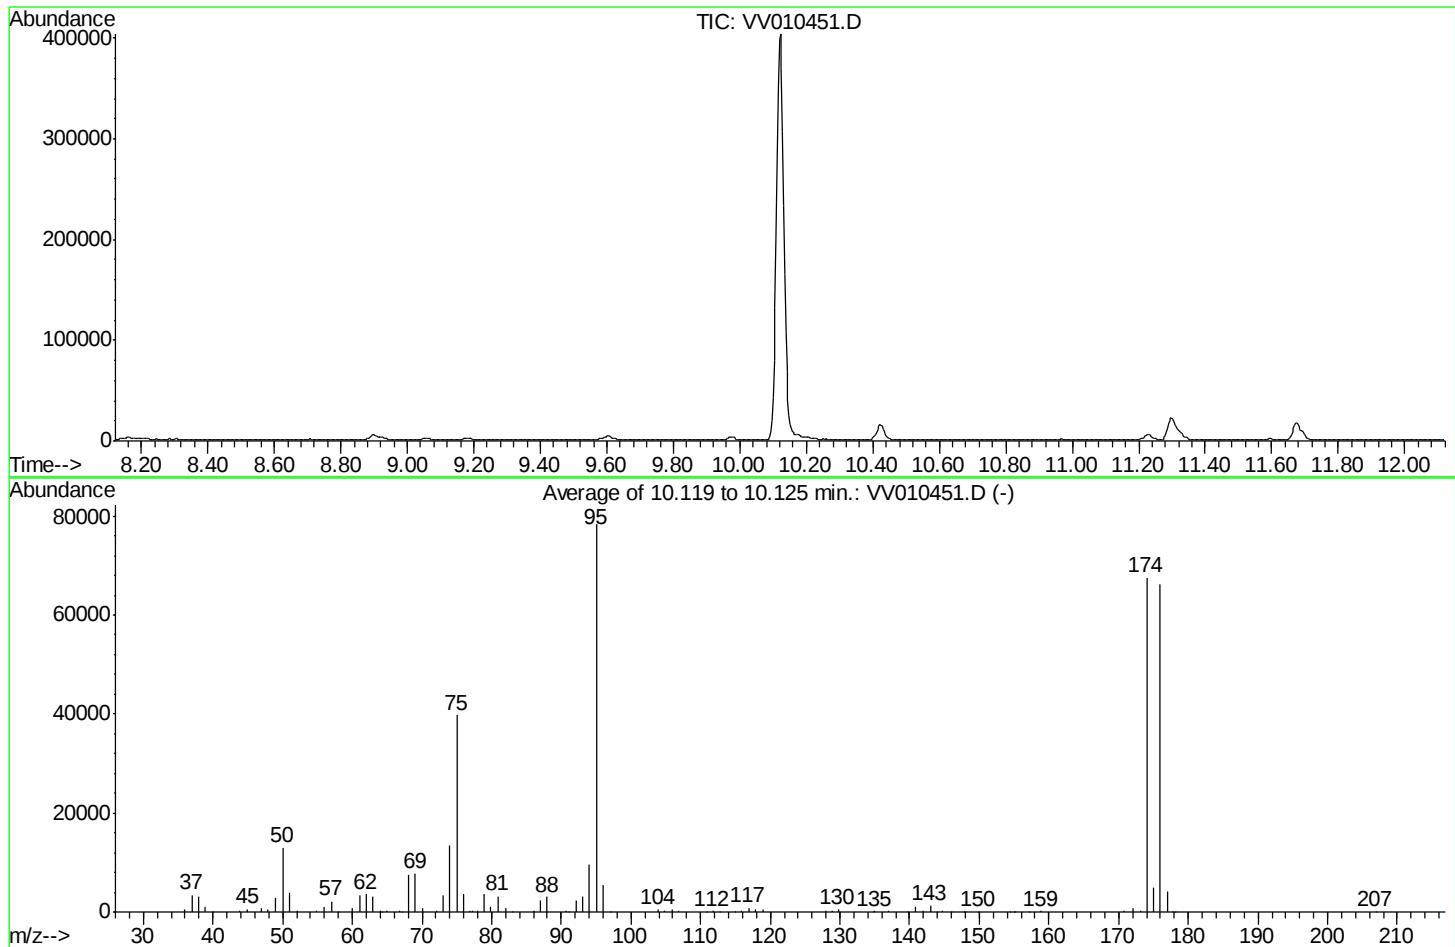

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	13059	PASS
75	95	30	80	50.8	39802	PASS
95	95	100	100	100.0	78317	PASS
96	95	5	9	6.8	5324	PASS
173	174	0.00	2	0.5	340	PASS
174	95	50	120	86.3	67584	PASS
175	174	5	9	7.3	4956	PASS
176	174	95	101	98.0	66210	PASS
177	176	5	9	6.3	4157	PASS

Scan 2794 (10.074 min): VV010451.D
BFB36

m/z	Abundance
39.90	681.0
40.80	159.0
43.90	494.0
45.90	105.0
168.90	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

m/z	Abundance
36.00	662.0
37.00	3657.0
38.00	3686.0
38.90	1195.0
39.90	798.0
43.90	954.0
45.00	601.0
46.90	766.0
48.00	535.0
49.00	3014.0
50.00	13678.0
51.00	3991.0
52.00	214.0
54.80	267.0
56.00	1189.0
57.10	2177.0
58.00	113.0
60.00	961.0
61.00	3778.0
62.00	3909.0
63.00	3263.0
64.00	283.0
65.10	321.0
66.80	132.0
67.20	162.0
68.00	8022.0
69.00	7969.0
70.00	810.0
72.10	399.0
73.00	3479.0
74.00	14264.0
75.00	40920.0
76.10	3925.0
77.00	385.0
77.30	408.0
78.00	220.0
78.90	3696.0
79.80	945.0
80.90	3313.0
81.90	834.0
82.90	111.0
86.00	254.0
86.90	2699.0
88.00	3057.0
90.70	348.0
91.10	340.0
92.00	2154.0
93.10	3472.0
94.00	9377.0
95.00	78704.0
96.10	5796.0
97.10	128.0
103.90	534.0
104.80	205.0
105.80	457.0
106.90	253.0
110.80	140.0
111.80	124.0
112.80	209.0
115.00	131.0
116.00	289.0
116.90	888.0
117.90	332.0
118.80	438.0
127.90	304.0
128.90	247.0
129.70	413.0
134.70	136.0
135.10	152.0
137.10	193.0
139.70	135.0
140.90	1127.0
142.10	104.0
143.00	1117.0
144.70	123.0
146.00	106.0
147.80	192.0
149.90	196.0
154.90	208.0
158.80	119.0
170.80	132.0
172.00	622.0
174.00	67672.0
175.00	4837.0
176.00	66024.0
177.00	4435.0
177.90	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

m/z	Abundance
36.00	614.0
37.00	3563.0
38.00	3313.0
38.90	1069.0
39.90	799.0
44.00	857.0
45.00	573.0
46.90	807.0
47.90	373.0
49.00	2962.0
50.00	13481.0
51.00	4037.0
52.00	161.0
54.80	271.0
55.90	1130.0
57.10	2190.0
58.00	122.0
60.00	844.0
61.00	3420.0
62.00	3644.0
63.00	3276.0
64.00	260.0
65.00	345.0
66.90	156.0
67.10	157.0
68.00	7790.0
69.00	7906.0
70.00	900.0
72.20	414.0
73.00	3482.0
74.00	13966.0
75.00	41192.0
76.10	3726.0
76.90	369.0
77.30	303.0
77.90	308.0
78.90	3672.0
79.80	1077.0
80.90	3230.0
81.90	786.0
82.90	101.0
86.00	346.0
87.00	2496.0
88.00	3166.0
90.70	351.0
92.10	2339.0
93.00	3305.0
94.00	9870.0
95.00	81392.0
96.10	5529.0
103.90	468.0
104.70	178.0
105.90	408.0
106.90	175.0
111.80	150.0
112.80	157.0
115.00	126.0
115.90	287.0
116.90	971.0
118.00	414.0
118.90	451.0
127.90	321.0
128.90	219.0
129.80	455.0
134.70	156.0
135.10	155.0
137.10	124.0
139.70	126.0
140.90	1039.0
141.90	135.0
142.90	1268.0
144.80	157.0
147.80	192.0
149.80	140.0
154.50	101.0
155.10	202.0
158.80	156.0
170.80	190.0
172.10	660.0
174.00	69864.0
175.00	5076.0
176.00	68552.0
177.00	4253.0
177.80	137.0
178.10	118.0
206.90	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

m/z	Abundance
36.00	470.0
37.00	3164.0
38.00	2668.0
38.90	936.0
40.00	779.0
44.00	717.0
44.90	565.0
46.10	107.0
46.90	787.0
47.90	282.0
49.00	2815.0
50.00	12018.0
50.90	3490.0
52.10	147.0
54.80	204.0
55.90	1152.0
57.00	1998.0
60.00	632.0
61.00	2936.0
62.00	3210.0
63.00	2955.0
63.90	238.0
64.20	248.0
64.90	318.0
66.90	216.0
68.00	6813.0
69.00	7096.0
70.00	955.0
72.20	353.0
73.00	3189.0
74.00	12248.0
75.00	37296.0
76.00	3478.0
76.90	319.0
77.90	330.0
78.90	3199.0
79.90	1026.0
80.90	2797.0
82.00	811.0
86.00	269.0
87.10	2073.0
88.00	3016.0
90.80	353.0
92.10	2323.0
92.90	2951.0
94.00	9280.0
95.00	74856.0
96.00	4648.0
104.00	339.0
104.80	106.0
106.00	417.0
106.90	114.0
111.80	149.0
115.00	119.0
115.80	273.0
116.90	847.0
118.00	510.0
119.00	400.0
127.90	301.0
129.00	193.0
129.90	363.0
134.90	210.0
137.00	112.0
140.90	890.0
141.80	200.0
142.90	1246.0
143.90	110.0
144.80	200.0
148.00	204.0
155.10	175.0
157.10	122.0
158.90	145.0
170.80	167.0
172.10	726.0
173.10	1021.0
174.00	65216.0
175.00	4956.0
176.00	64056.0
177.00	3785.0
206.90	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36